




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036335.D
Acq On : 06 Feb 2025 14:45
Operator : RC/JU
Sample : PB166464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK464

Manual IntegrationsAPPROVED

Quant Time: Feb 06 15:22:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 14:44:03 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025

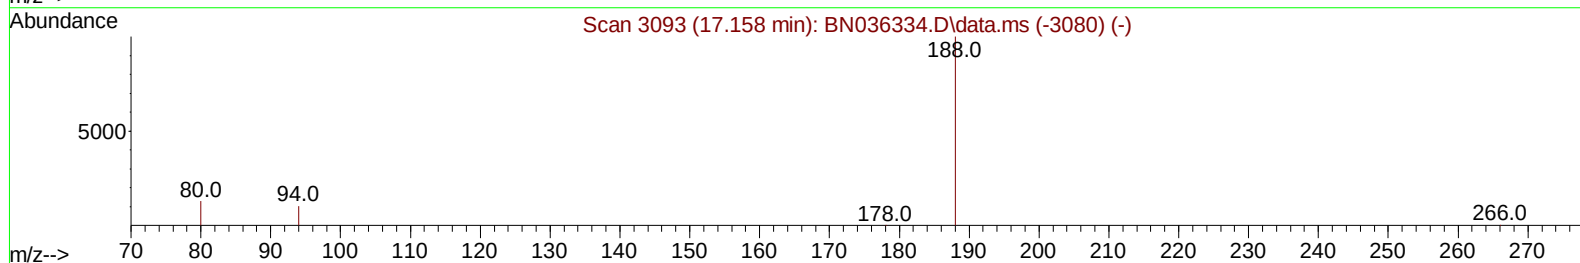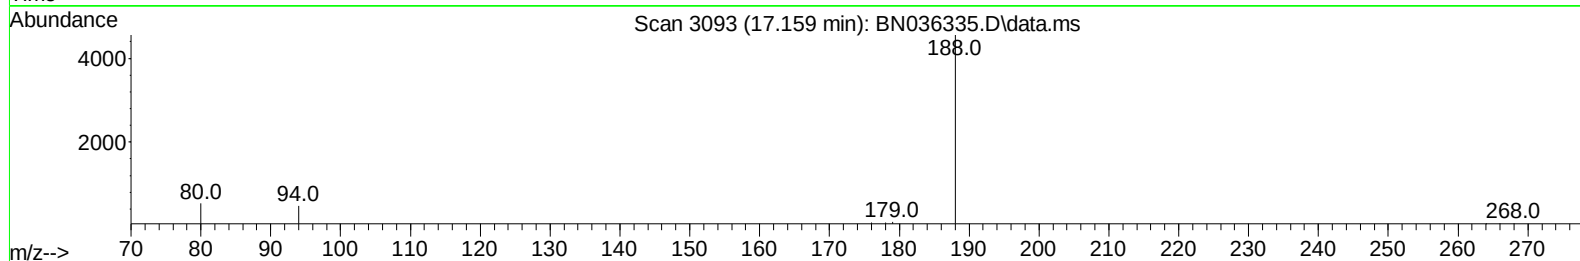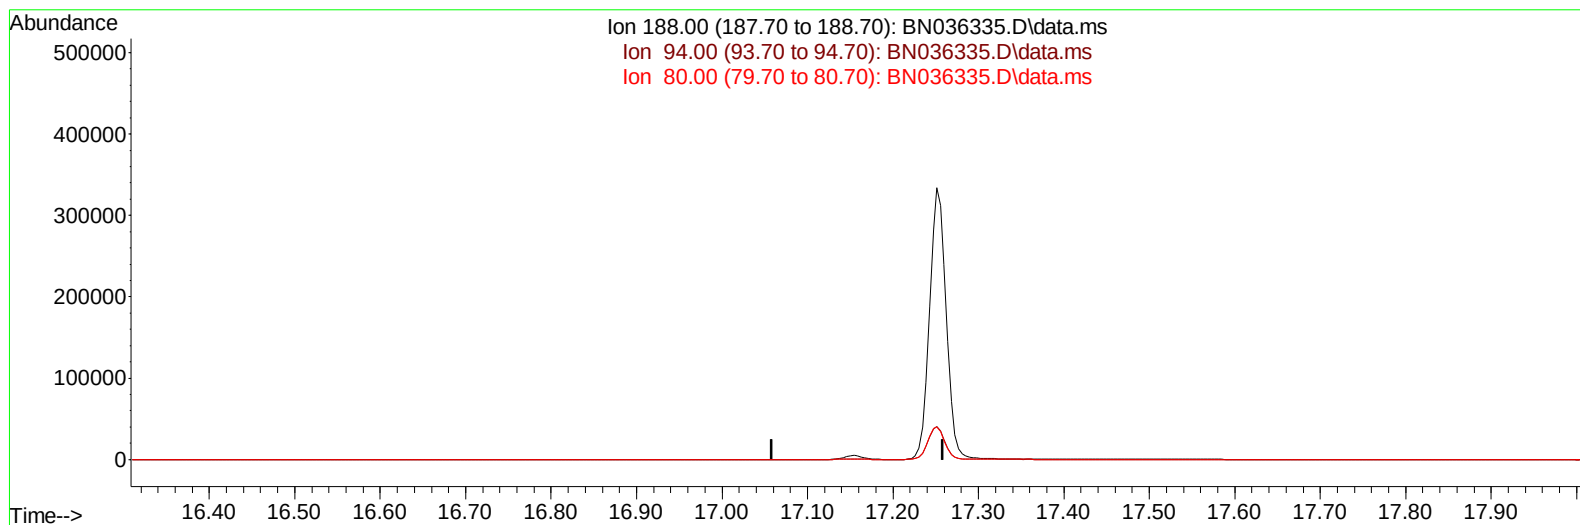

TIC: BN036335.D\data.ms

(13) Phenanthrene-d10 (I)

17.158min (-17.158) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	10.10	0.00#
80.00	10.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036335.D
Acq On : 06 Feb 2025 14:45
Operator : RC/JU
Sample : PB166464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK464

Manual IntegrationsAPPROVED

Quant Time: Feb 06 15:22:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 14:44:03 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025

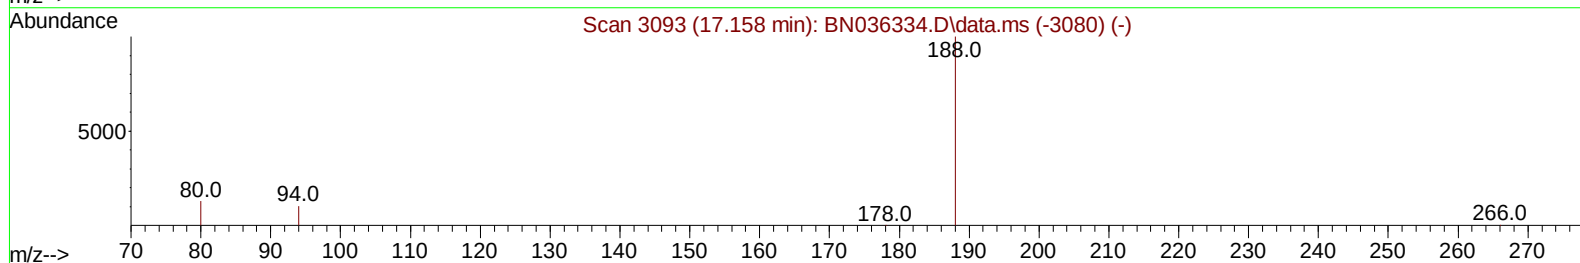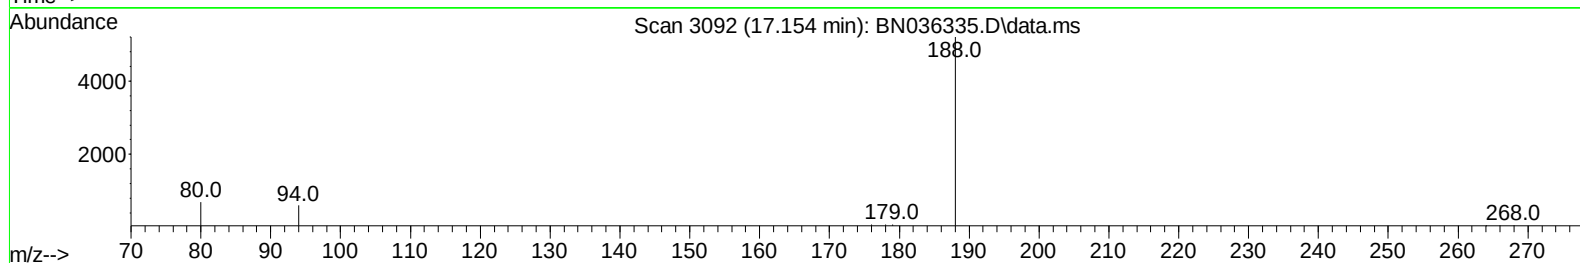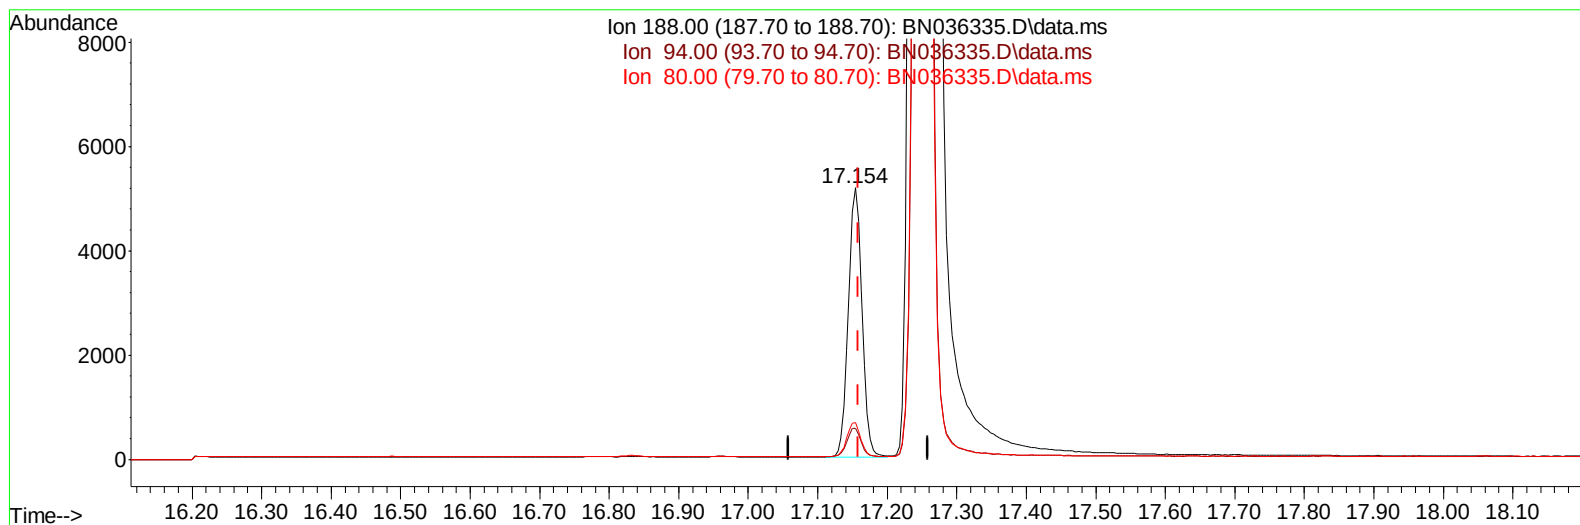

TIC: BN036335.D\data.ms

(13) Phenanthrene-d10 (I)

17.154min (-0.004) 0.40 ng/ul m

response 7047

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	11.49
80.00	10.90	13.47#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036335.D
Acq On : 06 Feb 2025 14:45
Operator : RC/JU
Sample : PB166464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK464

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 06 15:22:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 14:44:03 2025
Response via : Initial Calibration

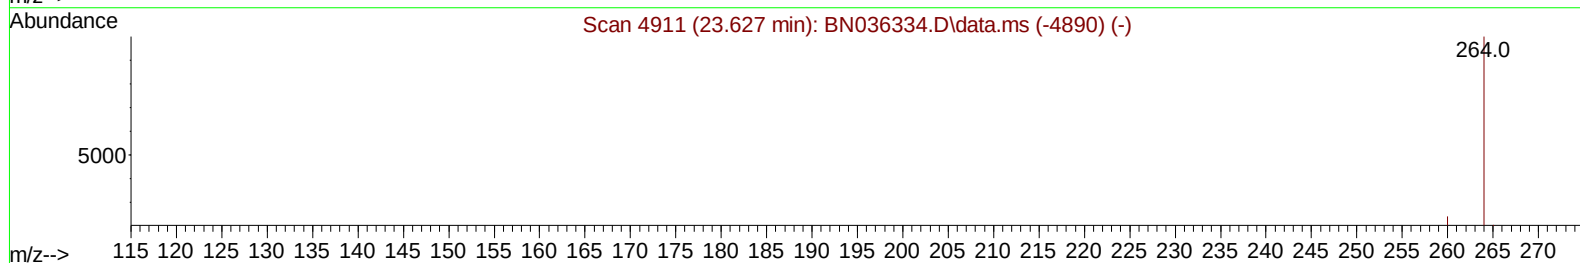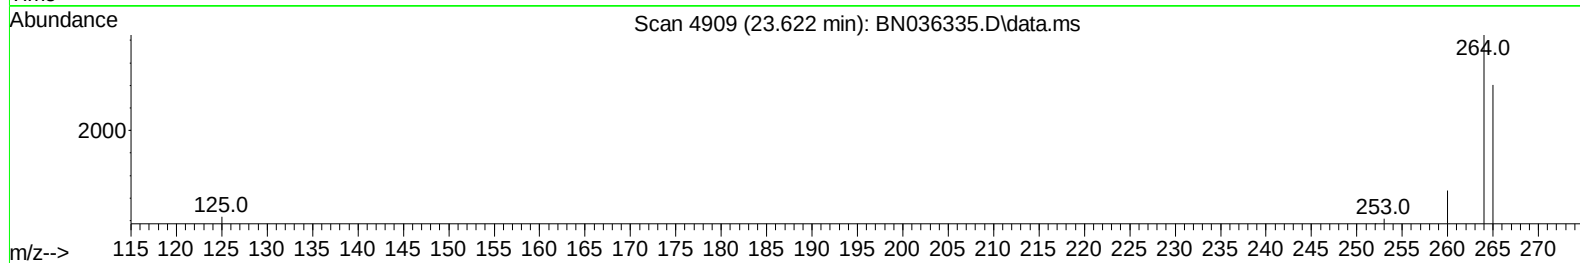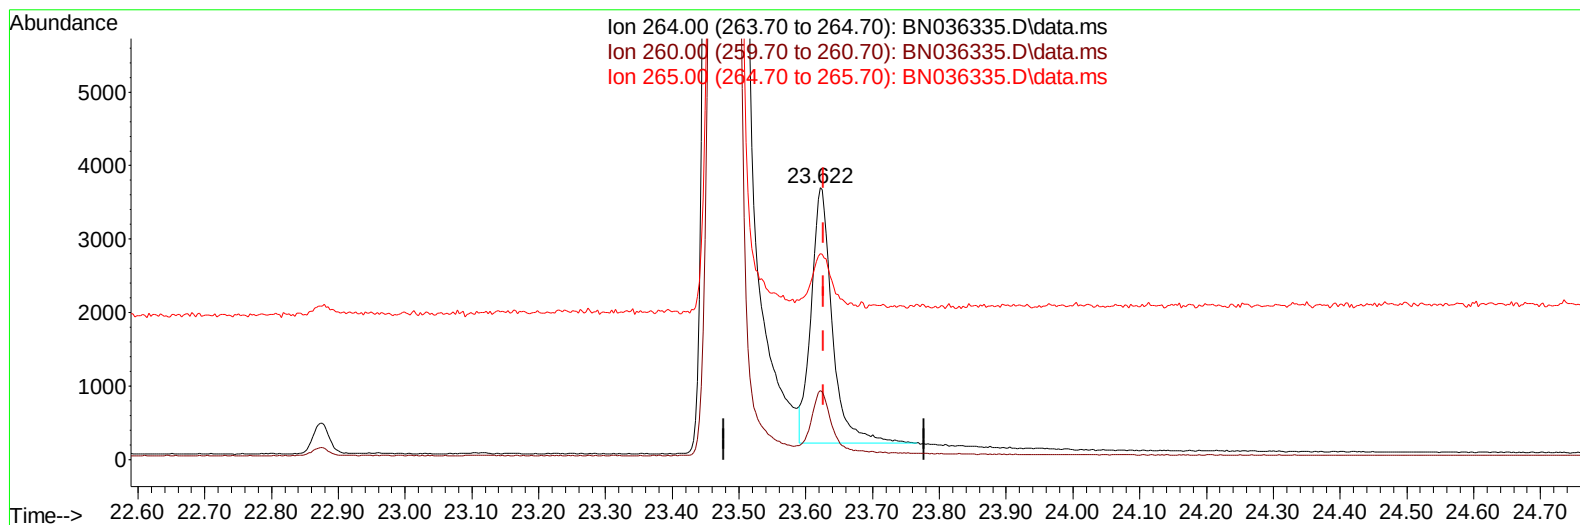

TIC: BN036335.D\data.ms

(23) Perylene-d12 (I)

23.622min (-0.006) 0.40 ng/u1

response 7748

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.32
265.00	53.20	75.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036335.D
Acq On : 06 Feb 2025 14:45
Operator : RC/JU
Sample : PB166464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK464

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 06 15:22:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 14:44:03 2025
Response via : Initial Calibration

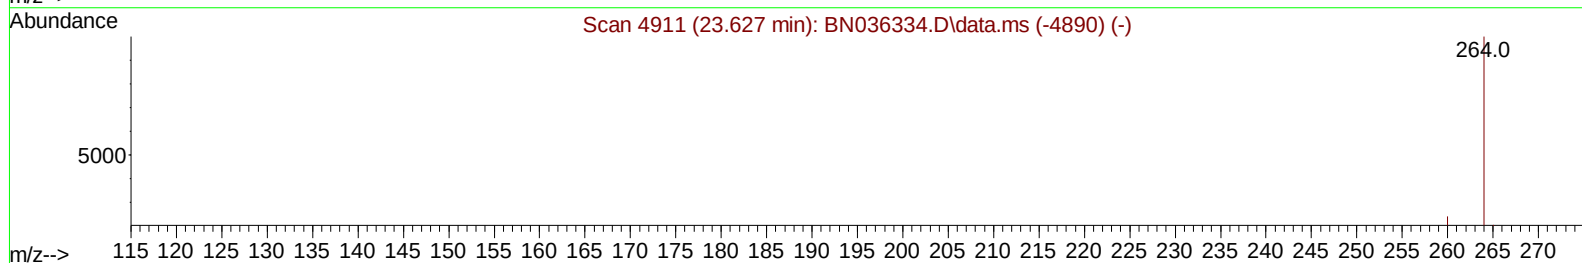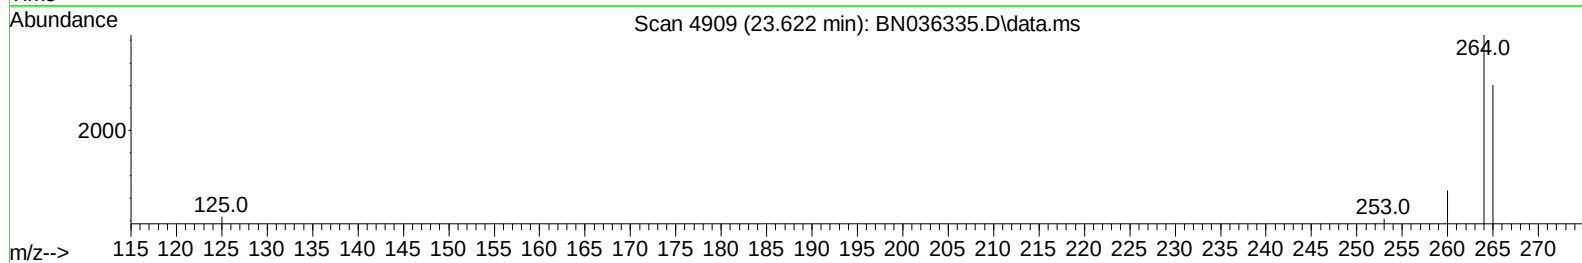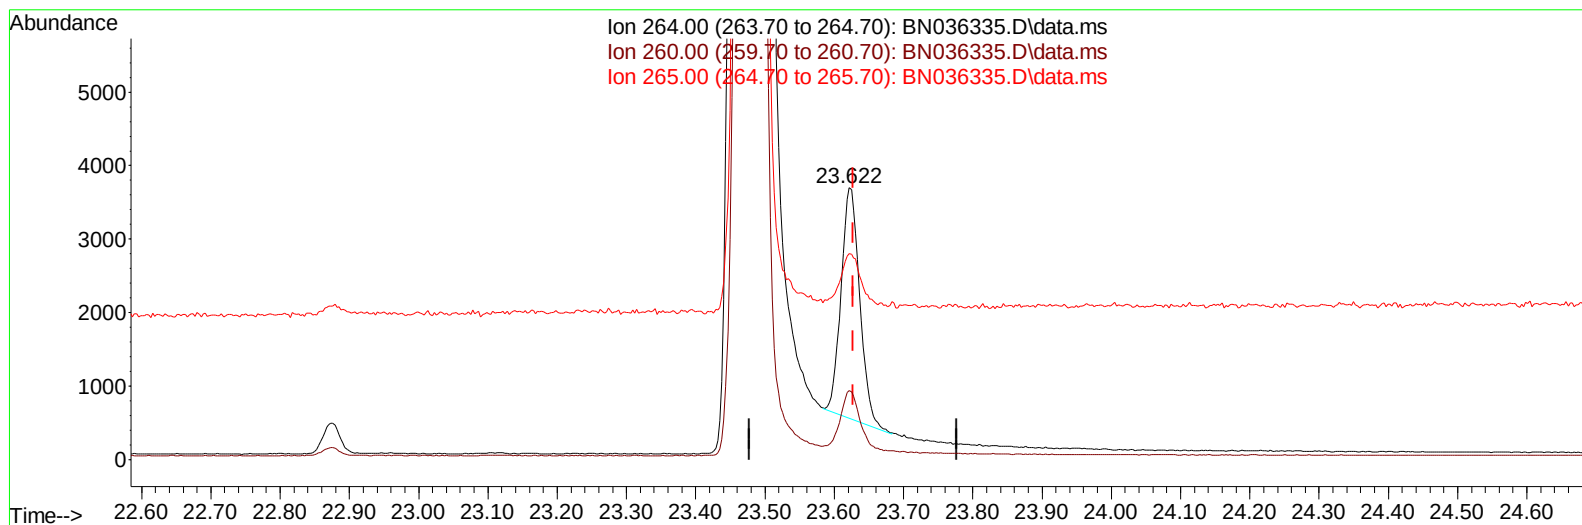

TIC: BN036335.D\data.ms

(23) Perylene-d12 (I)

23.622min (-0.006) 0.40 ng/ul m

response 5890

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.32
265.00	53.20	75.89#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
 Data File : BN036335.D
 Acq On : 06 Feb 2025 14:45
 Operator : RC/JU
 Sample : PB166464BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK464

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
 Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 06 15:22:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 06 14:44:03 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.771	152	2594	0.400	ng/ul	0.00
4) Naphthalene-d8	10.557	136	6192	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.409	164	3498	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.154	188	7047m	0.400	ng/ul	0.00
17) Chrysene-d12	21.348	240	5953	0.400	ng/ul	# 0.00
23) Perylene-d12	23.622	264	5890m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	15255	5.371	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.163	152	2203	0.282	ng/ul	0.00
18) Fluoranthene-d10	19.184	212	4877	0.298	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036335.D
Acq On : 06 Feb 2025 14:45
Operator : RC/JU
Sample : PB166464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK464

Manual IntegrationsAPPROVED

Quant Time: Feb 06 15:22:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 14:44:03 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025

