




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036342.D
Acq On : 06 Feb 2025 19:10
Operator : RC/JU
Sample : Q1247-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6337

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 07 07:35:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 14:44:03 2025
Response via : Initial Calibration

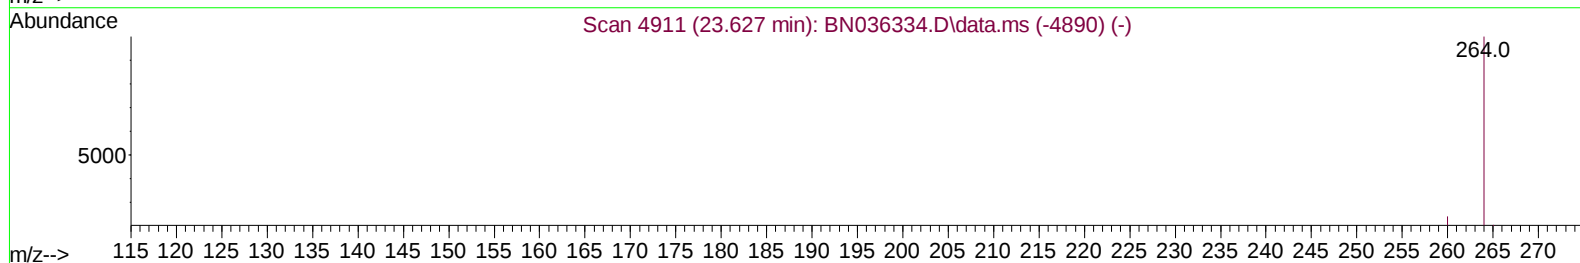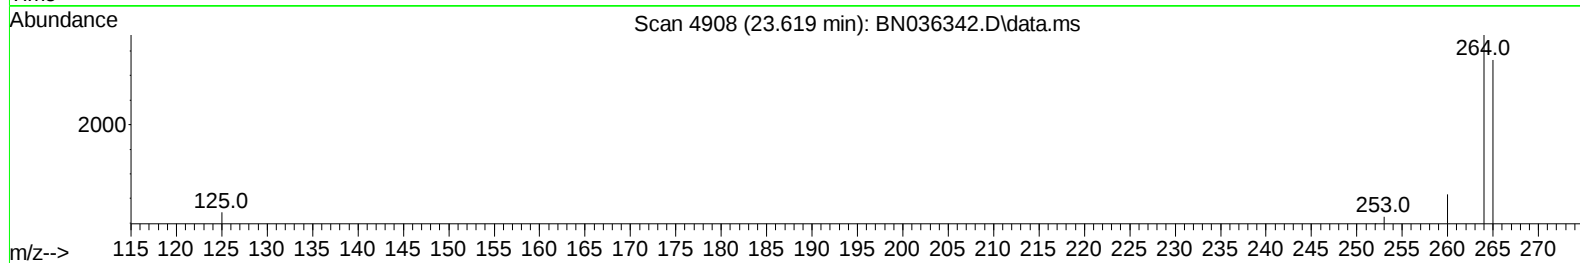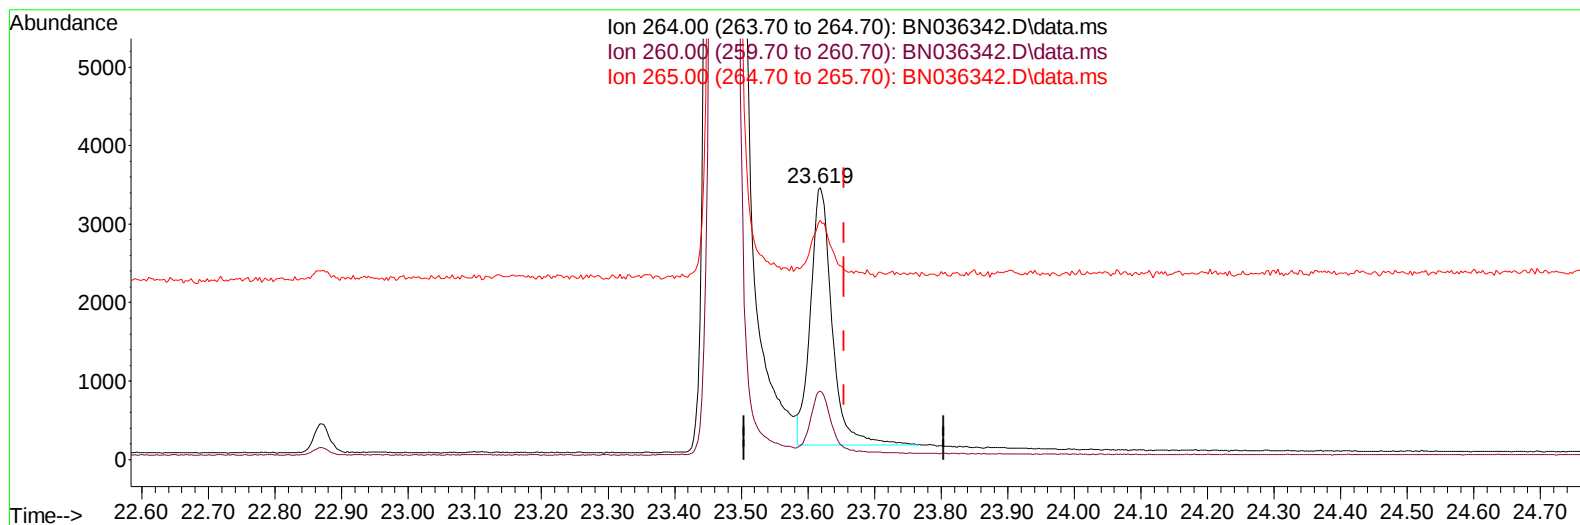

TIC: BN036342.D\data.ms

(23) Perylene-d12 (I)

23.619min (-0.036) 0.40 ng/u1

response 7390

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.14
265.00	53.20	88.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036342.D
Acq On : 06 Feb 2025 19:10
Operator : RC/JU
Sample : Q1247-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6337

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 07 07:35:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 14:44:03 2025
Response via : Initial Calibration

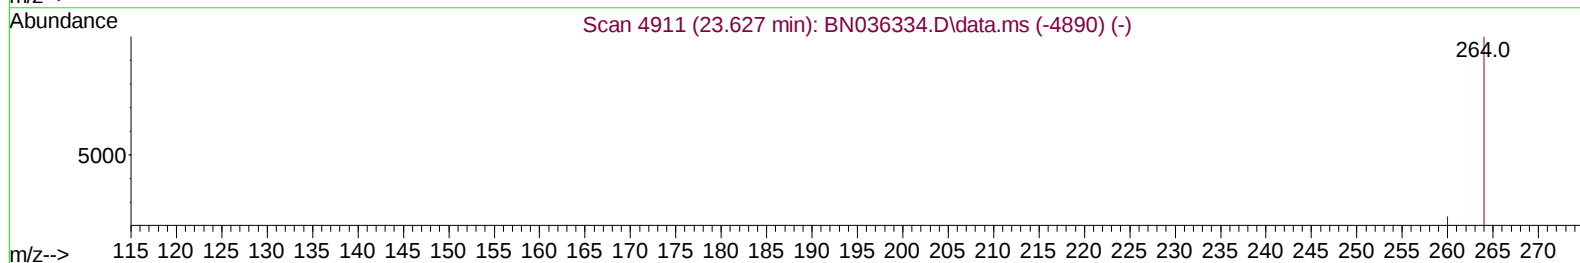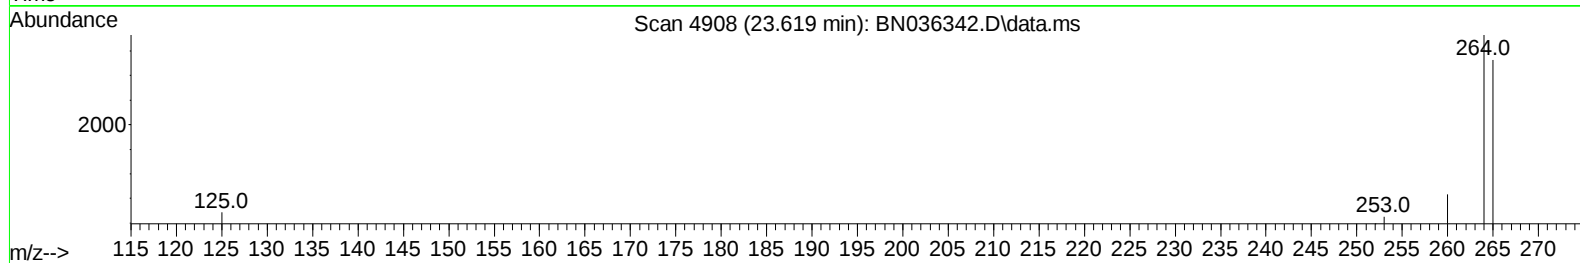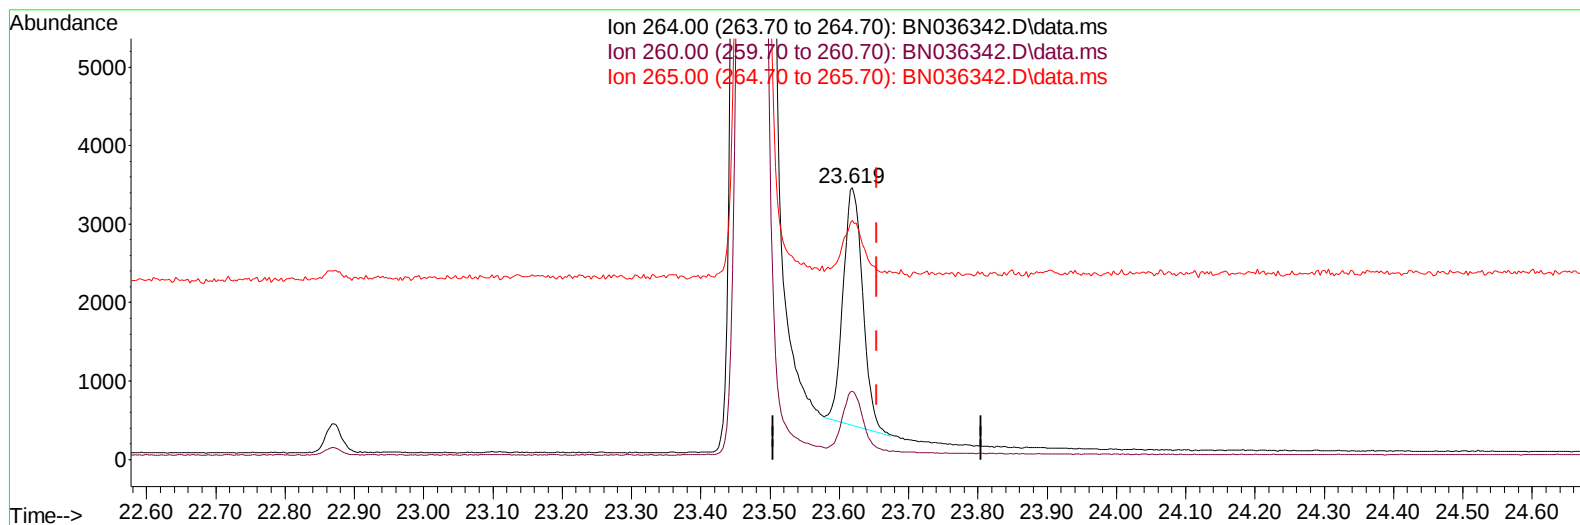

TIC: BN036342.D\data.ms

(23) Perylene-d12 (I)

23.619min (-0.036) 0.40 ng/ul m

response 5951

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.14
265.00	53.20	88.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
 Data File : BN036342.D
 Acq On : 06 Feb 2025 19:10
 Operator : RC/JU
 Sample : Q1247-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A6337

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
 Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 07 07:35:03 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 06 14:44:03 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.771	152	2642	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.557	136	6199	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.409	164	3458	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.154	188	6828	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.342	240	5979	0.400	ng/ul	#-0.02
23) Perylene-d12	23.619	264	5951m	0.400	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	16303	5.636	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.152	152	1576	0.201	ng/ul	-0.02
18) Fluoranthene-d10	19.184	212	3952	0.241	ng/ul	-0.02

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036342.D
Acq On : 06 Feb 2025 19:10
Operator : RC/JU
Sample : Q1247-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6337

Manual IntegrationsAPPROVED

Quant Time: Feb 07 07:35:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 14:44:03 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025

