




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036370.D
Acq On : 07 Feb 2025 12:35
Operator : RC/JU
Sample : Q1229-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2991

Manual IntegrationsAPPROVED

Quant Time: Feb 10 11:19:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/10/2025
Supervised By :Sohil Jodhani 02/18/2025

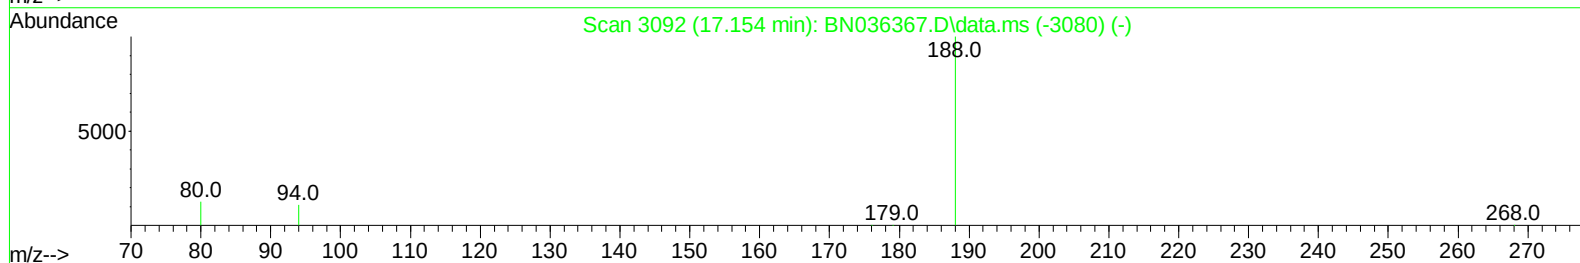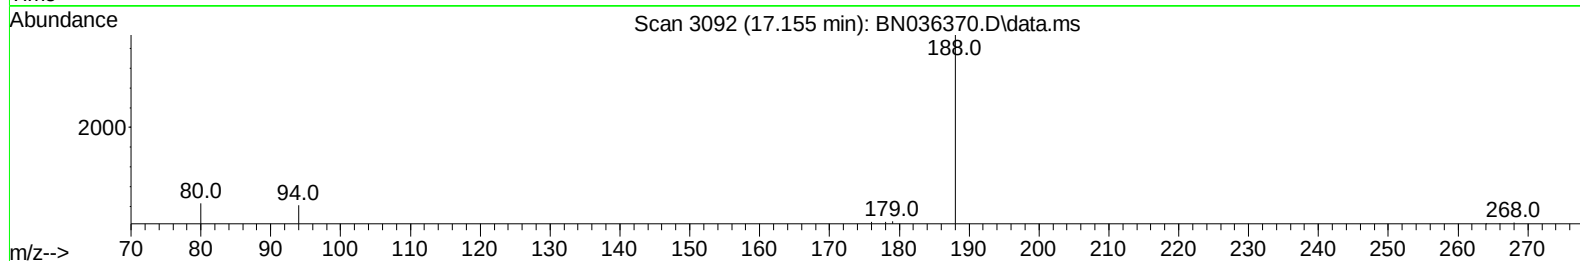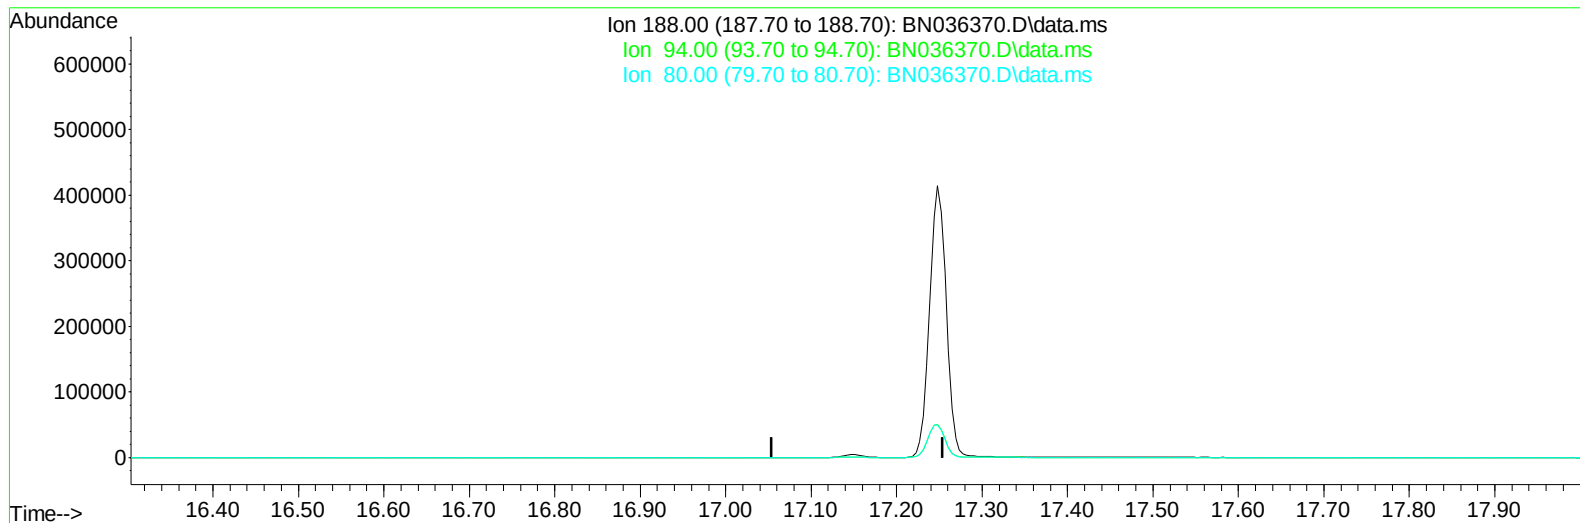

TIC: BN036370.D\data.ms

(13) Phenanthrene-d10 (I)

17.154min (-17.154) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	10.10	0.00#
80.00	10.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036370.D
Acq On : 07 Feb 2025 12:35
Operator : RC/JU
Sample : Q1229-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2991

Manual IntegrationsAPPROVED

Quant Time: Feb 10 11:19:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/10/2025
Supervised By :Sohil Jodhani 02/18/2025

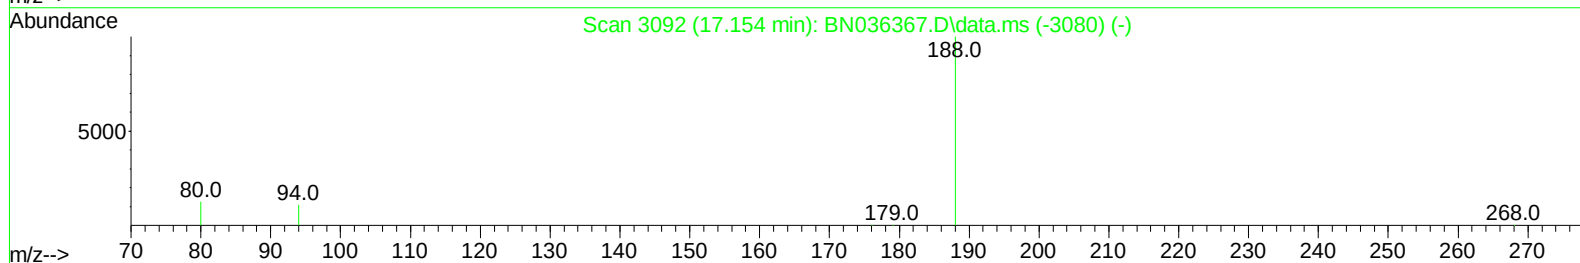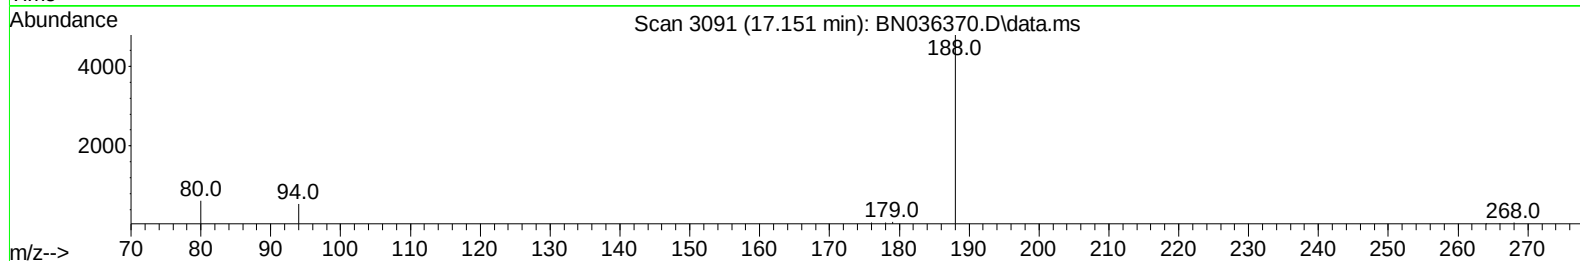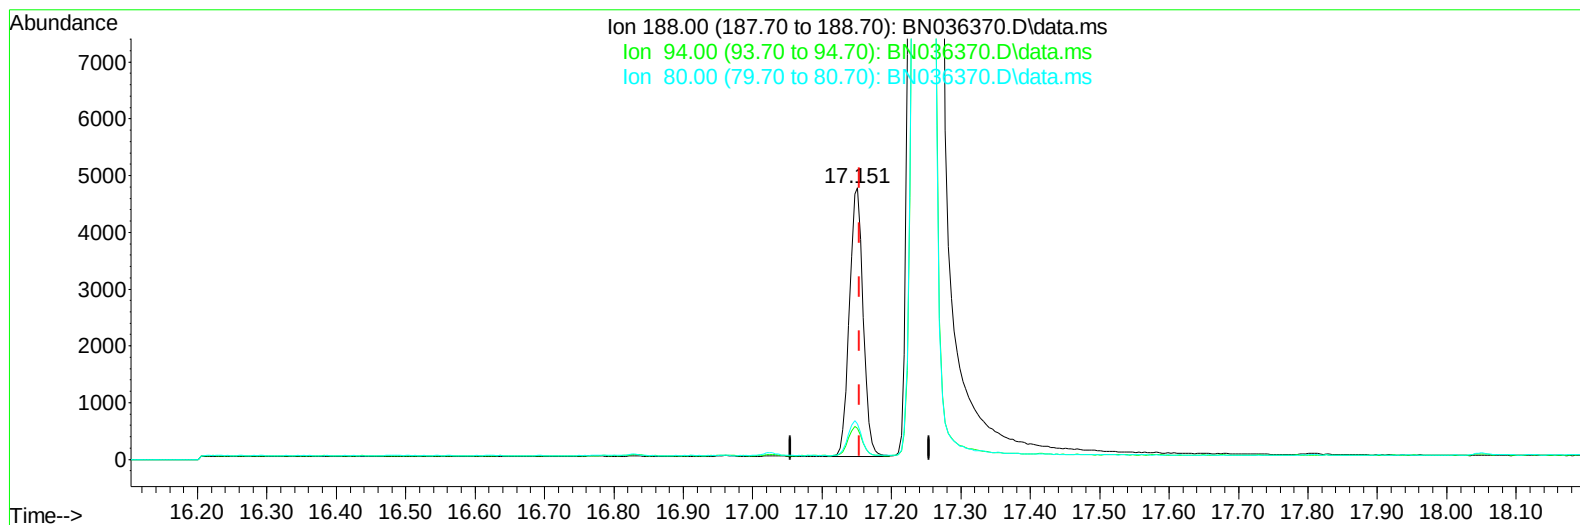

TIC: BN036370.D\data.ms

(13) Phenanthrene-d10 (I)

17.151min (-0.003) 0.40 ng/ul m

response 6527

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	11.52
80.00	10.90	13.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036370.D
Acq On : 07 Feb 2025 12:35
Operator : RC/JU
Sample : Q1229-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2991

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/10/2025
Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 10 11:19:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

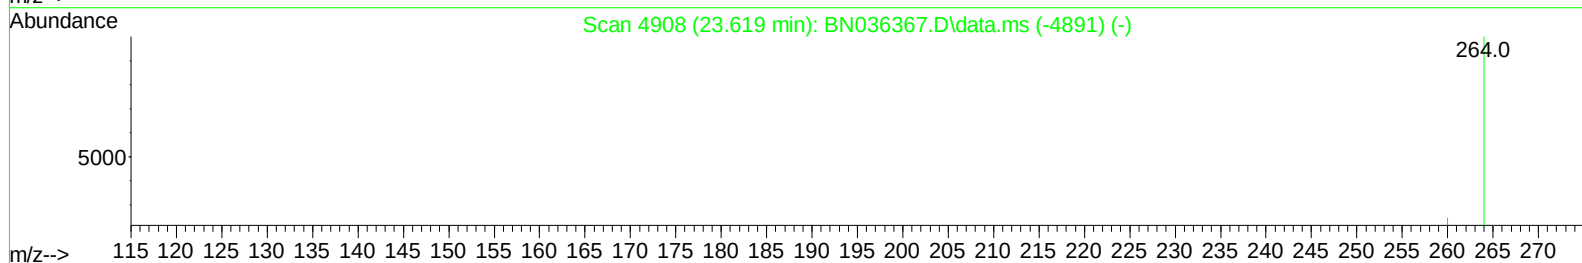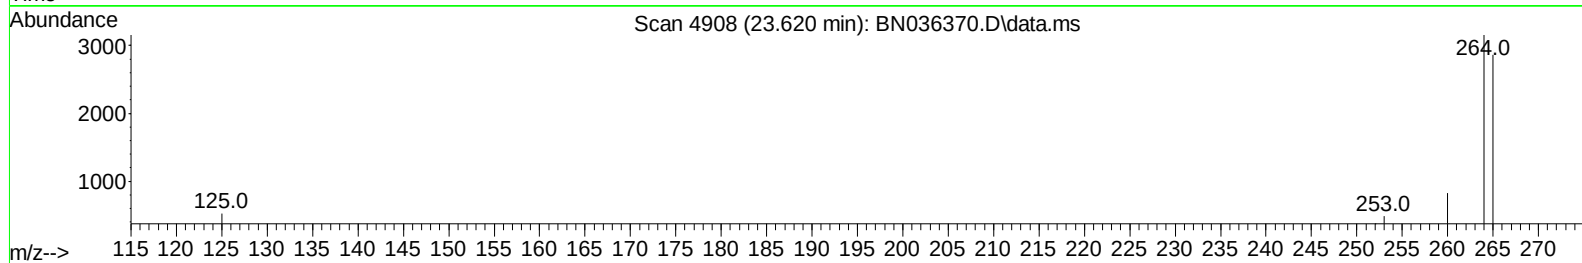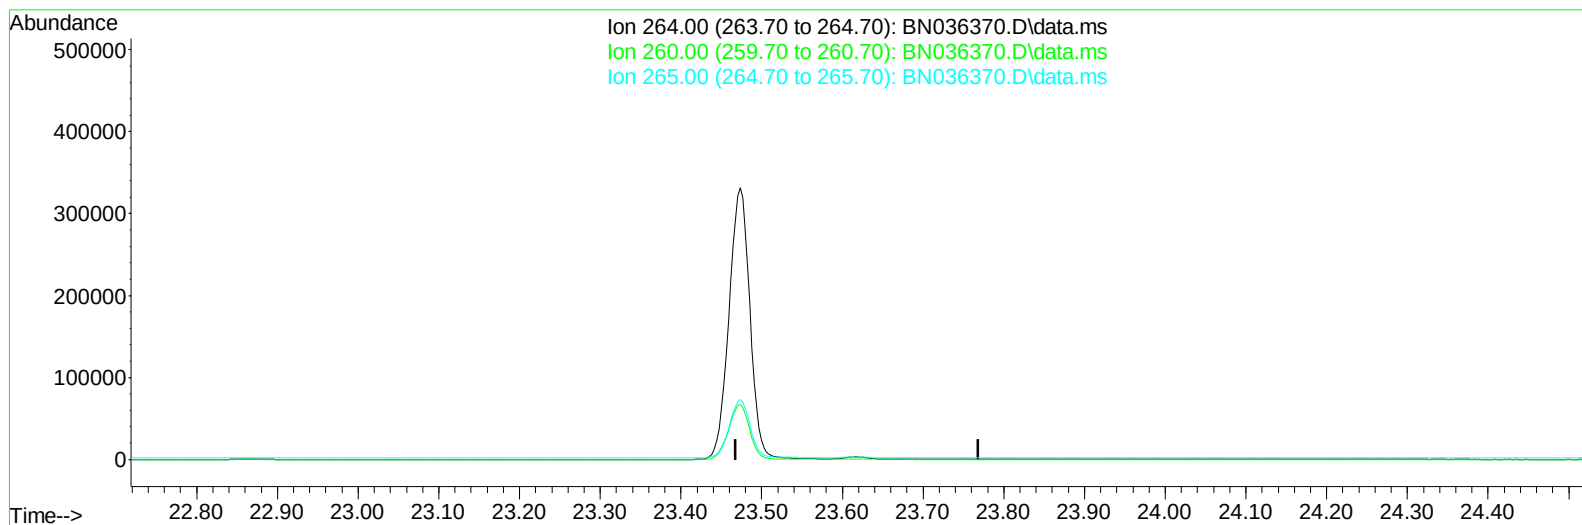

TIC: BN036370.D\data.ms

(23) Perylene-d12 (I)

23.619min (-23.619) 0.00 ng/u1

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	26.80	0.00#
265.00	53.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036370.D
Acq On : 07 Feb 2025 12:35
Operator : RC/JU
Sample : Q1229-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2991

Manual IntegrationsAPPROVED

Quant Time: Feb 10 11:19:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/10/2025
Supervised By :Sohil Jodhani 02/18/2025

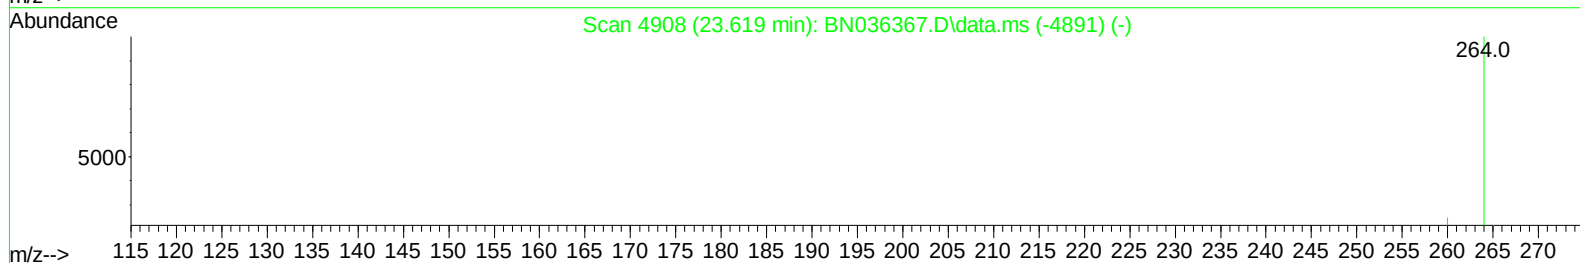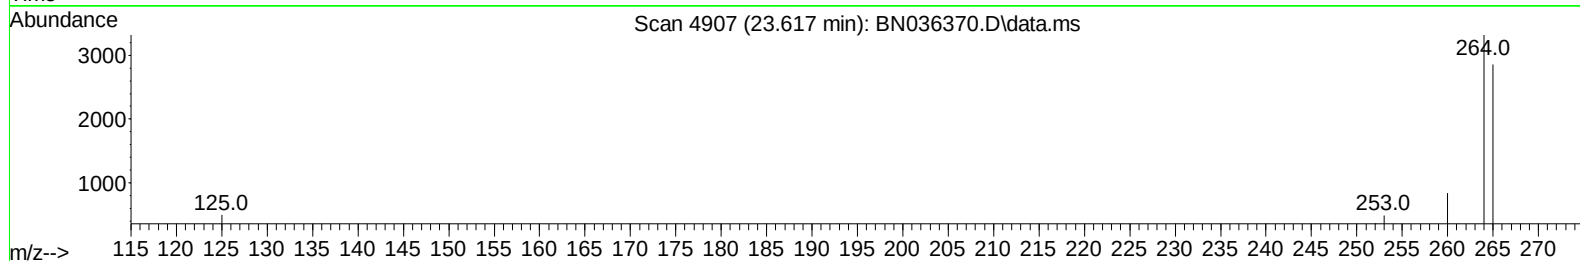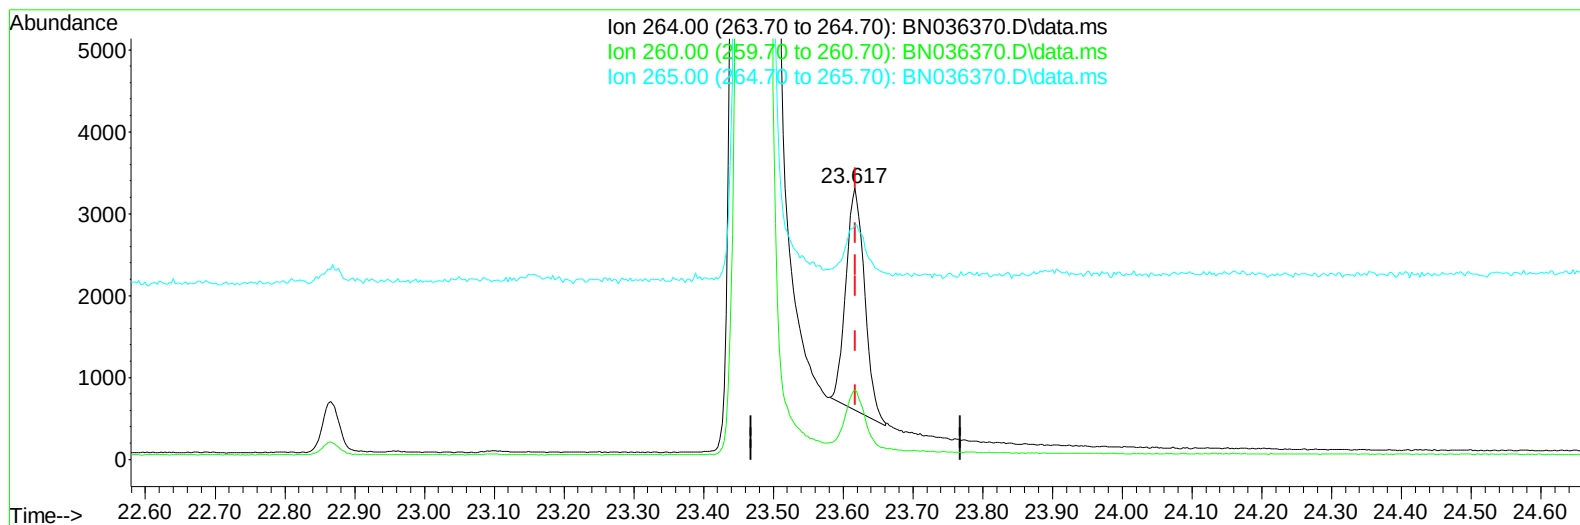

TIC: BN036370.D\data.ms

(23) Perylene-d12 (I)

23.617min (-0.002) 0.40 ng/ul m

response 5022

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.52
265.00	53.20	86.12#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
 Data File : BN036370.D
 Acq On : 07 Feb 2025 12:35
 Operator : RC/JU
 Sample : Q1229-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2991

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/10/2025
 Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 10 11:19:41 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 07 11:25:57 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.766	152	2757	0.400	ng/ul	0.00
4) Naphthalene-d8	10.557	136	6358	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.406	164	3381	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.151	188	6527m	0.400	ng/ul	0.00
17) Chrysene-d12	21.337	240	5364	0.400	ng/ul	# 0.00
23) Perylene-d12	23.617	264	5022m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.248	96	14231	4.714	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.152	152	2826	0.352	ng/ul	0.00
18) Fluoranthene-d10	19.180	212	6297	0.427	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036370.D
Acq On : 07 Feb 2025 12:35
Operator : RC/JU
Sample : Q1229-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2991

Manual IntegrationsAPPROVED

Quant Time: Feb 10 11:19:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/10/2025
Supervised By :Sohil Jodhani 02/18/2025

