




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036387.D
Acq On : 08 Feb 2025 00:00
Operator : RC/JU
Sample : Q1226-06
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCZM3

Manual IntegrationsAPPROVED

Quant Time: Feb 11 14:25:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/11/2025
Supervised By :Sohil Jodhani 02/18/2025

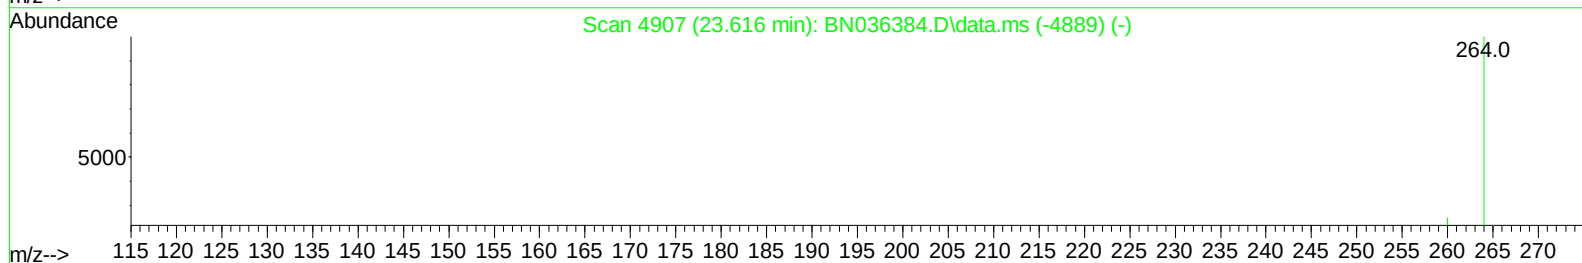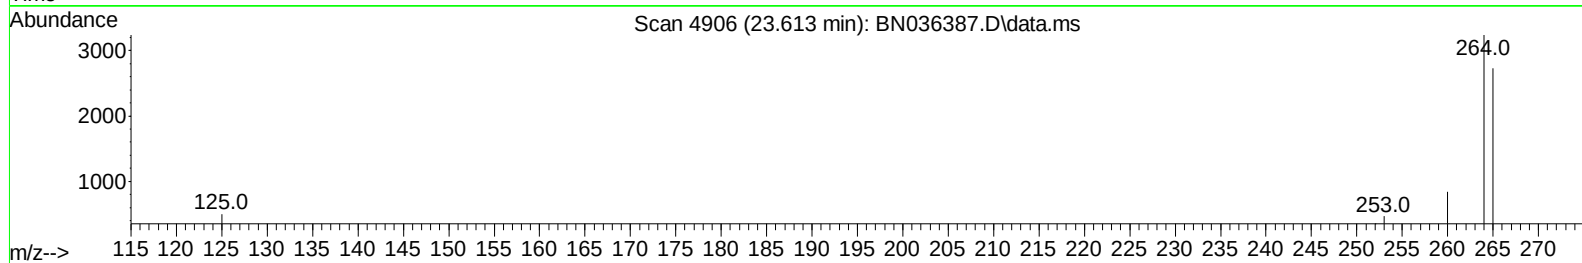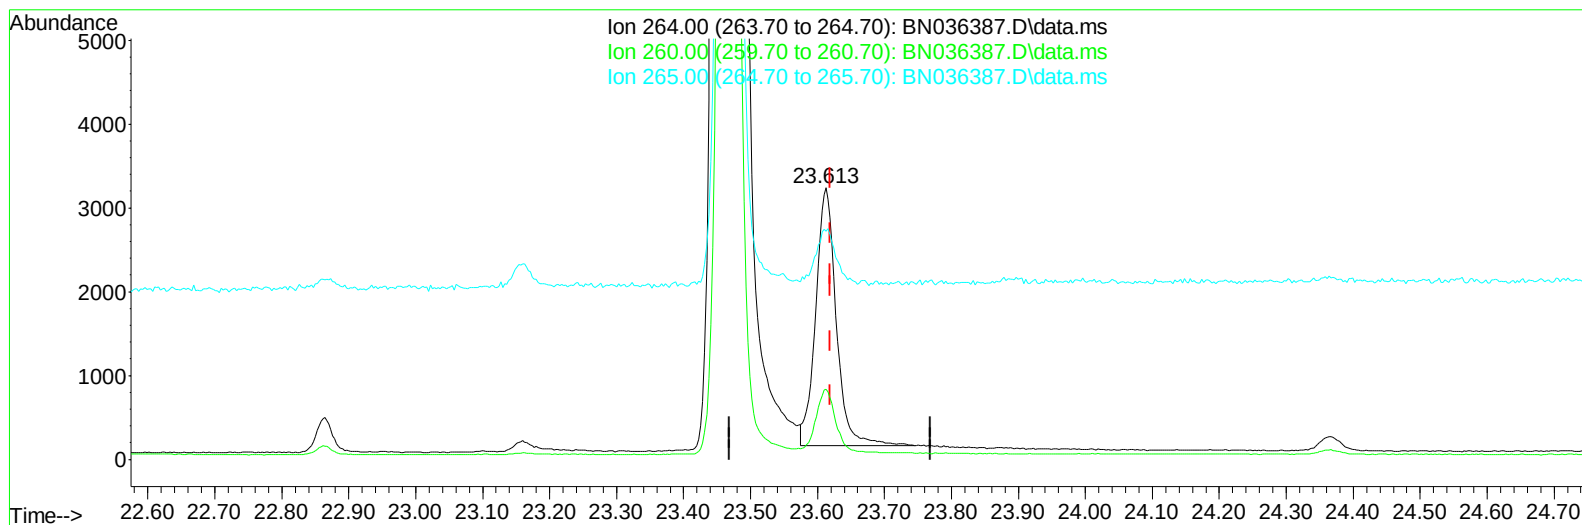

TIC: BN036387.D\data.ms

(23) Perylene-d12 (I)

23.613min (-0.006) 0.40 ng/u1

response 6629

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.85
265.00	53.20	84.16#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036387.D
Acq On : 08 Feb 2025 00:00
Operator : RC/JU
Sample : Q1226-06
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCZM3

Manual IntegrationsAPPROVED

Quant Time: Feb 11 14:25:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/11/2025
Supervised By :Sohil Jodhani 02/18/2025

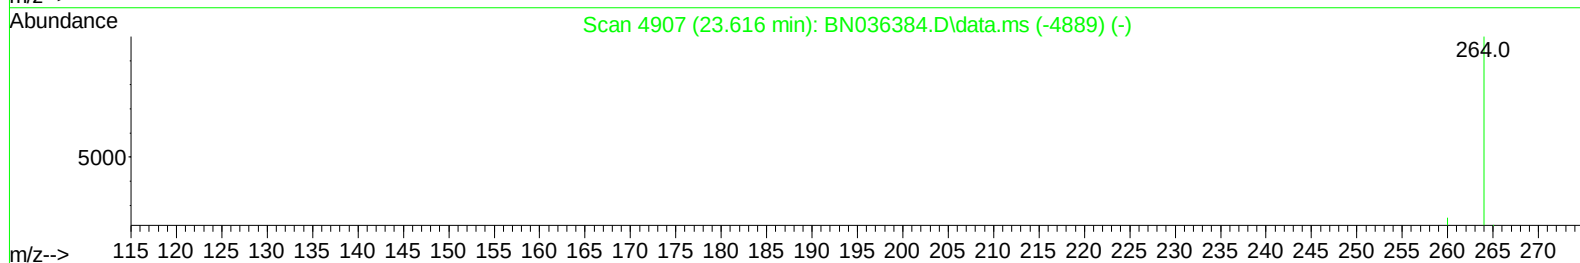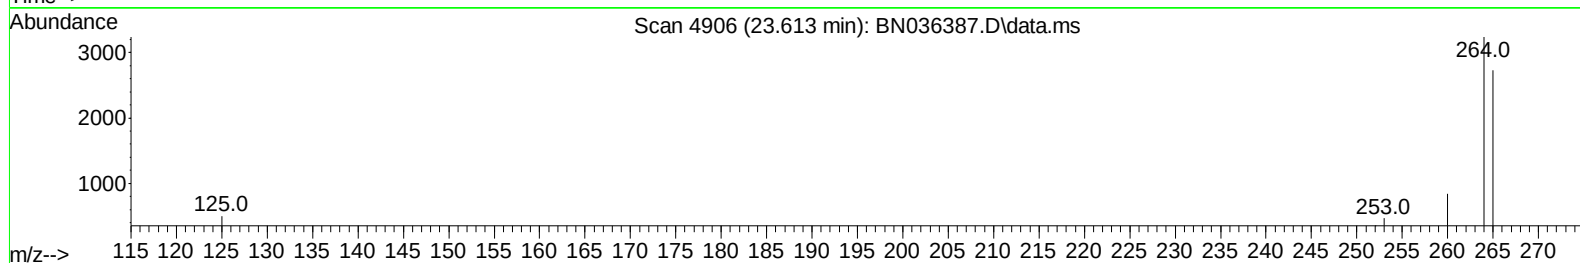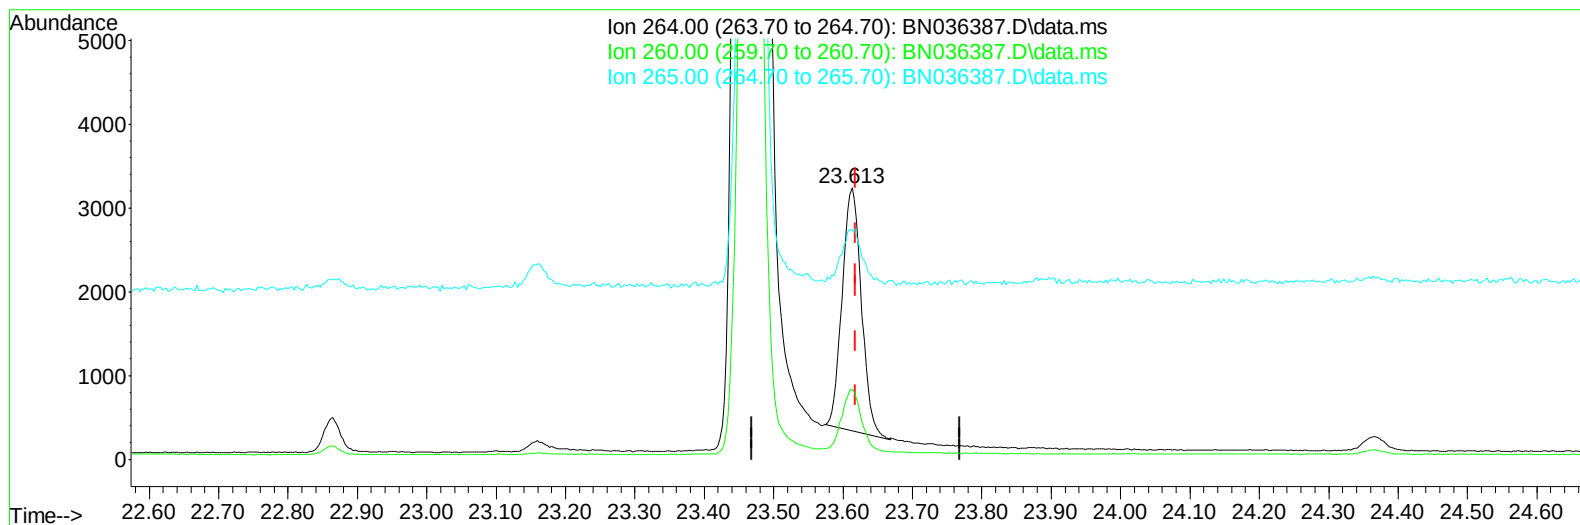

TIC: BN036387.D\data.ms

(23) Perylene-d12 (I)

23.613min (-0.006) 0.40 ng/ul m

response 5533

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.85
265.00	53.20	84.16#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
 Data File : BN036387.D
 Acq On : 08 Feb 2025 00:00
 Operator : RC/JU
 Sample : Q1226-06
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCZM3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/11/2025
 Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 11 14:25:17 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 07 11:25:57 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.766	152	2551	0.400	ng/ul	0.00
4) Naphthalene-d8	10.551	136	6022	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.405	164	3172	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.146	188	6871	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.336	240	5881	0.400	ng/ul	# 0.00
23) Perylene-d12	23.613	264	5533m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.248	96	16903	6.052	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.146	152	1271	0.167	ng/ul	-0.01
18) Fluoranthene-d10	19.174	212	6940	0.429	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036387.D
Acq On : 08 Feb 2025 00:00
Operator : RC/JU
Sample : Q1226-06
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCZM3

Manual IntegrationsAPPROVED

Quant Time: Feb 11 14:25:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/11/2025
Supervised By :Sohil Jodhani 02/18/2025

