

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
 Data File : BN036338.D
 Acq On : 06 Feb 2025 16:45
 Operator : RC/JU
 Sample : Q1226-24
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCZN2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
 Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 06 17:57:48 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 06 14:44:03 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.771	152	2763	0.400	ng/ul	0.00
4) Naphthalene-d8	10.557	136	6482	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.409	164	3598	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.154	188	7251m	0.400	ng/ul	0.00
17) Chrysene-d12	21.342	240	6369	0.400	ng/ul	# 0.00
23) Perylene-d12	23.622	264	6205m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	14202	4.695	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.157	152	2559	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.184	212	6180	0.353	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.812	266	60	0.024	ng/ul	Qvalue 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036338.D
Acq On : 06 Feb 2025 16:45
Operator : RC/JU
Sample : Q1226-24
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCZN2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025


Quant Time: Feb 06 17:57:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 14:44:03 2025
Response via : Initial Calibration

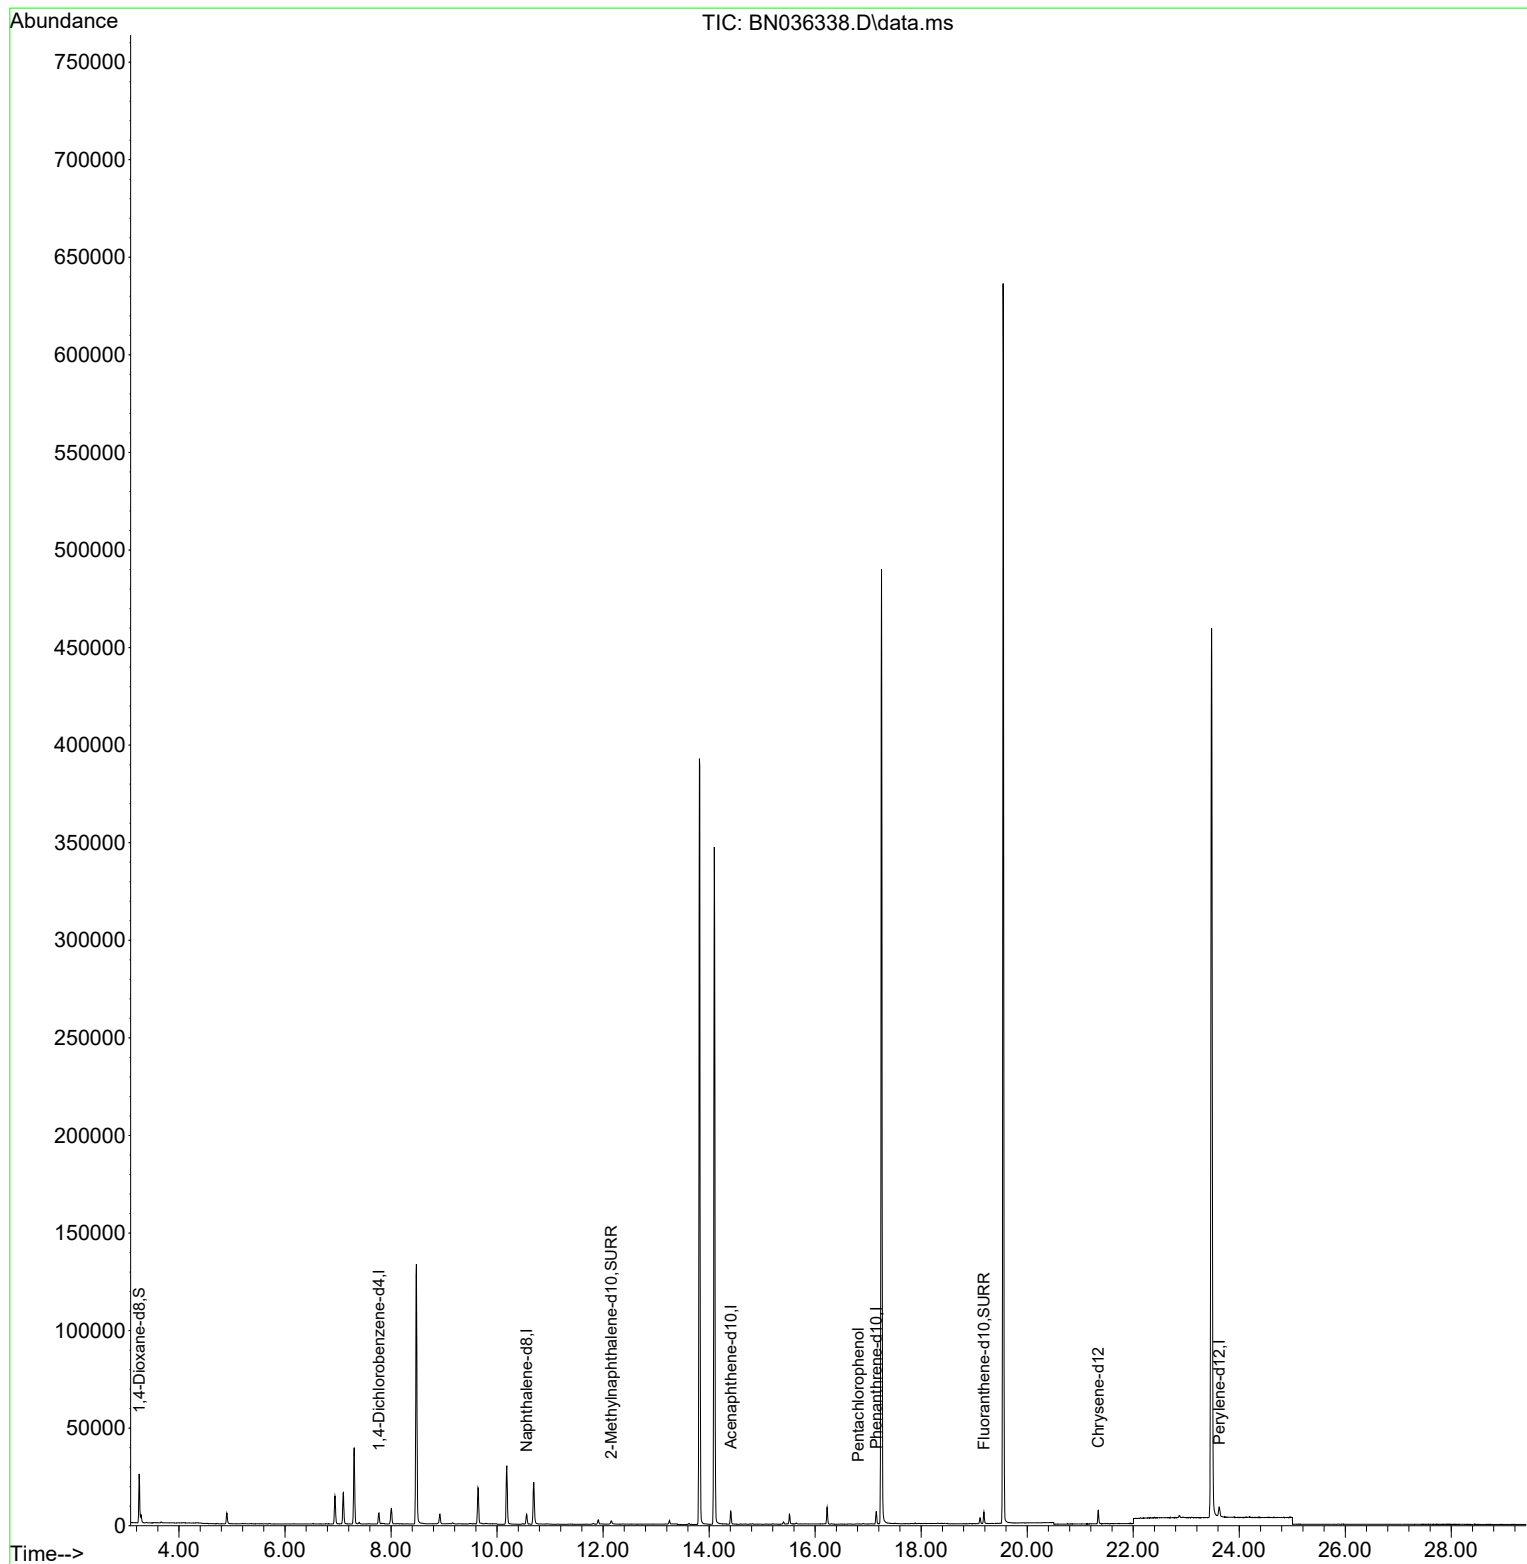

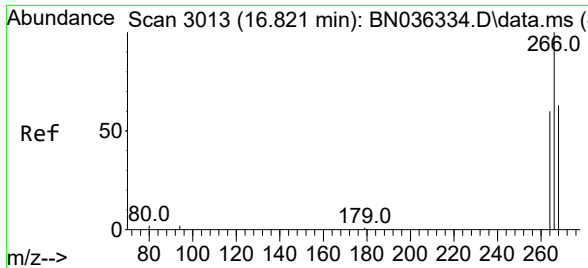

#14
 Pentachlorophenol
 Concen: 0.024 ng/ul
 RT: 16.812 min Scan# 3011
 Delta R.T. -0.008 min
 Lab File: BN036338.D
 Acq: 06 Feb 2025 16:45

Instrument :
 BNA_N
 ClientSampleId :
 DCZN2

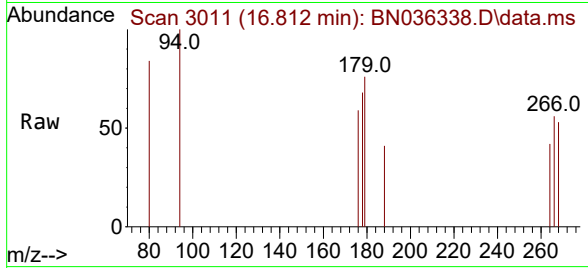

Tgt Ion: 266 Resp: 60

Ion	Ratio	Lower	Upper
266	100		
264	66.7	50.6	75.8
268	75.0	50.6	75.8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
 Supervised By :Sohil Jodhani 02/18/2025

