

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
 Data File : BN036346.D
 Acq On : 06 Feb 2025 21:34
 Operator : RC/JU
 Sample : Q1226-26
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCZP4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
 Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 07 07:46:27 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 06 14:44:03 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.771	152	3034	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.557	136	7817	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.410	164	4725	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.151	188	9694m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.340	240	7215	0.400	ng/ul	#-0.02
23) Perylene-d12	23.617	264	5957m	0.400	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.248	96	16631	5.007	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.157	152	3425	0.347	ng/ul	-0.01
18) Fluoranthene-d10	19.185	212	8939	0.451	ng/ul	-0.02
Target Compounds						Qvalue
14) Pentachlorophenol	16.809	266	1141	0.336	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036346.D
Acq On : 06 Feb 2025 21:34
Operator : RC/JU
Sample : Q1226-26
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCZP4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025


Quant Time: Feb 07 07:46:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 14:44:03 2025
Response via : Initial Calibration

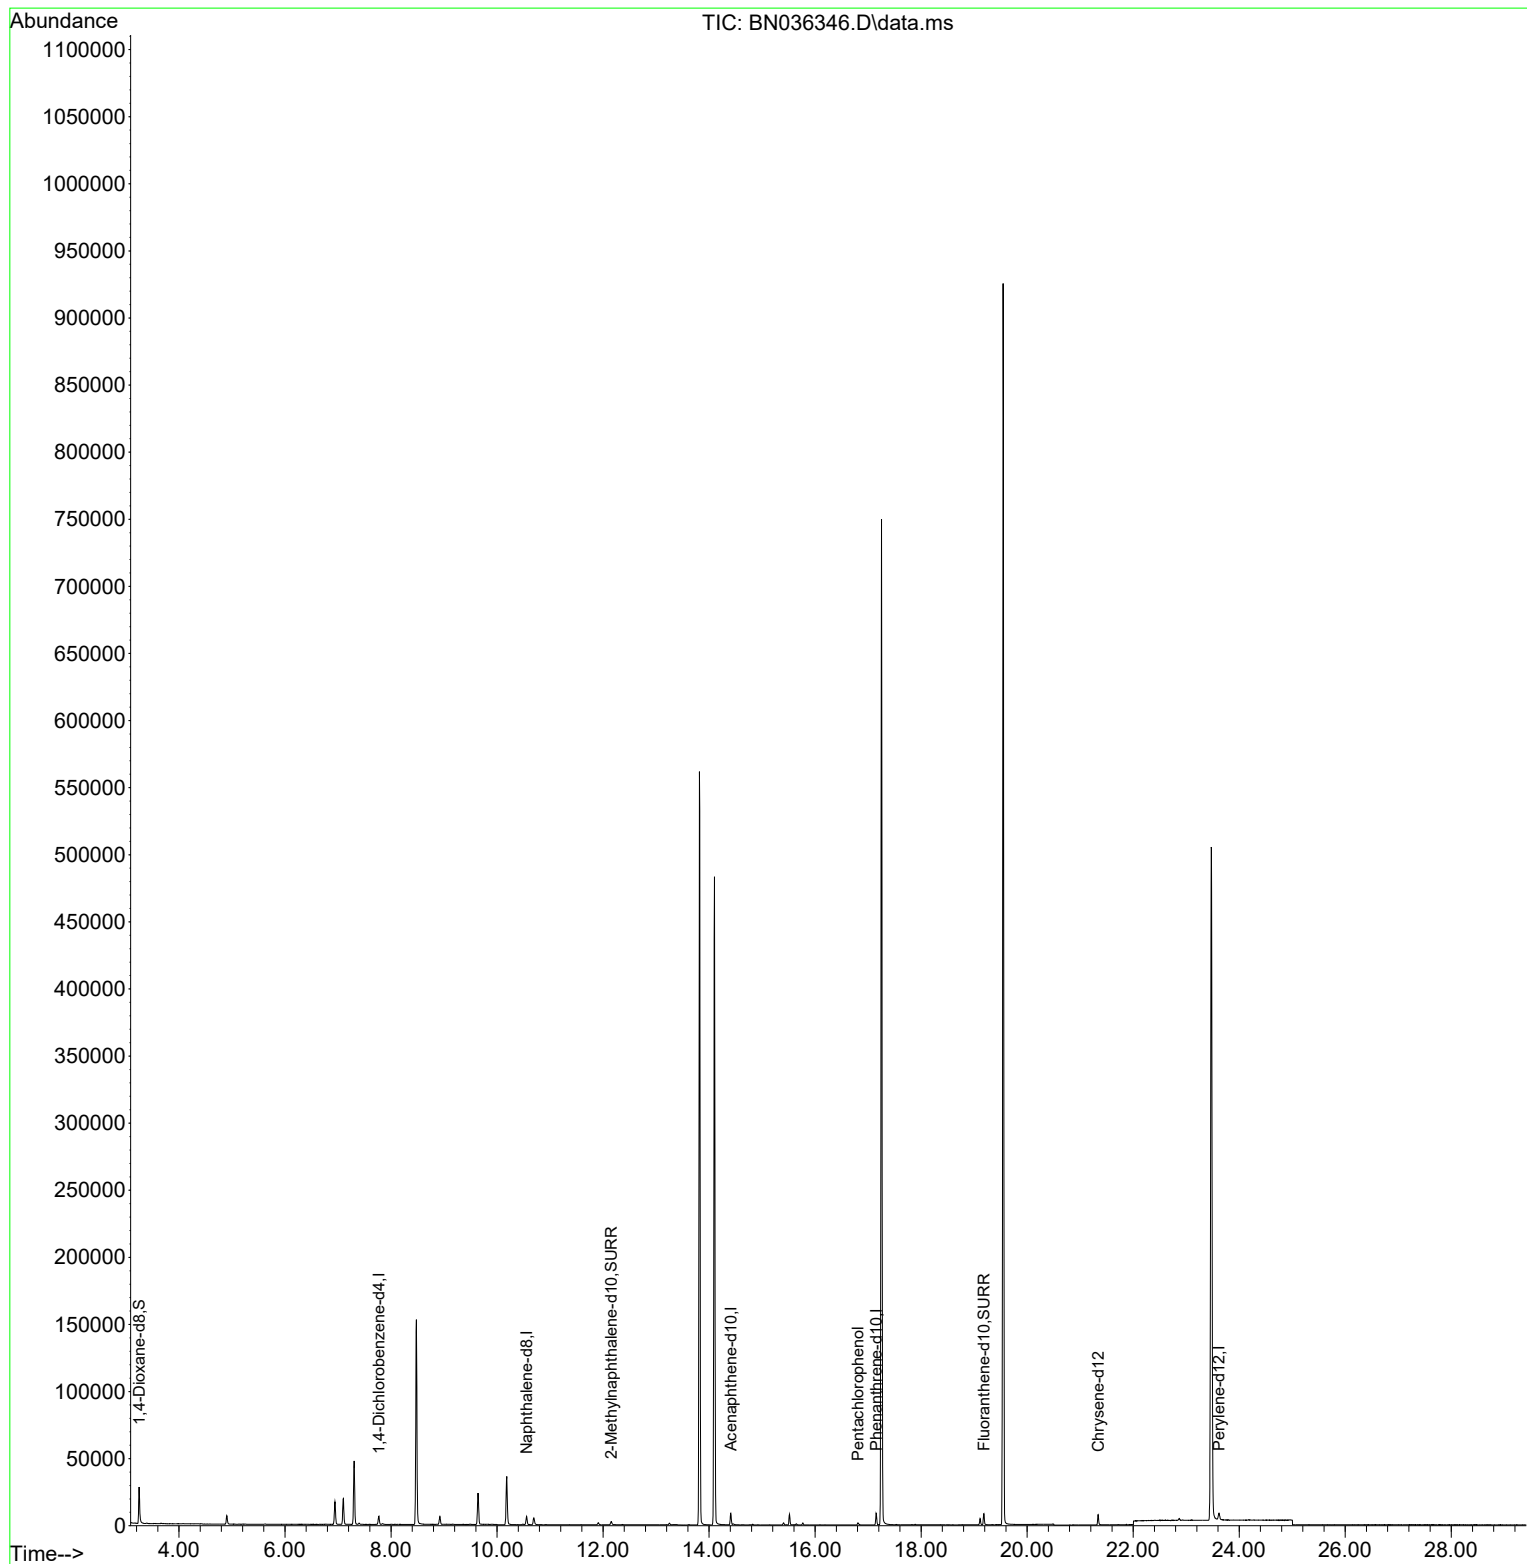

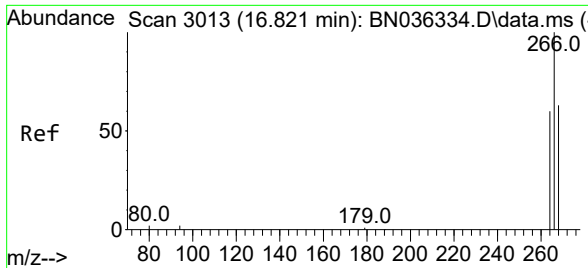

#14
Pentachlorophenol
Concen: 0.336 ng/ul
RT: 16.809 min Scan# 3010
Delta R.T. -0.019 min
Lab File: BN036346.D
Acq: 06 Feb 2025 21:34

Instrument :
BNA_N
ClientSampleId :
DCZP4

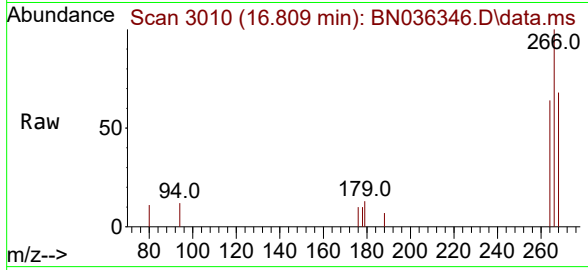

Tgt Ion: 266 Resp: 114

Ion	Ratio	Lower	Upper
266	100		
264	63.5	50.6	75.8
268	65.1	50.6	75.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/18/2025

