

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
 Data File : BN036379.D
 Acq On : 07 Feb 2025 18:35
 Operator : RC/JU
 Sample : Q1229-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29B9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/11/2025
 Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 11 12:46:08 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 07 11:25:57 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.766	152	2816	0.400	ng/u1	0.00
4) Naphthalene-d8	10.551	136	6632	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.405	164	3570	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.146	188	6972m	0.400	ng/u1	0.00
17) Chrysene-d12	21.336	240	5921	0.400	ng/u1	# 0.00
23) Perylene-d12	23.613	264	5902m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.248	96	14074	4.565	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.152	152	2479	0.296	ng/u1	0.00
18) Fluoranthene-d10	19.179	212	6173	0.379	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.804	266	8375	3.429	ng/u1	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036379.D
Acq On : 07 Feb 2025 18:35
Operator : RC/JU
Sample : Q1229-13
Misc :
ALS Vial : 49 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E29B9

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/11/2025
Supervised By :Sohil Jodhani 02/18/2025


Quant Time: Feb 11 12:46:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

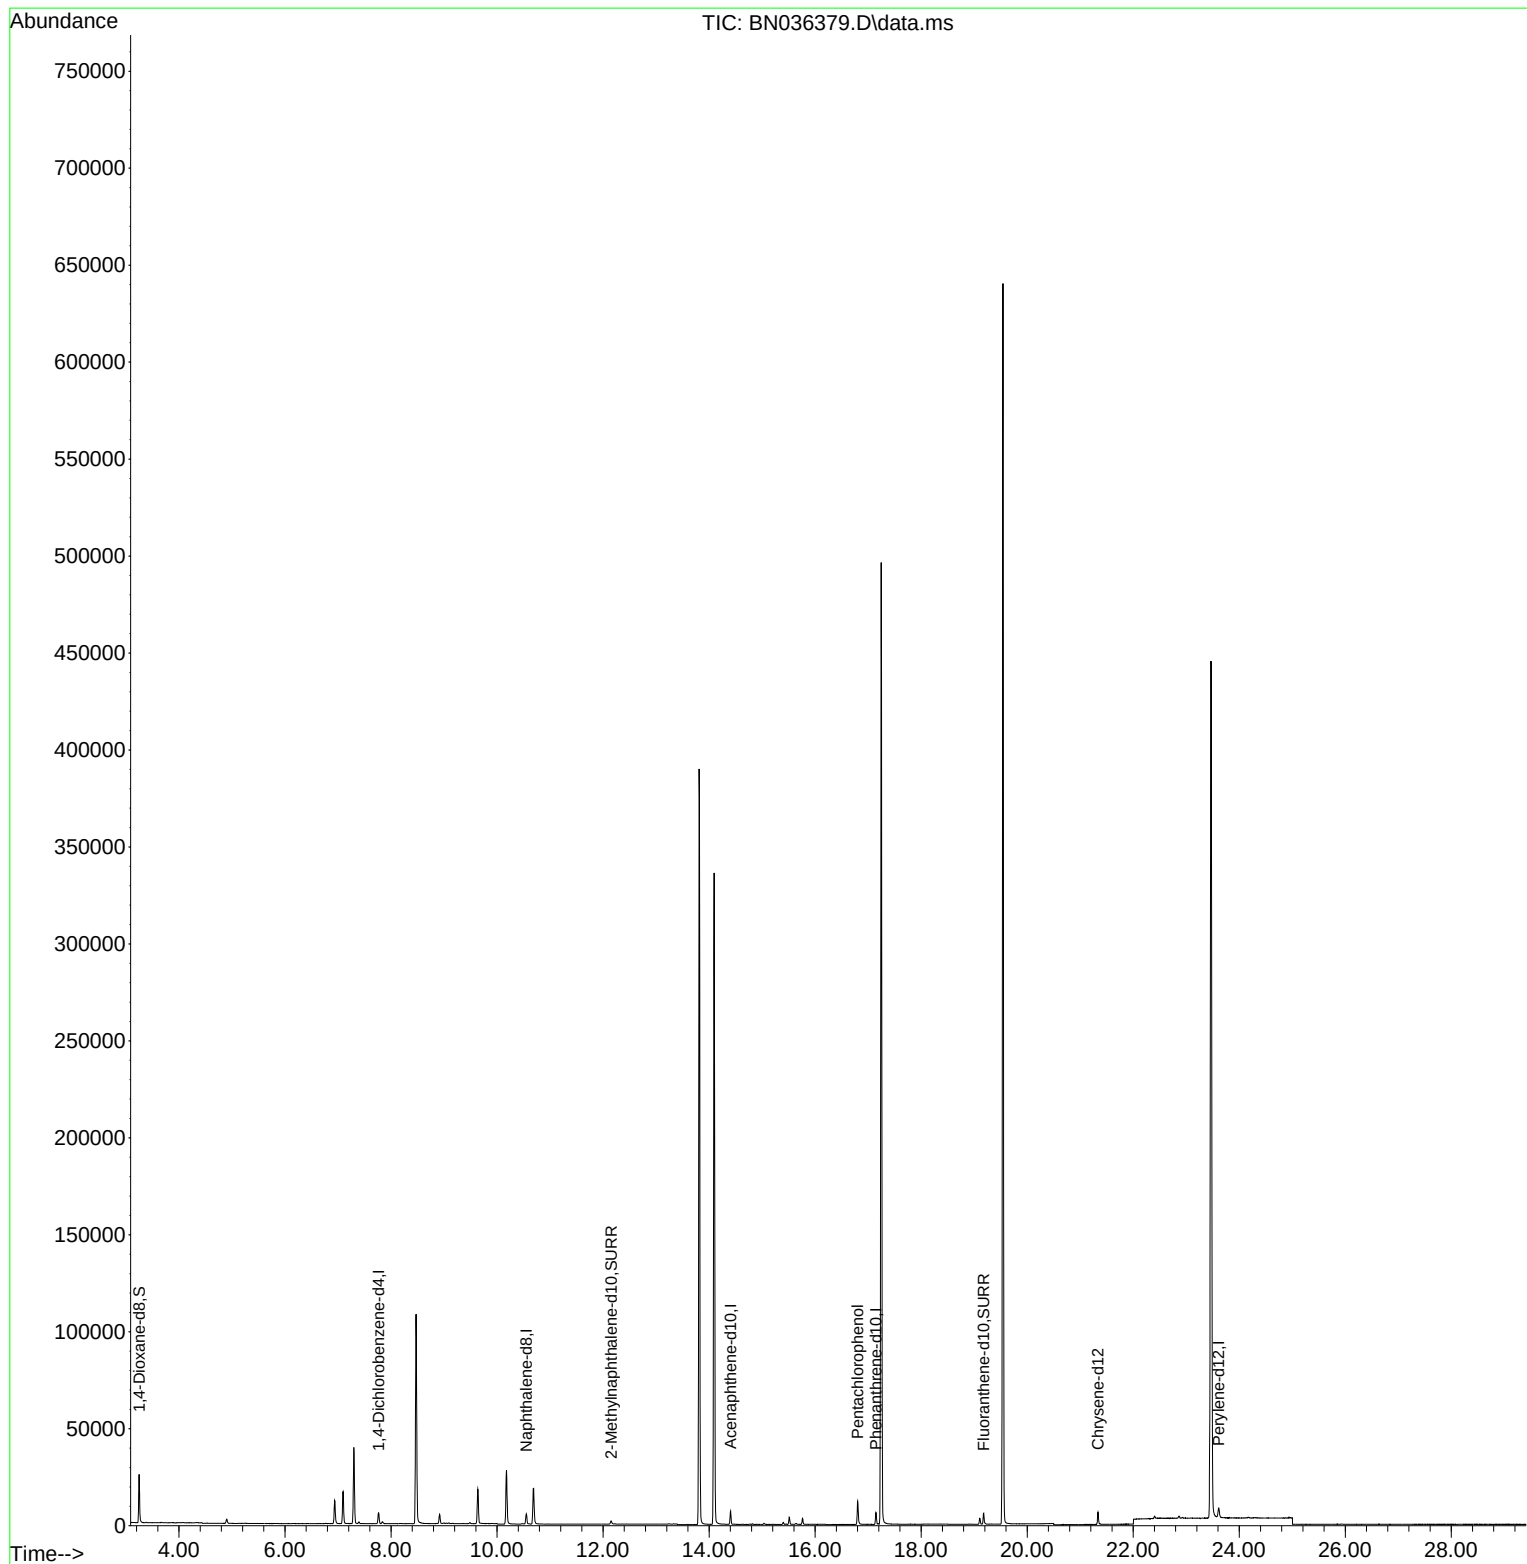

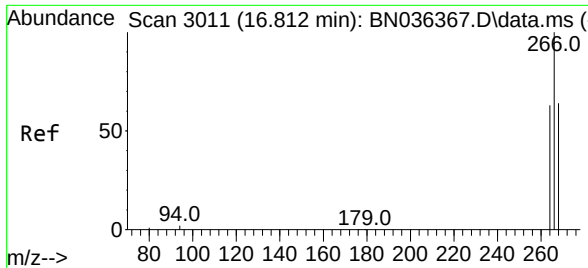

#14
Pentachlorophenol
Concen: 3.429 ng/ul
RT: 16.804 min Scan# 3011
Delta R.T. -0.008 min
Lab File: BN036379.D
Acq: 07 Feb 2025 18:35

Instrument :
BNA_N
ClientSampleId :
E29B9

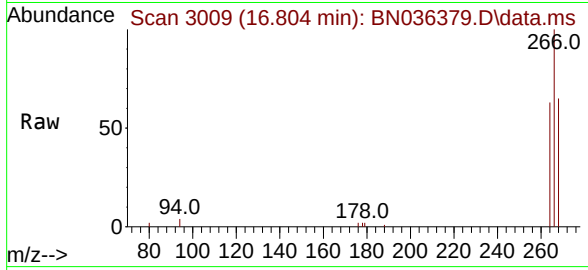

Tgt Ion:	266	Resp:	837
Ion Ratio	Lower	Upper	
266	100		
264	63.1	50.6	75.8
268	63.8	50.6	75.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/11/2025
Supervised By :Sohil Jodhani 02/18/2025

