

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
 Data File : BN036391.D
 Acq On : 08 Feb 2025 02:25
 Operator : RC/JU
 Sample : Q1247-14
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A6341

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/11/2025
 Supervised By :Sohil Jodhani 02/18/2025

Quant Time: Feb 11 14:50:55 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 07 11:25:57 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.762	152	3016	0.400	ng/ul	0.00
4) Naphthalene-d8	10.551	136	6997	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.405	164	3810	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.146	188	7552m	0.400	ng/ul	0.00
17) Chrysene-d12	21.333	240	6407	0.400	ng/ul	# 0.00
23) Perylene-d12	23.607	264	6308m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.248	96	13836	4.190	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.152	152	2253	0.255	ng/ul	0.00
18) Fluoranthene-d10	19.179	212	5546	0.315	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.601	128	430	0.022	ng/ul#	66

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020625\
Data File : BN036391.D
Acq On : 08 Feb 2025 02:25
Operator : RC/JU
Sample : Q1247-14
Misc :
ALS Vial : 62 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A6341

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/11/2025
Supervised By :Sohil Jodhani 02/18/2025


Quant Time: Feb 11 14:50:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

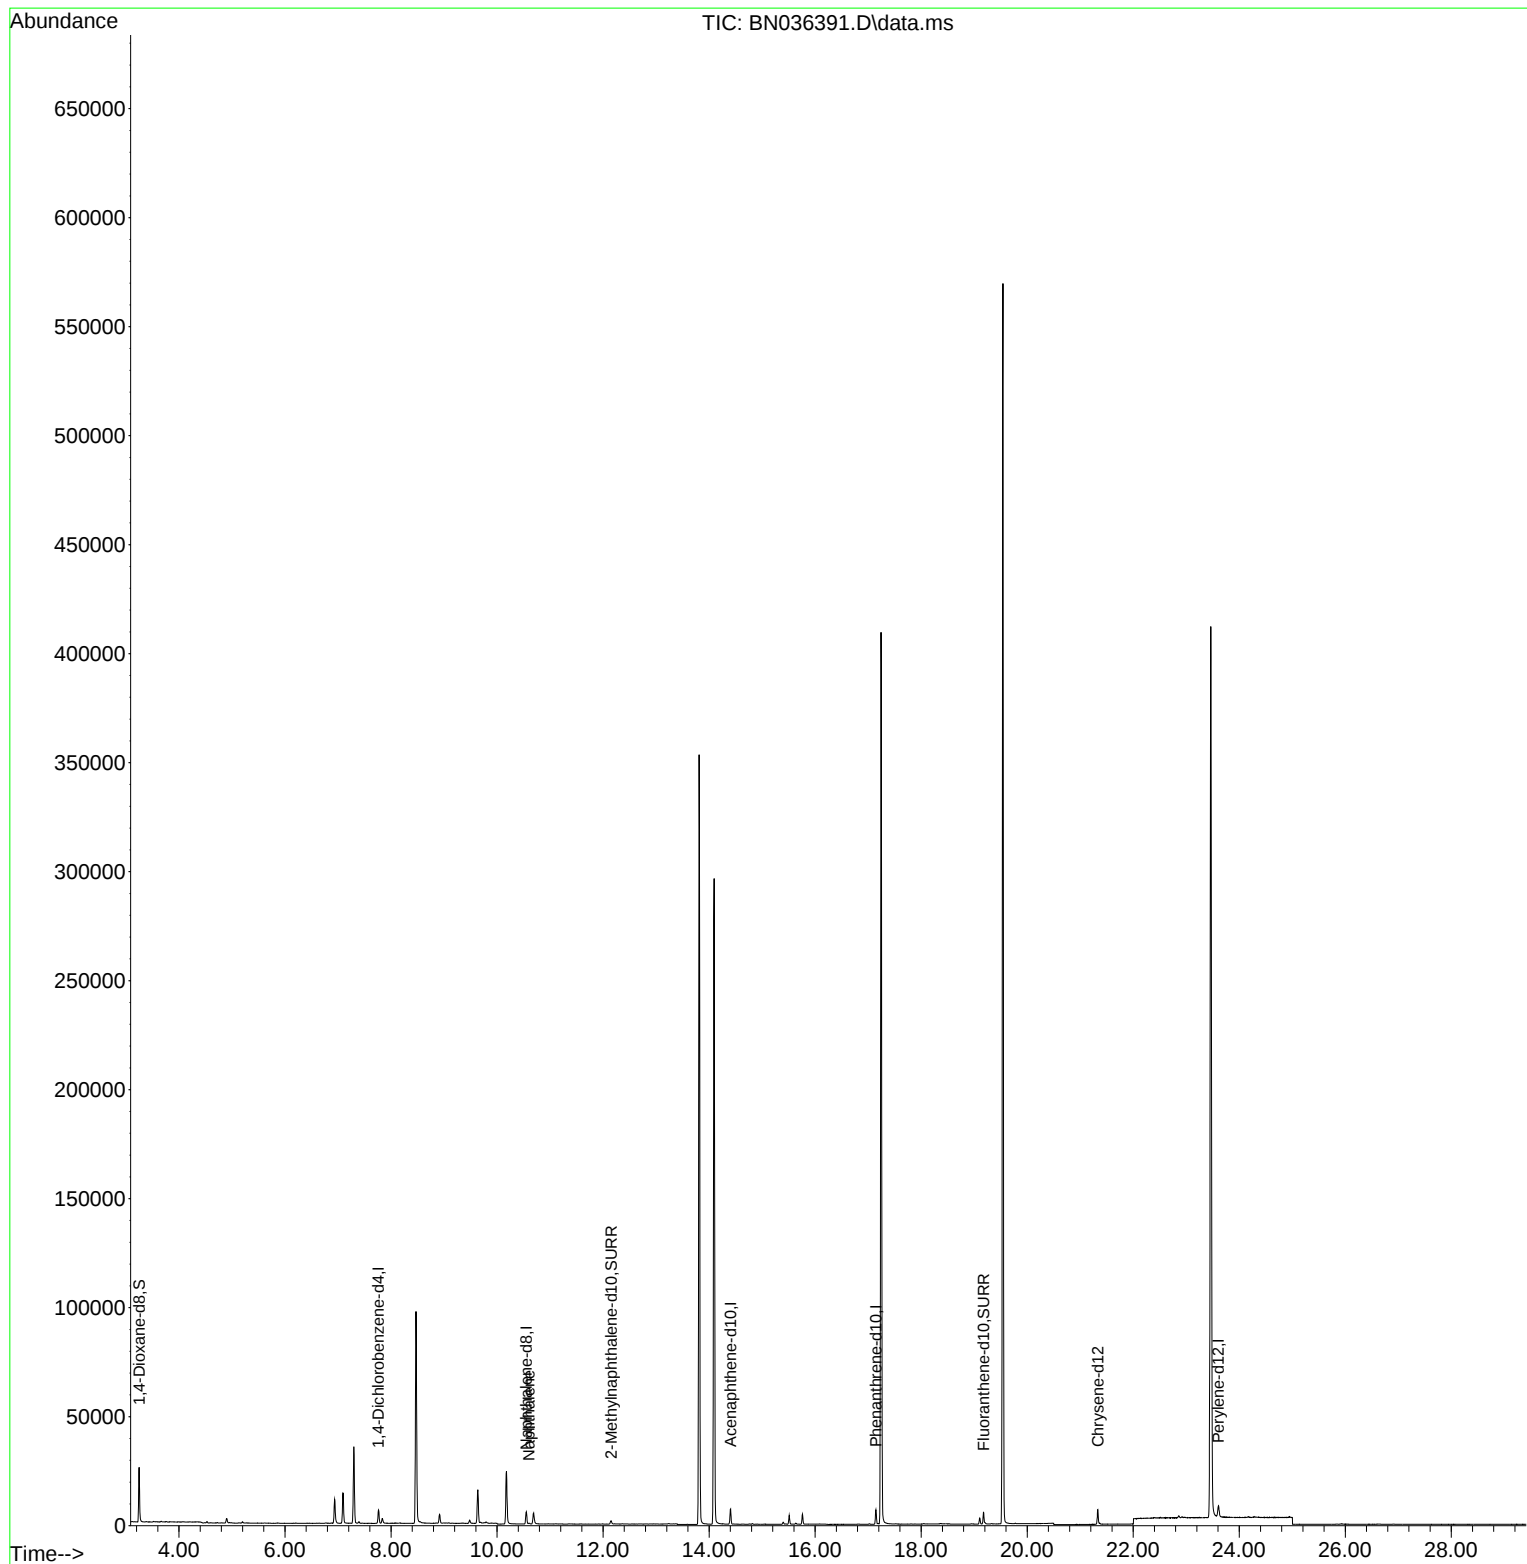

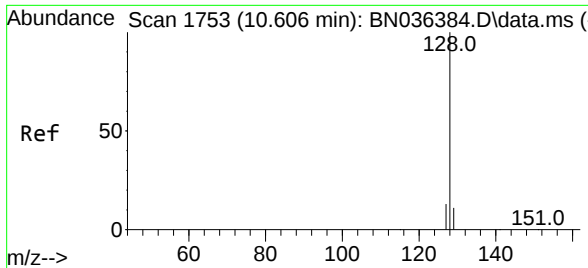

#5
Naphthalene
Concen: 0.022 ng/ul
RT: 10.601 min Scan# 1752
Delta R.T. -0.005 min
Lab File: BN036391.D
Acq: 08 Feb 2025 02:25

Instrument :
BNA_N
ClientSampleId :
A6341

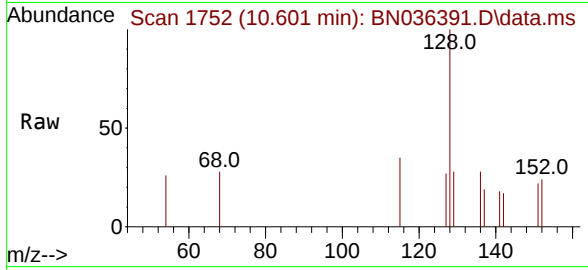

Tgt Ion:128 Resp: 430

Ion	Ratio	Lower	Upper
128	100		
129	27.8	9.6	14.4
127	27.2	12.0	18.0

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/11/2025
Supervised By :Sohil Jodhani 02/18/2025

