




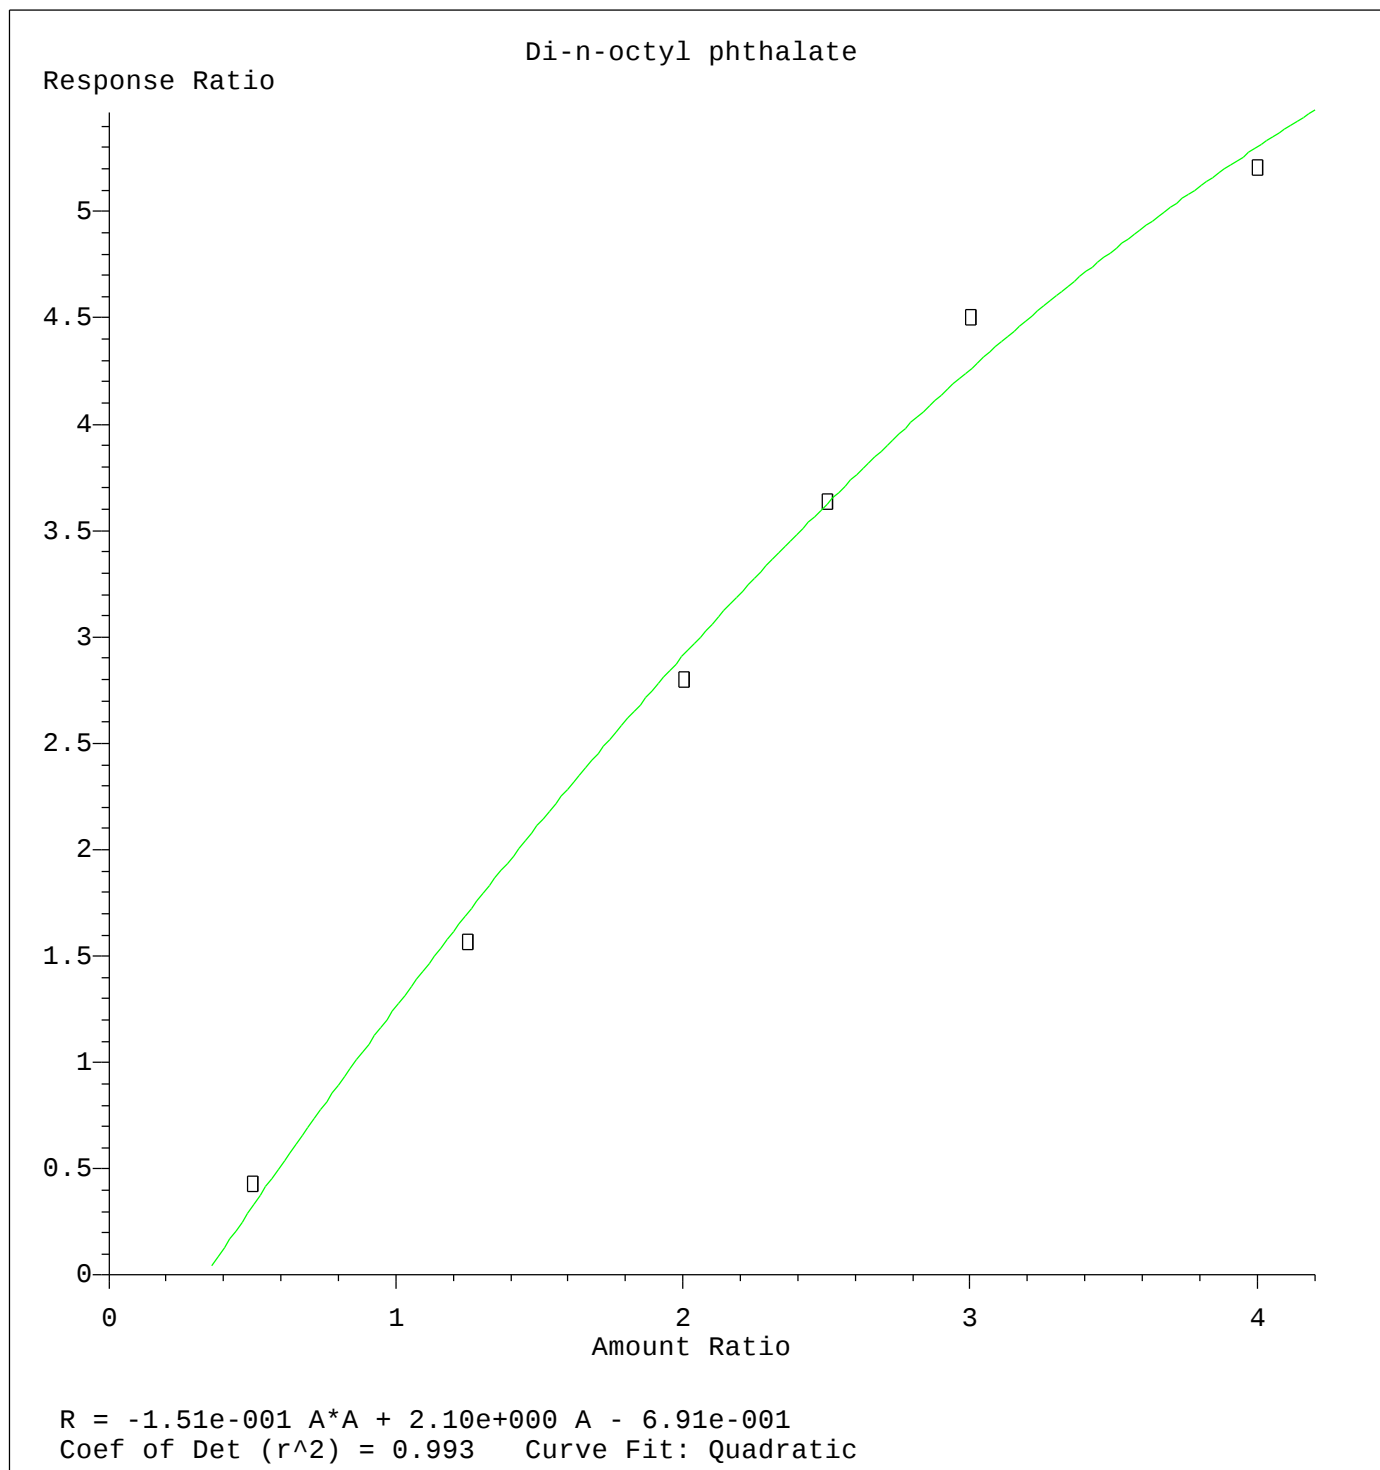


Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018

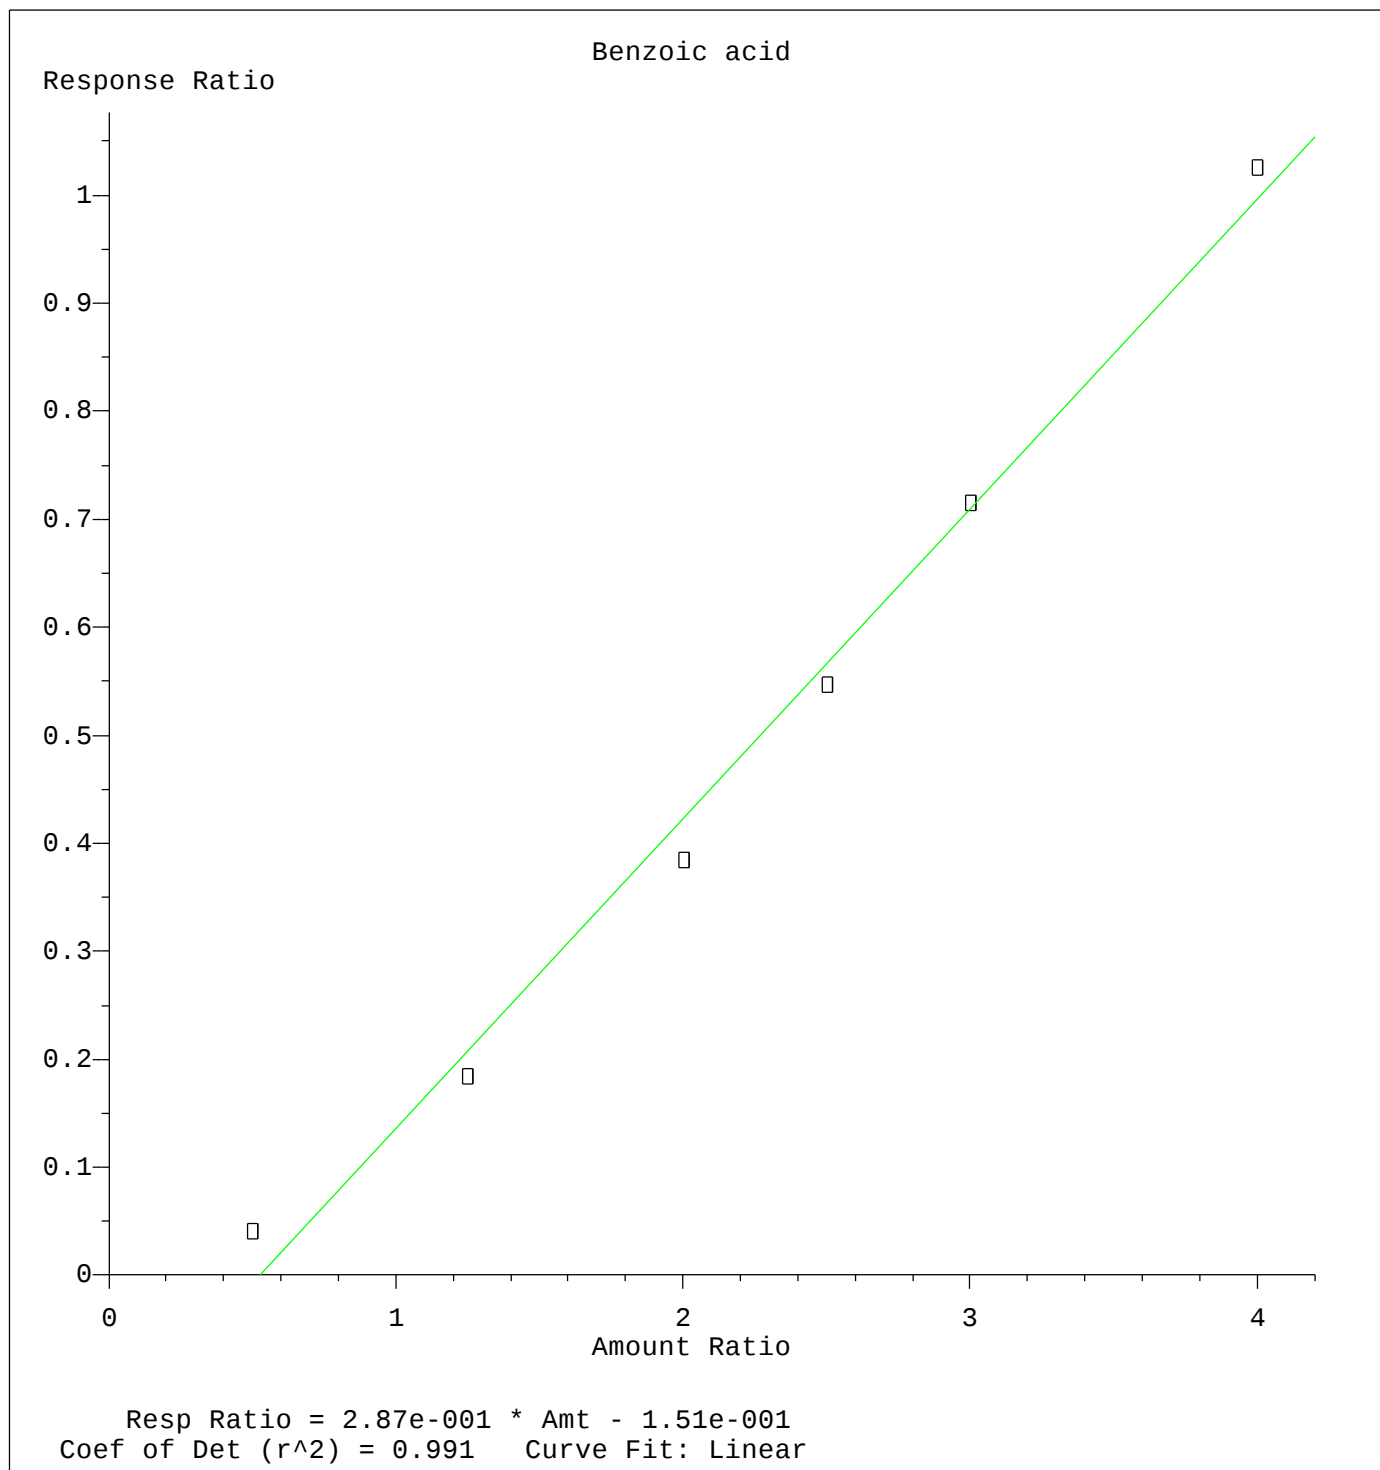


Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018

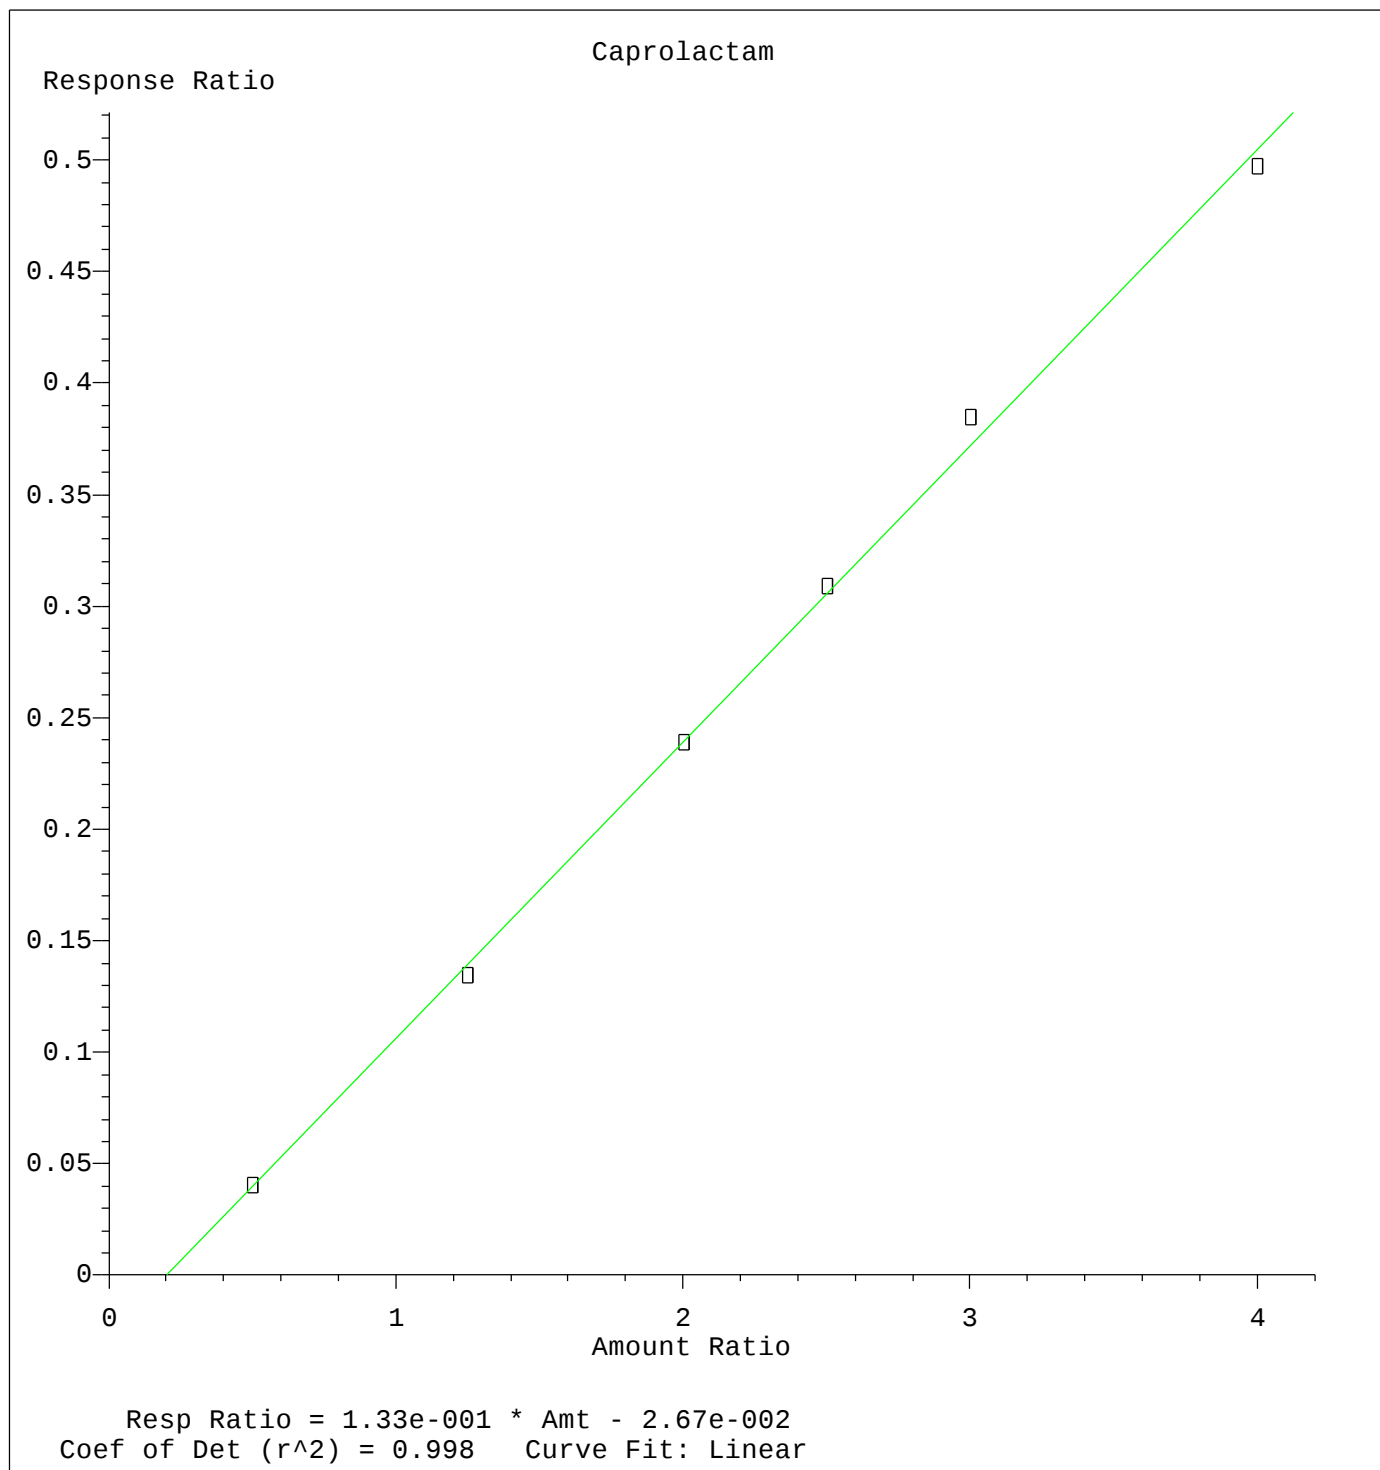


Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018

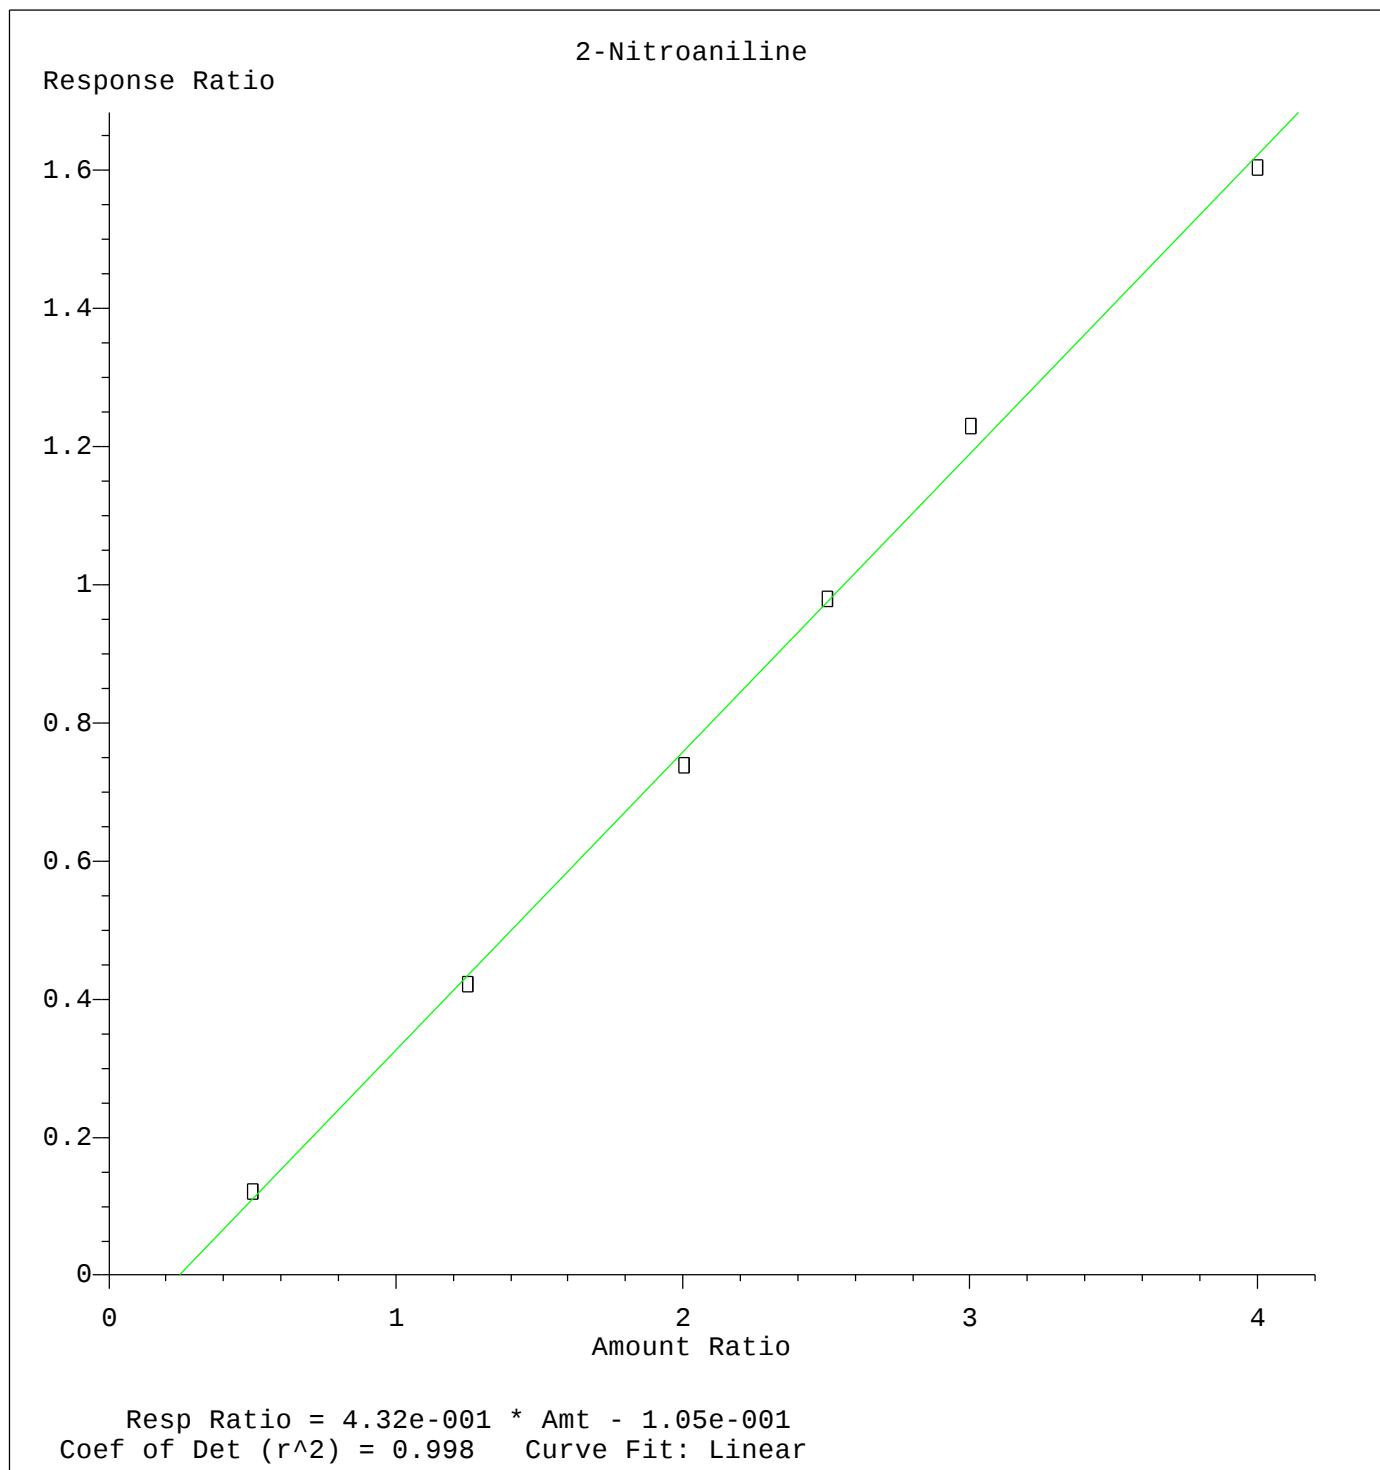

Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018

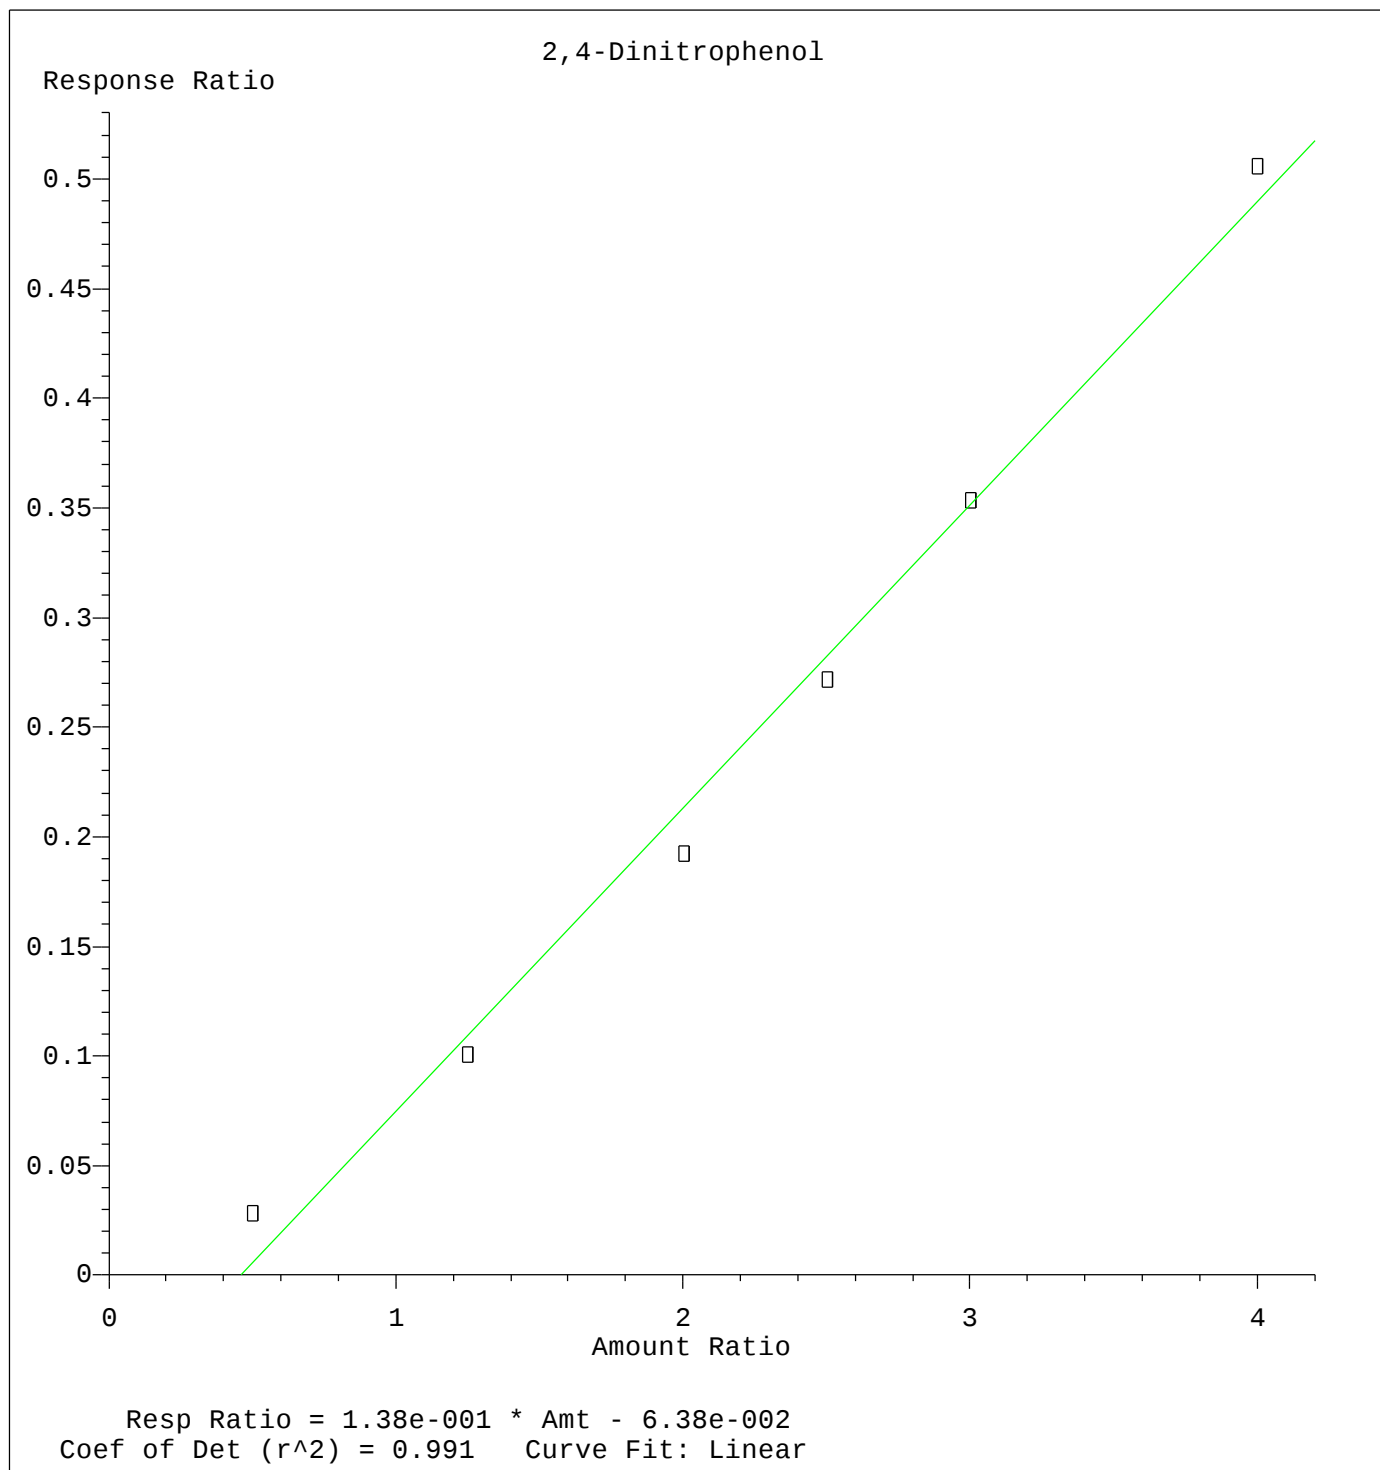


Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018

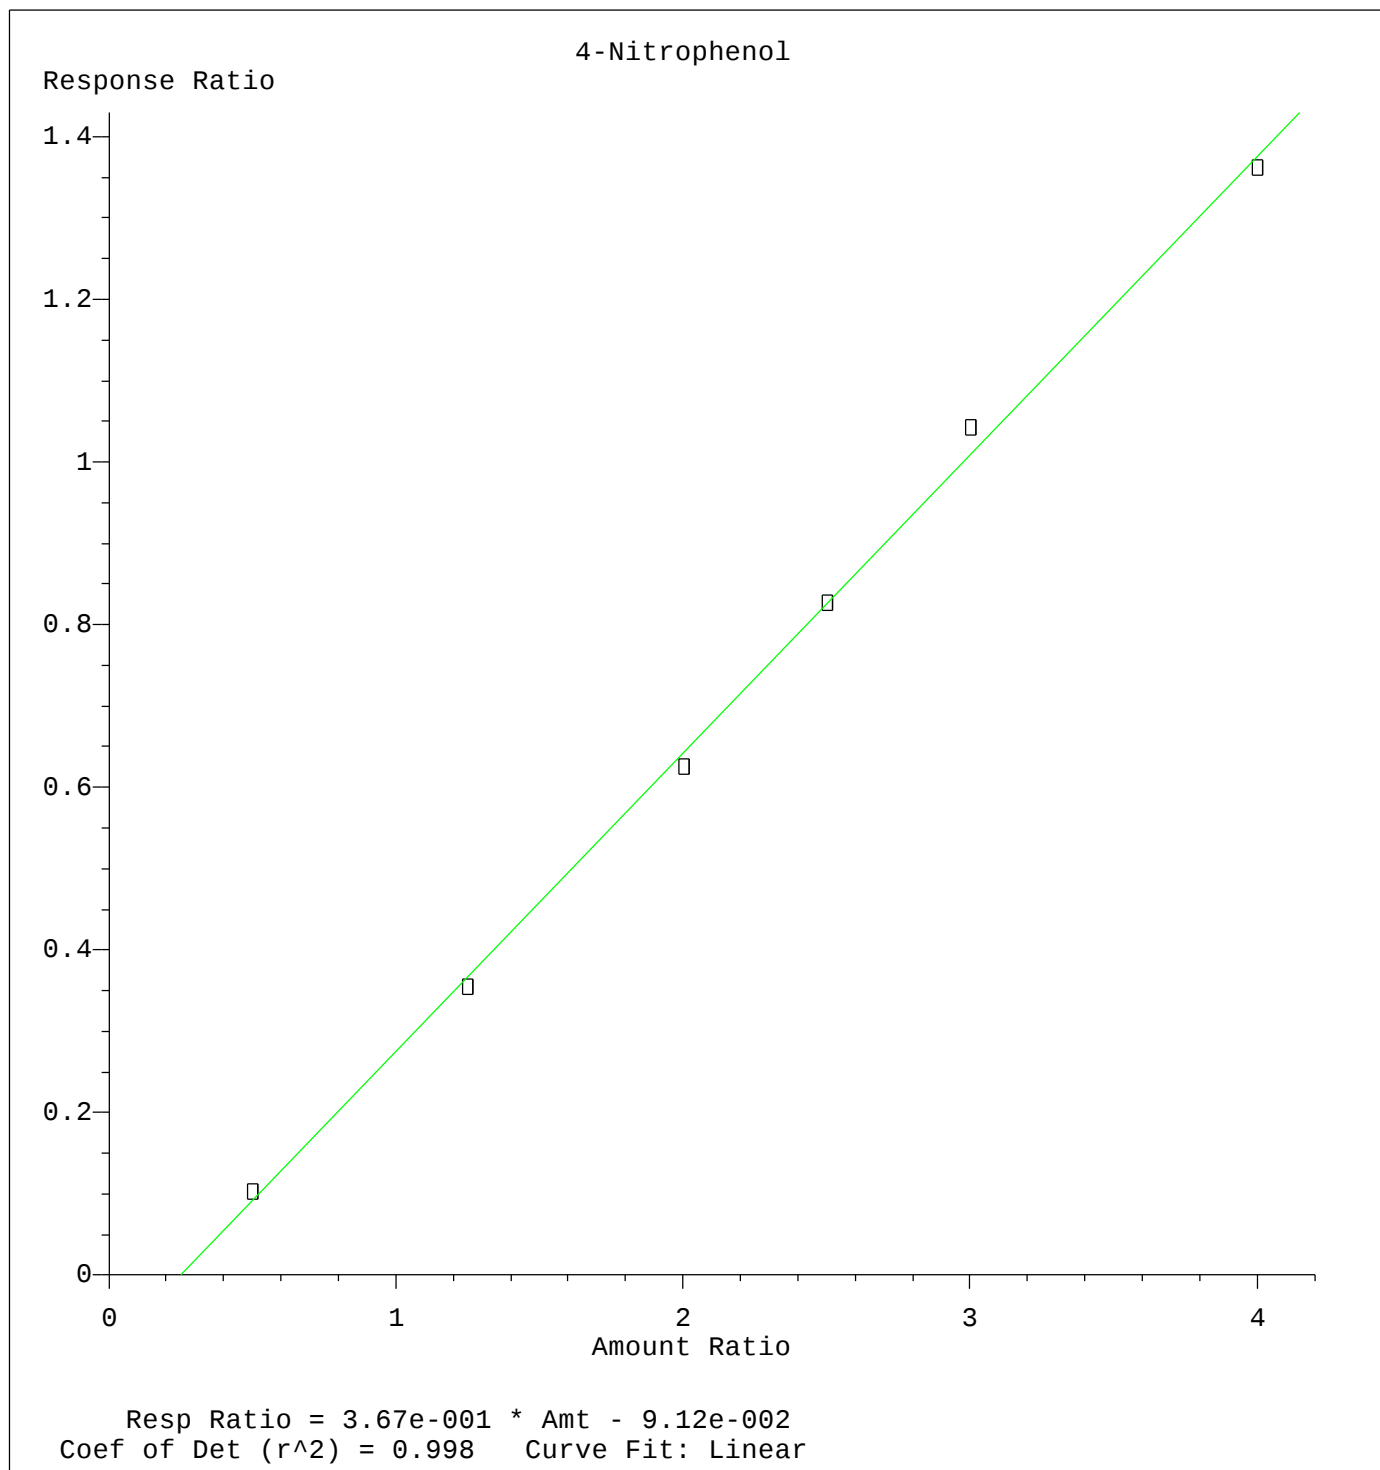

Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018

2,4-Dinitrotoluene


Response Ratio

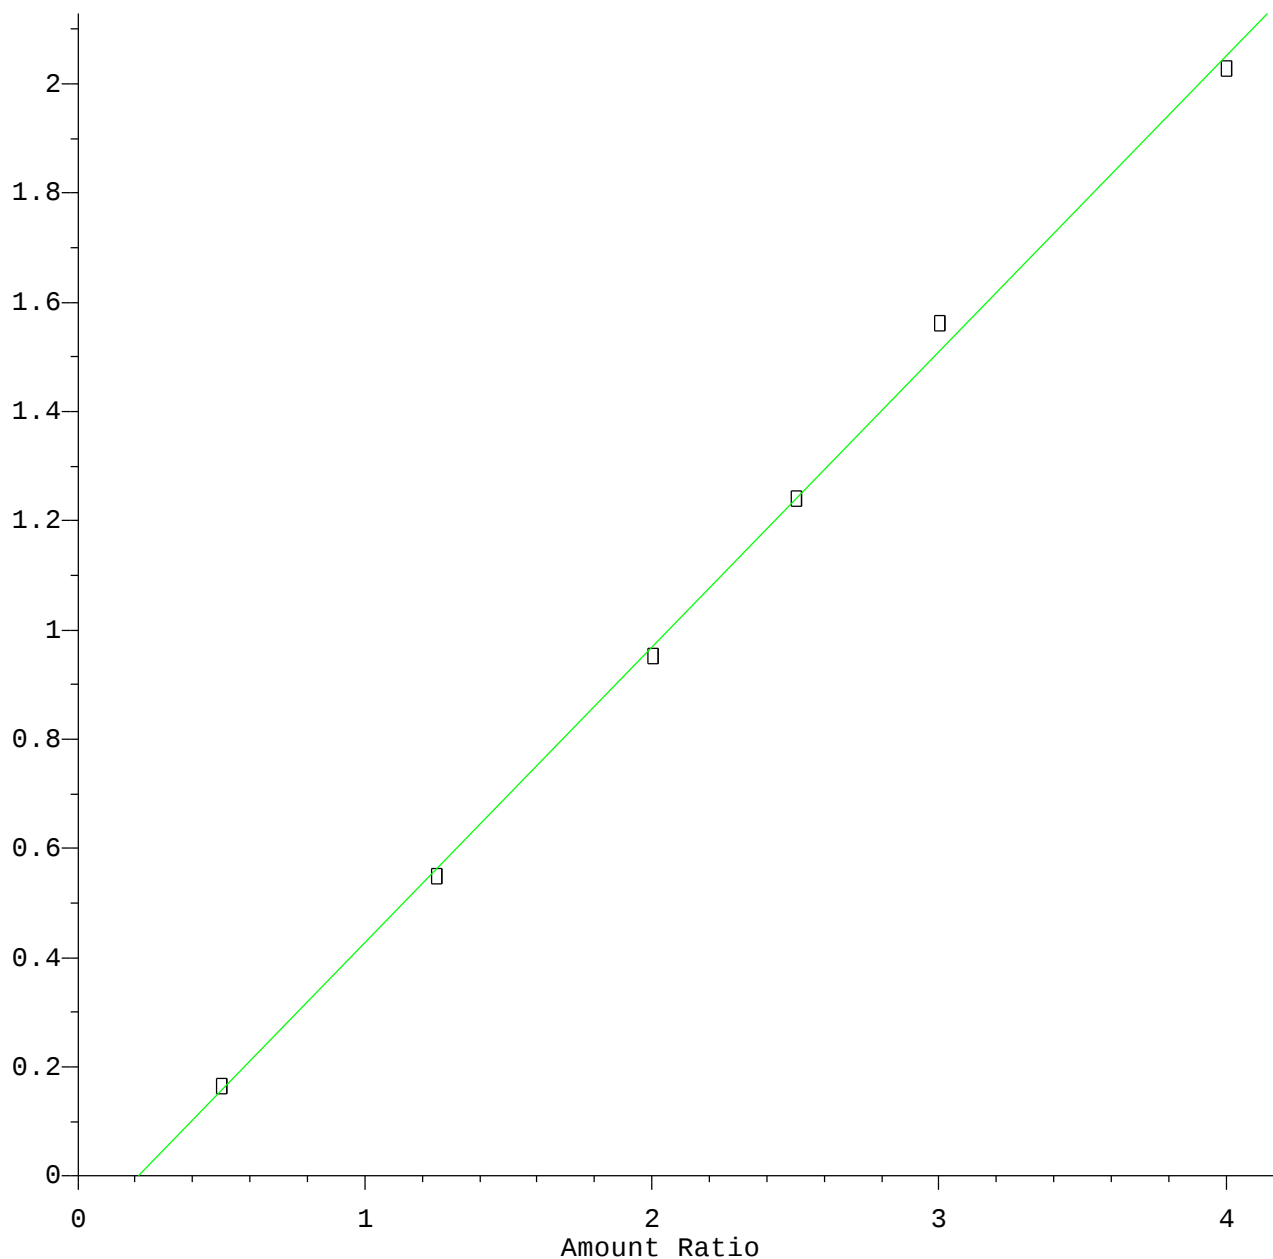

Resp Ratio = $5.41 \times 10^{-1} \times \text{Amt} - 1.13 \times 10^{-1}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018

4,6-Dinitro-2-methylphenol

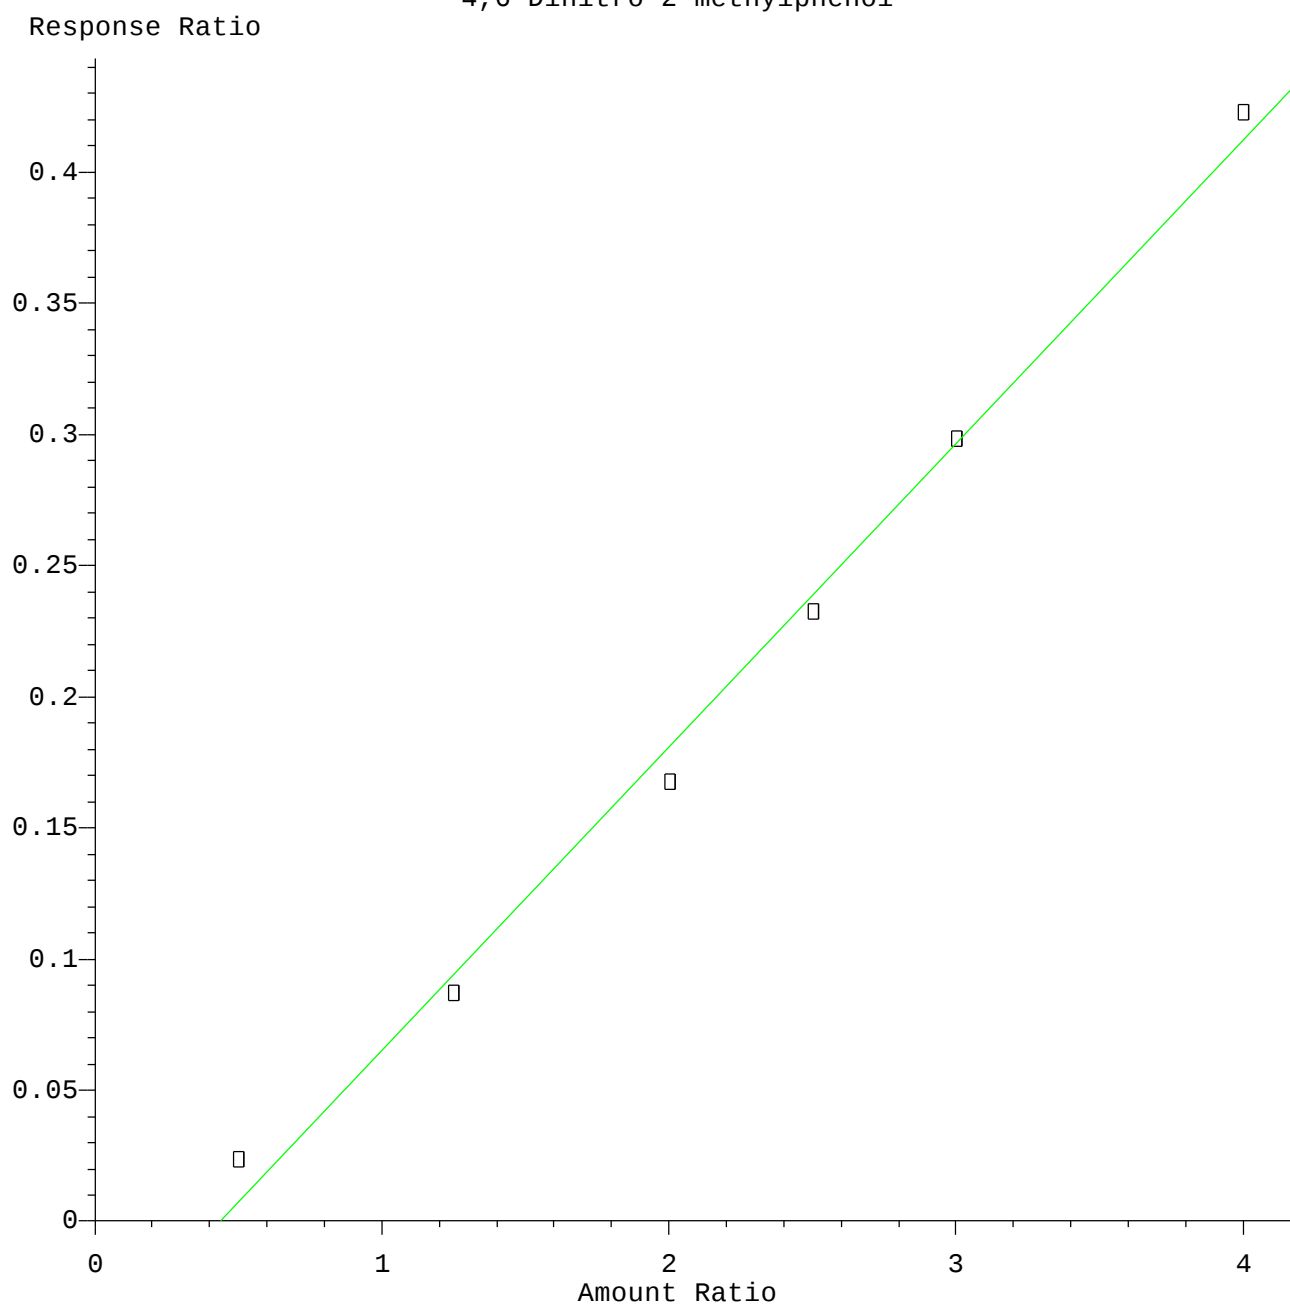


Resp Ratio = $1.16 \times 10^{-1} \times \text{Amt} - 5.04 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018

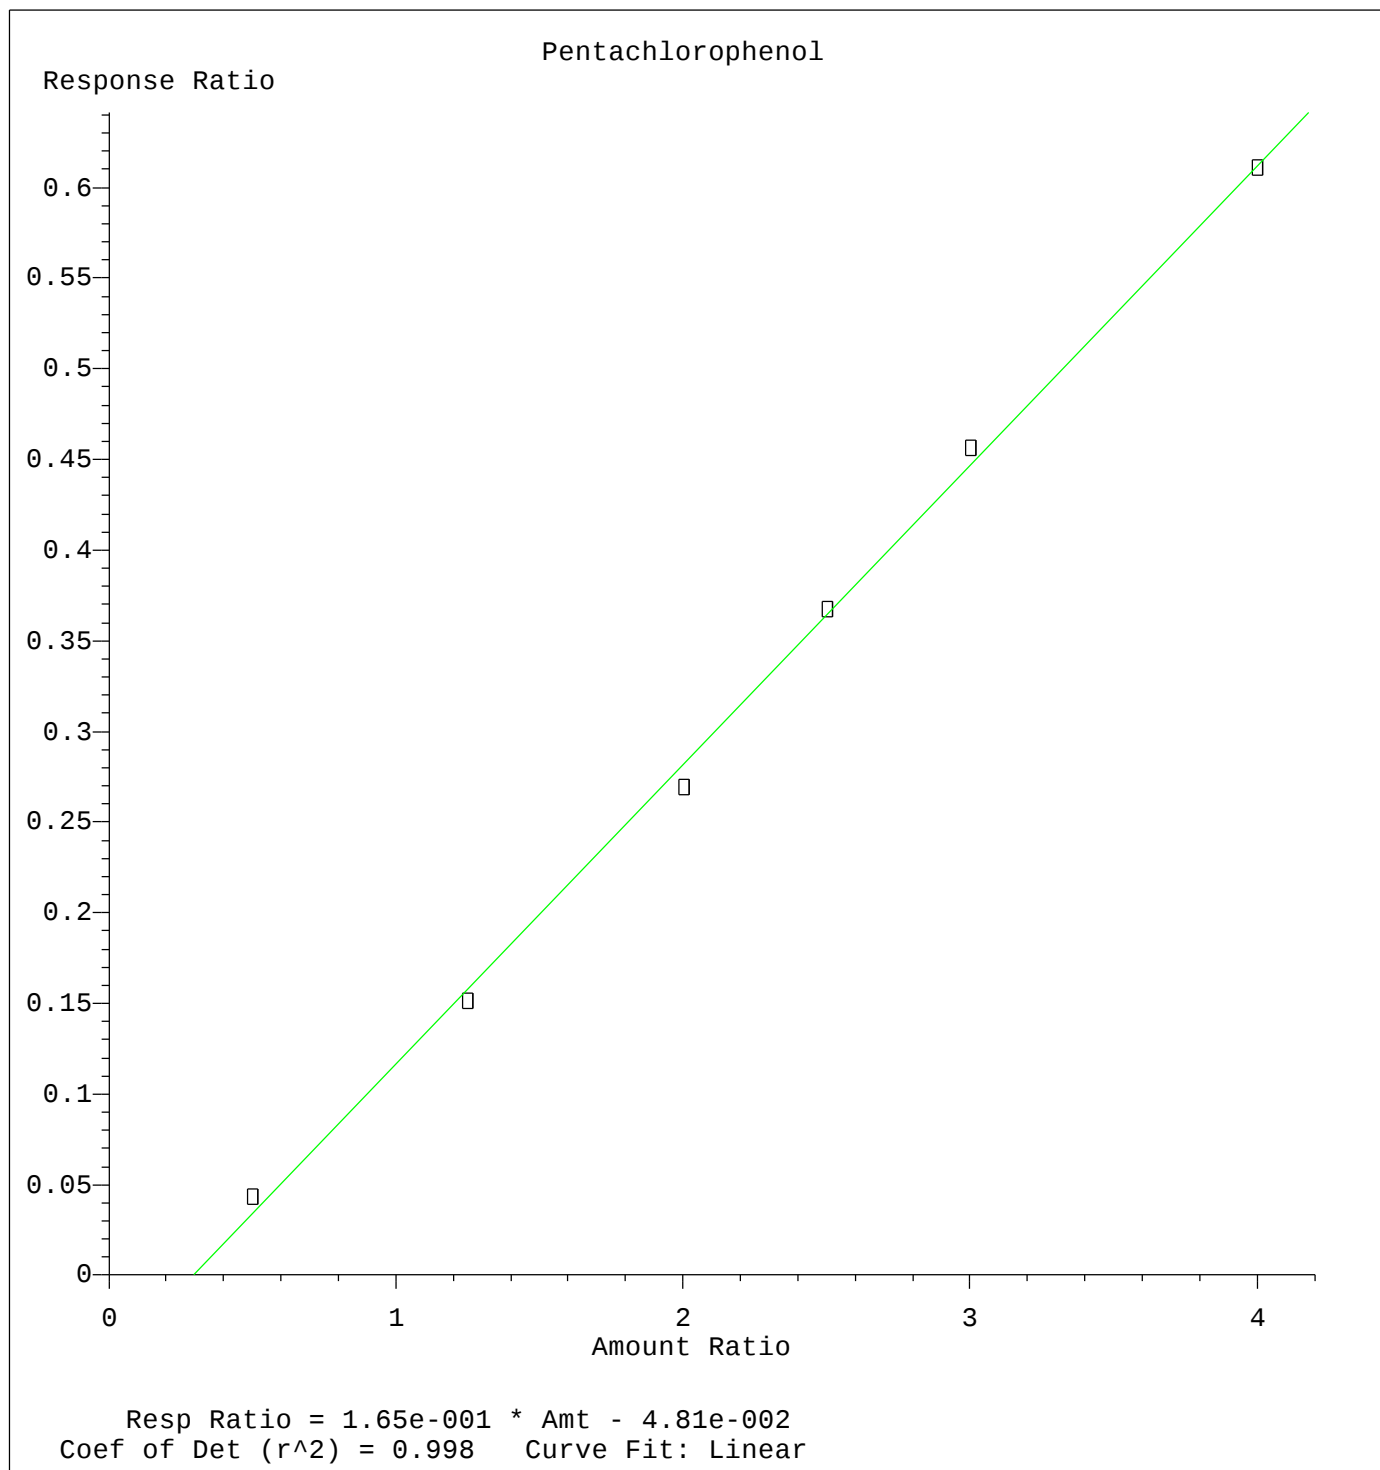


Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018

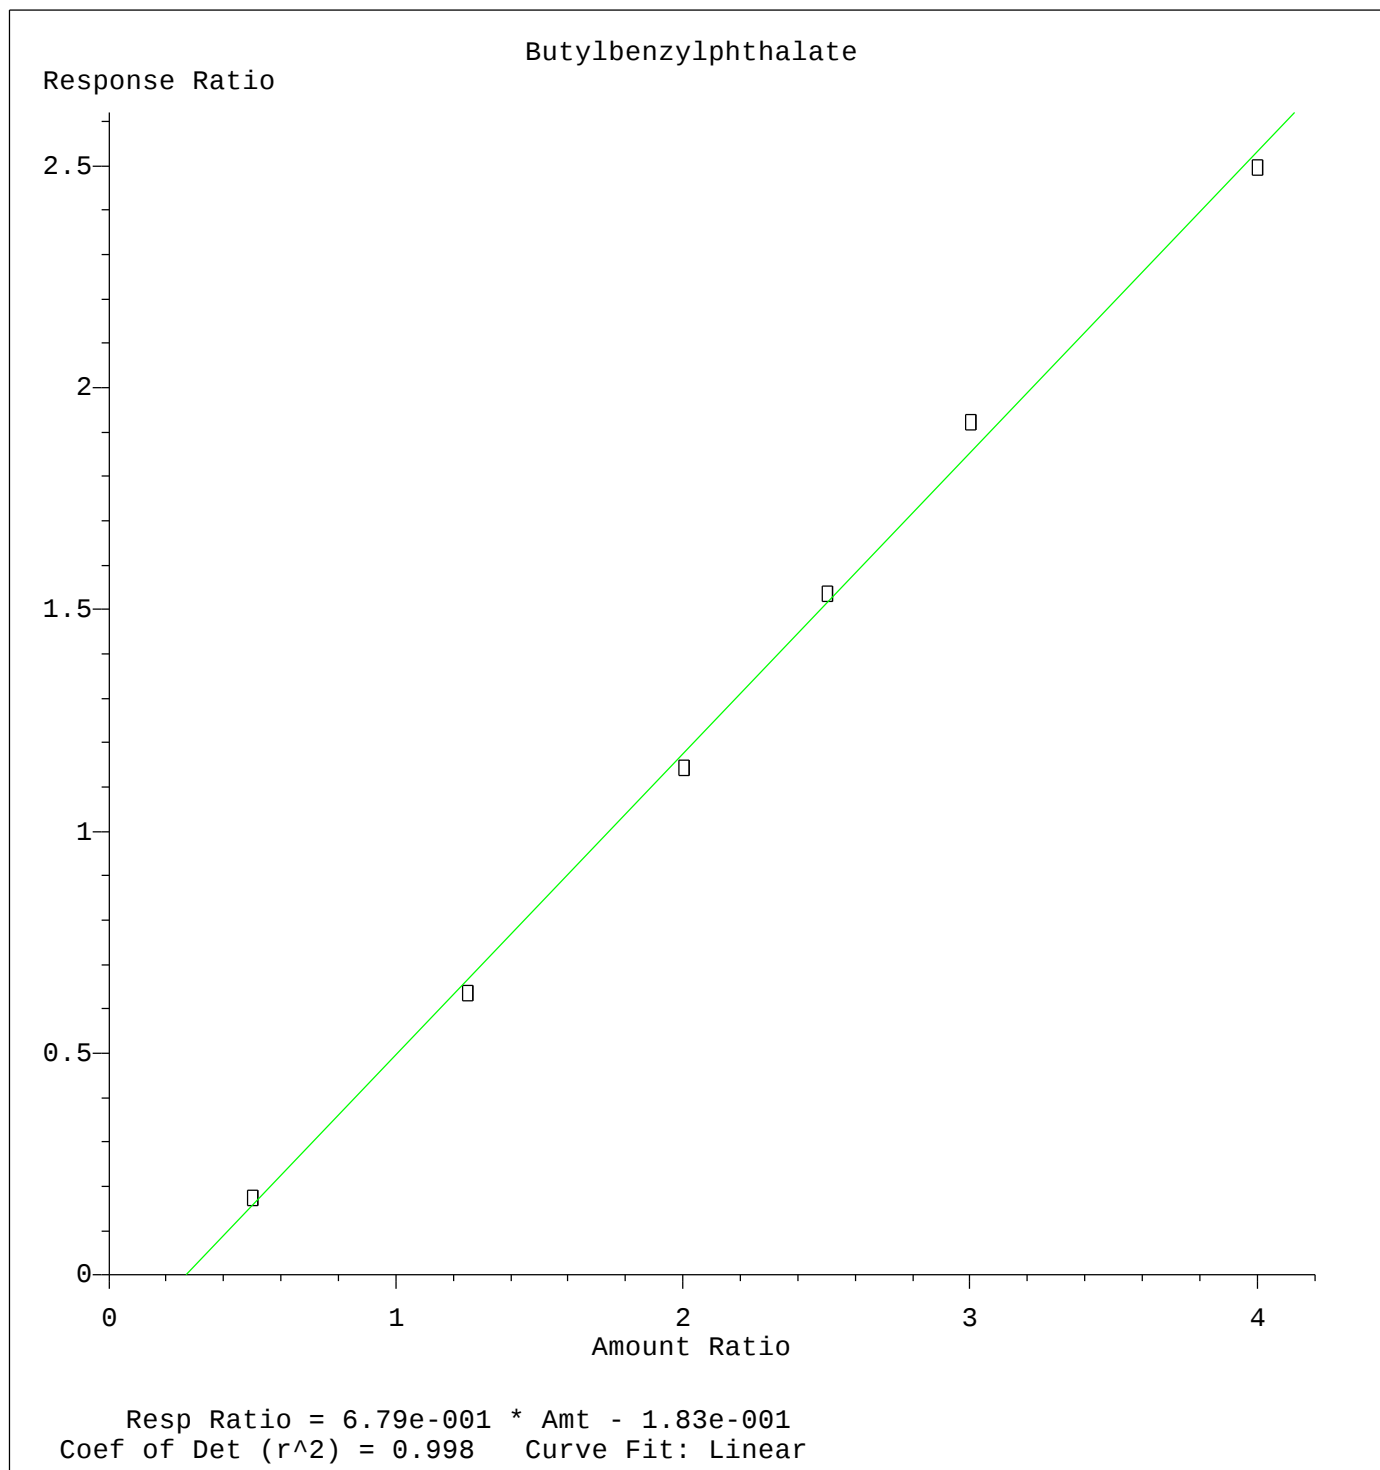

Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018

Bis(2-ethylhexyl)phthalate

Response Ratio

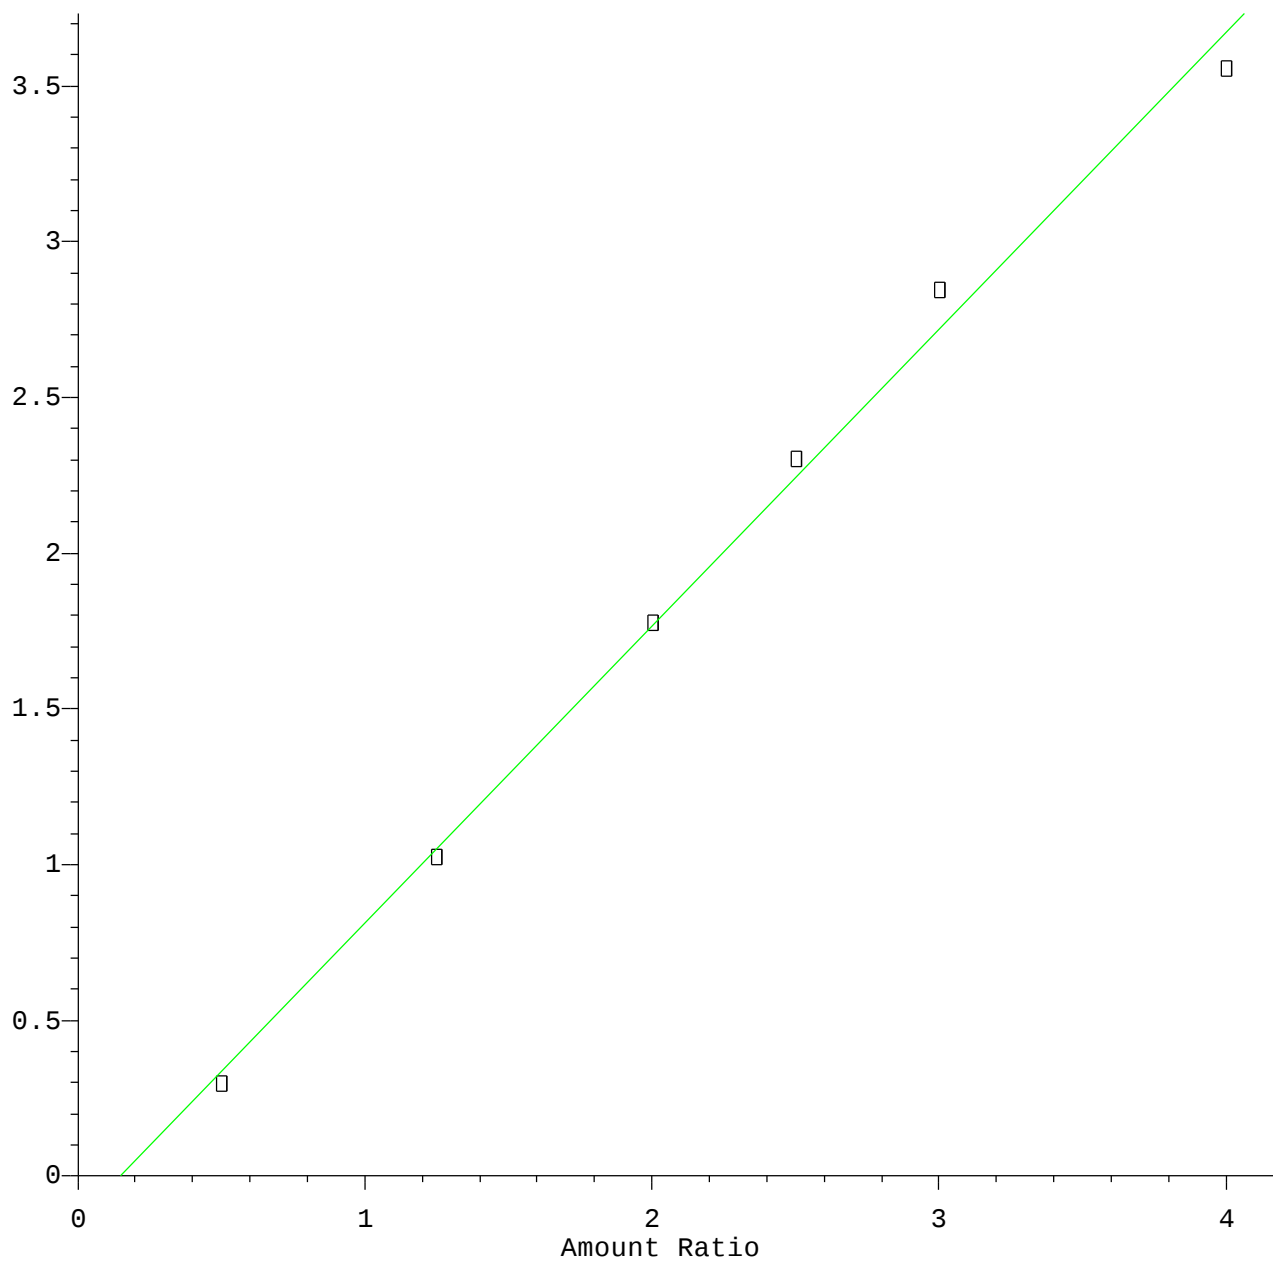

Resp Ratio = $9.52 \times 10^{-1} \times \text{Amt} - 1.38 \times 10^{-1}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Calibration Table Last Updated: Wed Feb 07 18:24:45 2018