
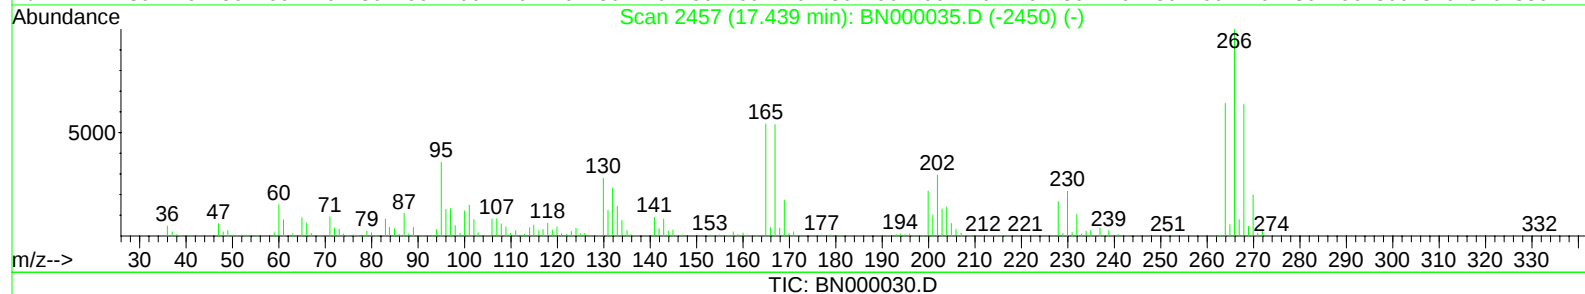
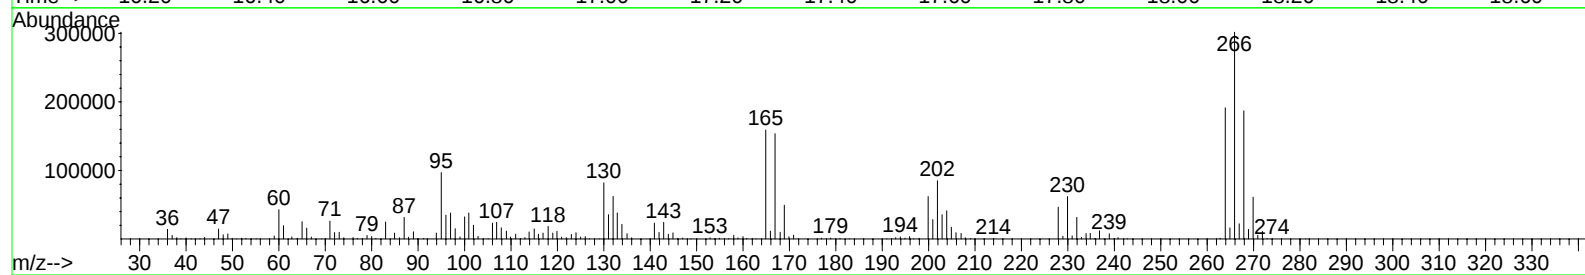


Data Path : Z:\HPCHEM1\BNA N\DATA\BN020718\
Data File : BN000030.D
Acq On : 07 Feb 2018 08:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:51:45 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 18:24:45 2018
Response via : Initial Calibration

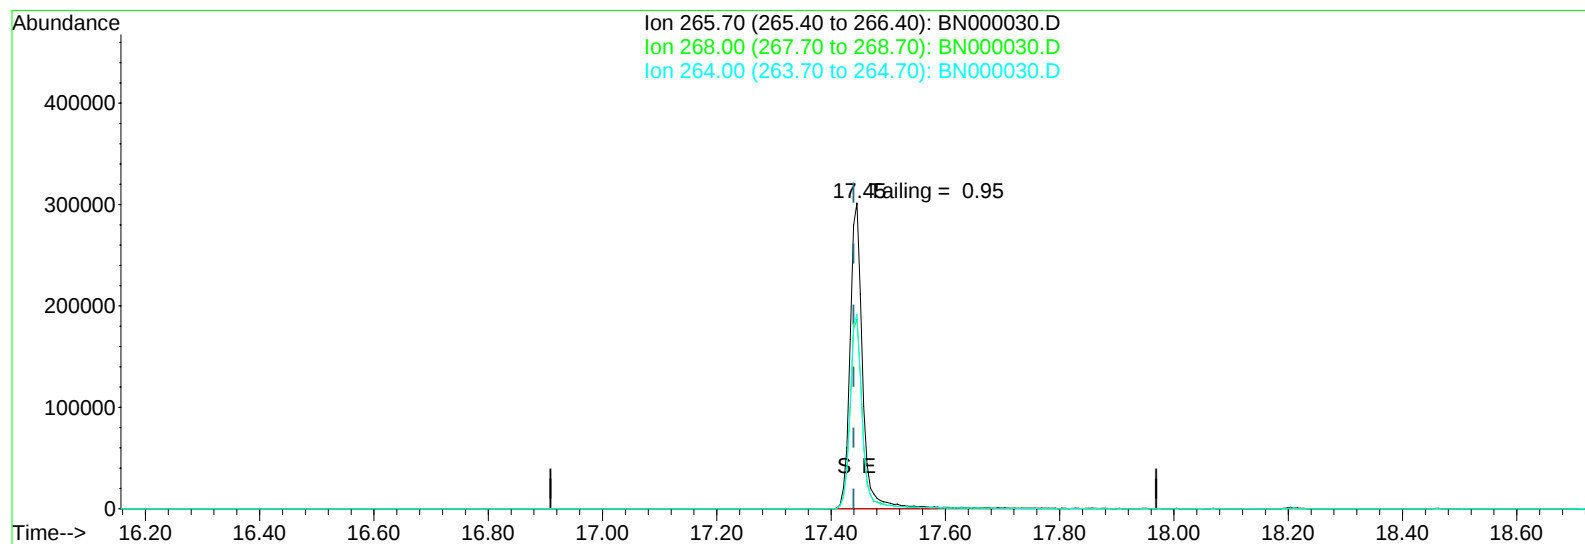

(69) Pentachlorophenol (C)




17.445min (+0.006) 440531.17ng

response 457801

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.00
264.00	62.00	63.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA N\DATA\BN020718\
Data File : BN000030.D
Acq On : 07 Feb 2018 08:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:51:45 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 18:24:45 2018
Response via : Initial Calibration

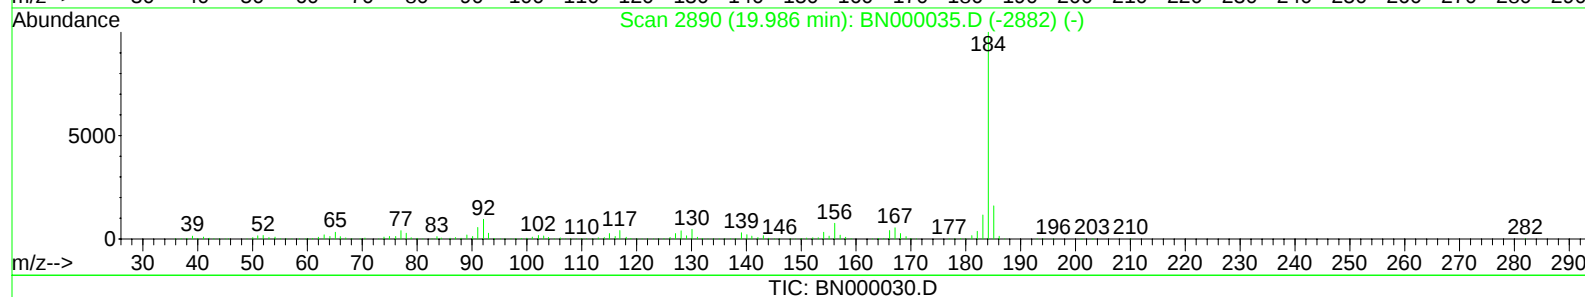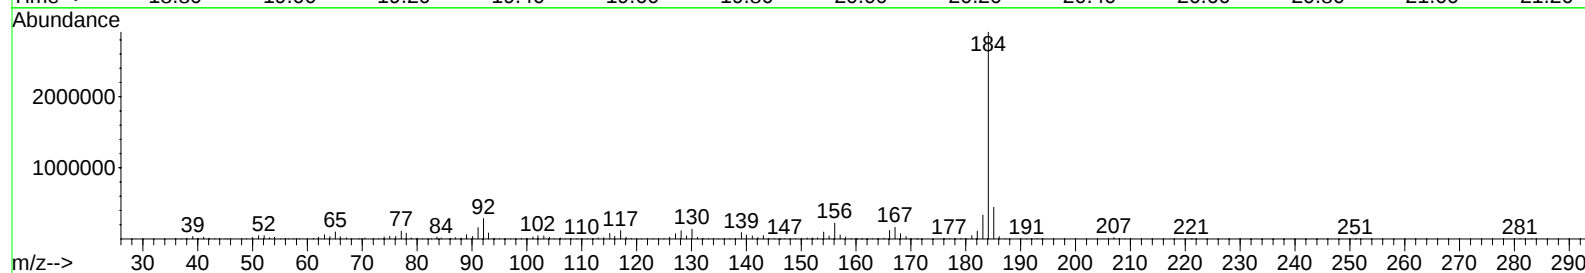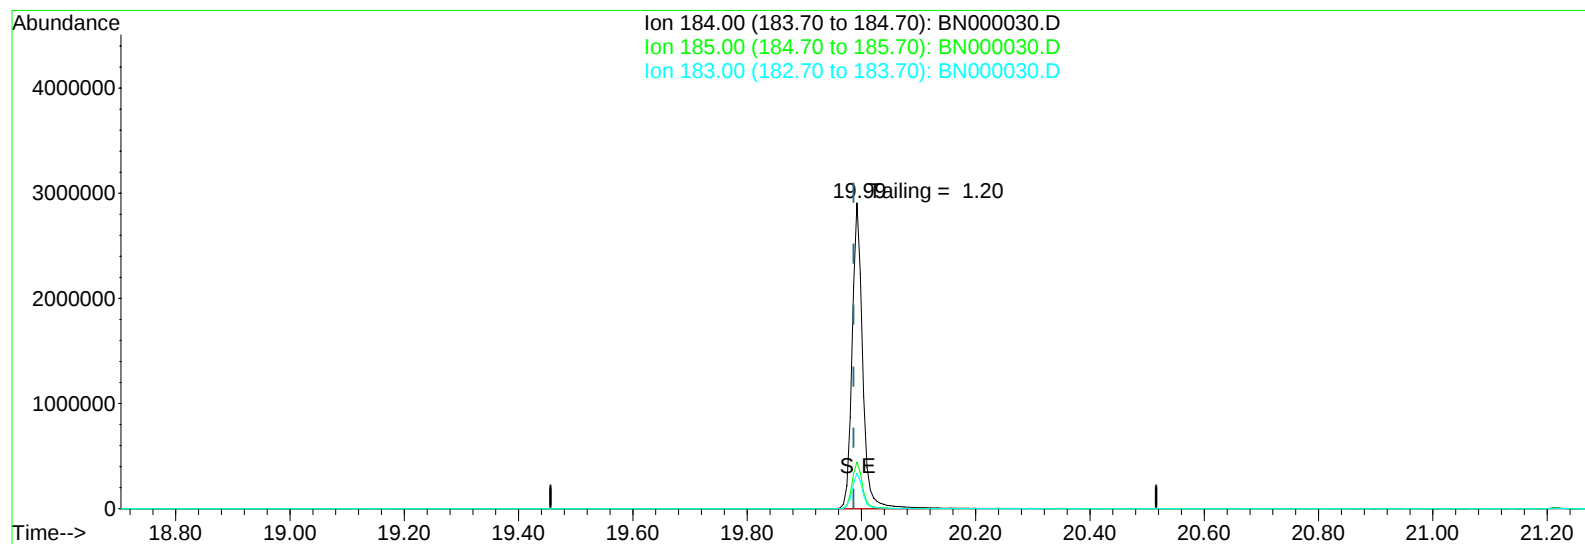

TIC: BN000030.D

(76) Benzidine

19.992min (+0.006) 13384.20ng

response 3723808

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.26
183.00	13.30	11.53
0.00	0.00	0.00