


Data Path : Z:\HPCHEM1\BNA N\DATA\BN020718\
 Data File : BN000030.D
 Acq On : 07 Feb 2018 08:24
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 18:24:45 2018

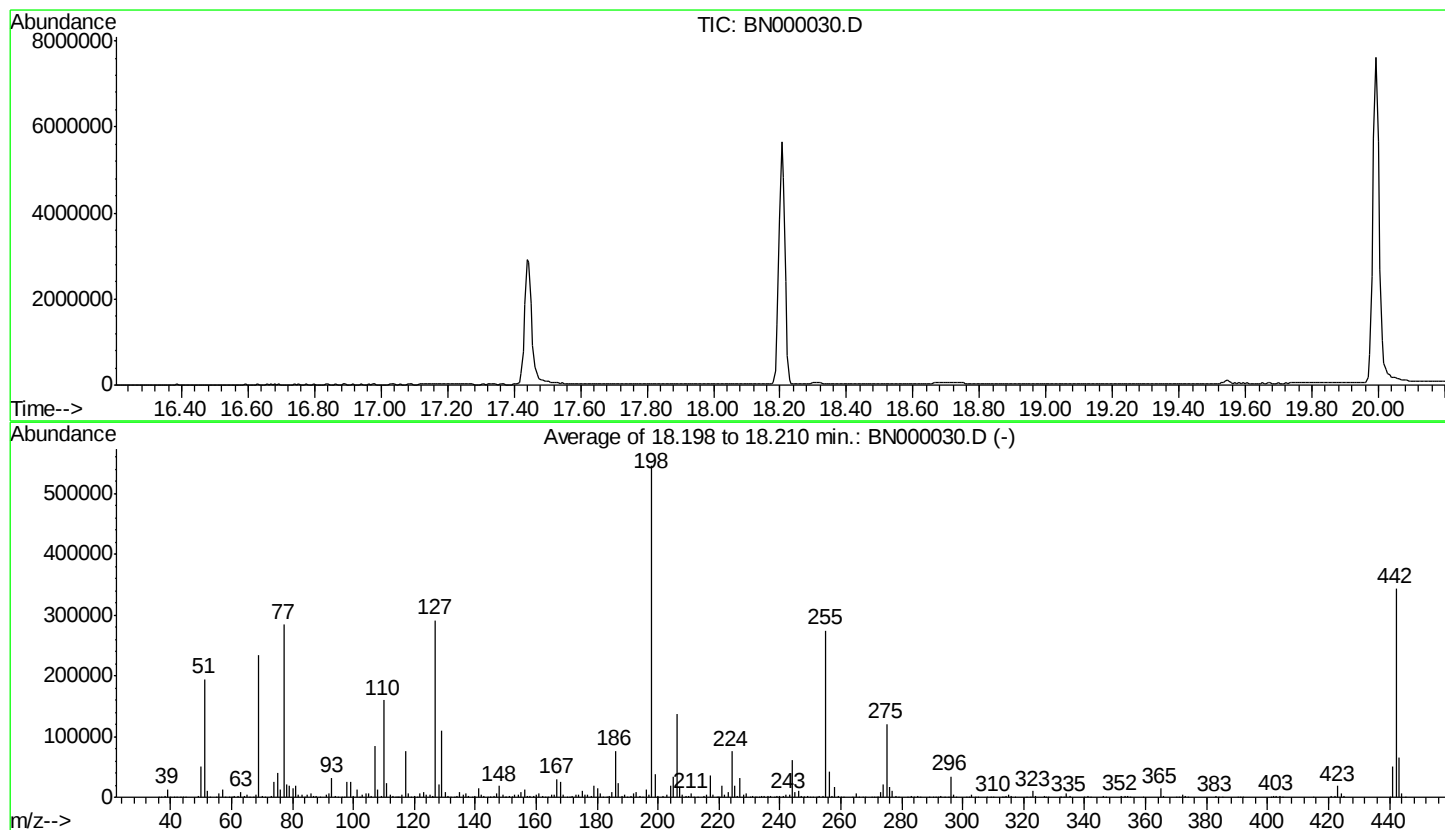

AutoFind: Scans 2586, 2587, 2588; Background Corrected with Scan 2579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	193962	PASS
68	69	0.00	2	1.7	3917	PASS
69	198	0.00	100	42.8	233652	PASS
70	69	0.00	2	0.6	1351	PASS
127	198	10	80	53.3	291221	PASS
197	198	0.00	2	0.6	3466	PASS
198	198	100	100	100.0	545877	PASS
199	198	5	9	7.0	38082	PASS
275	198	10	60	22.0	120149	PASS
365	198	1	100	2.6	13989	PASS
441	443	0.01	100	77.5	51210	PASS
442	198	50	100	62.8	342613	PASS
443	442	15	24	19.3	66120	PASS