


Data Path : Z:\HPCHEM1\BNA N\DATA\BN020718\
 Data File : BN000040.D
 Acq On : 07 Feb 2018 17:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 18:24:45 2018

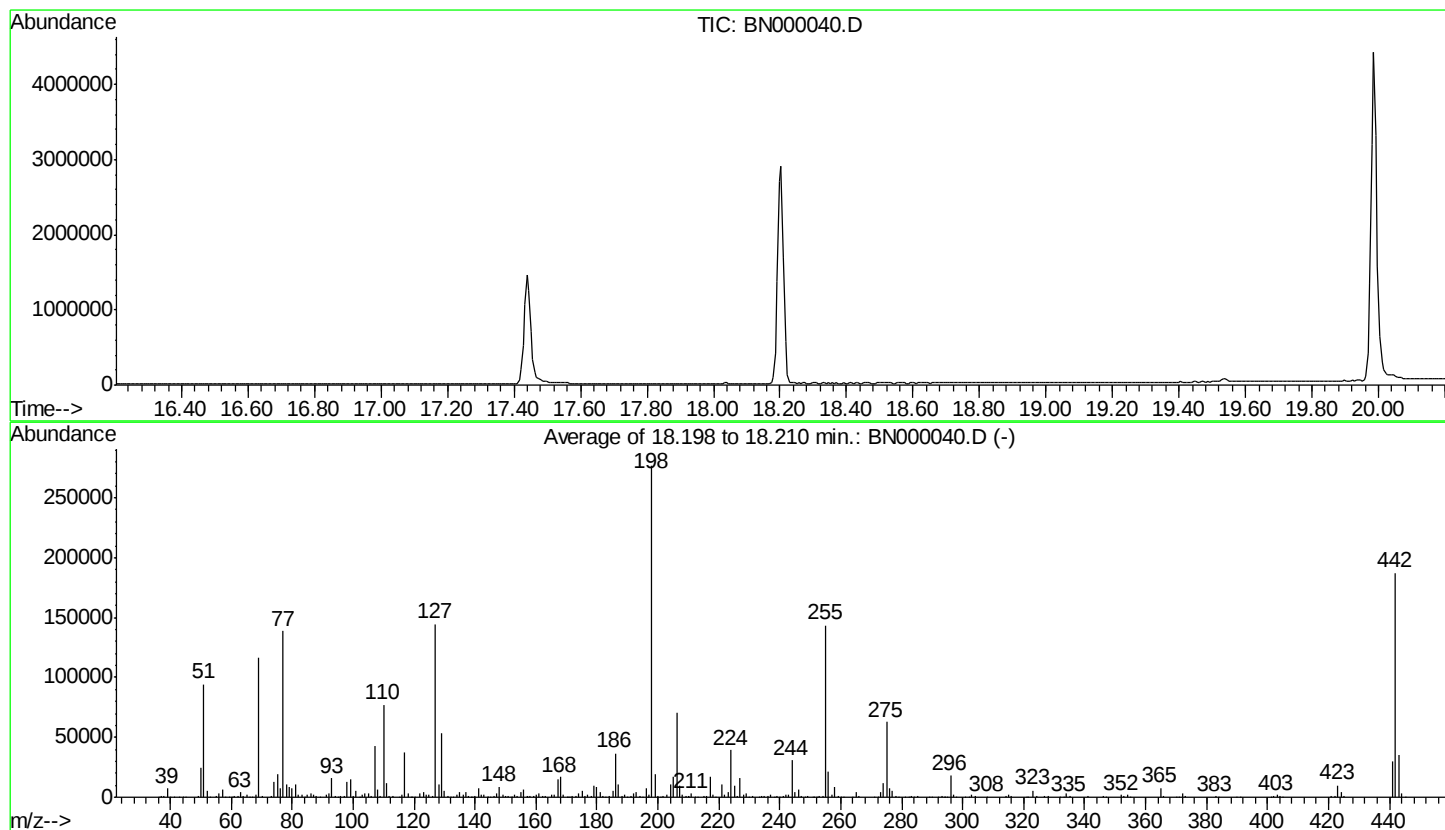

AutoFind: Scans 2586, 2587, 2588; Background Corrected with Scan 2579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	94400	PASS
68	69	0.00	2	1.7	2016	PASS
69	198	0.00	100	42.1	116426	PASS
70	69	0.00	2	0.6	720	PASS
127	198	10	80	52.2	144474	PASS
197	198	0.00	2	0.6	1660	PASS
198	198	100	100	100.0	276821	PASS
199	198	5	9	6.9	19210	PASS
275	198	10	60	22.7	62770	PASS
365	198	1	100	2.8	7808	PASS
441	443	0.01	100	83.9	29589	PASS
442	198	50	100	67.7	187285	PASS
443	442	15	24	18.8	35250	PASS