
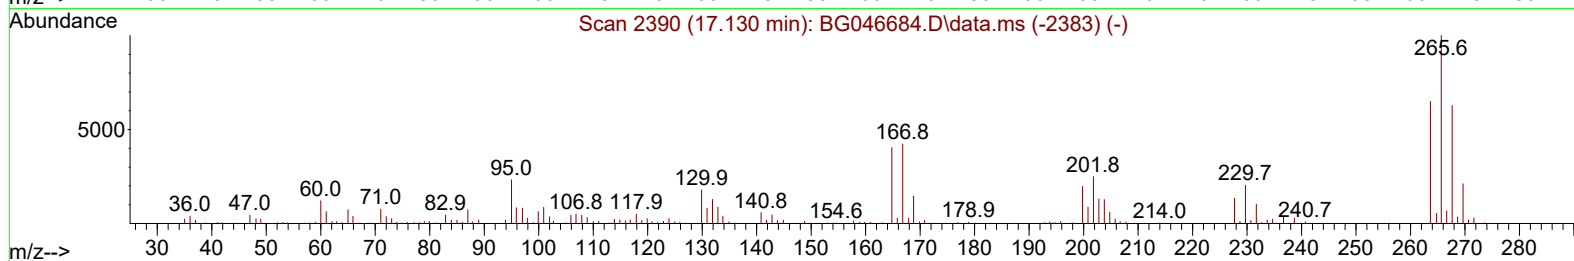
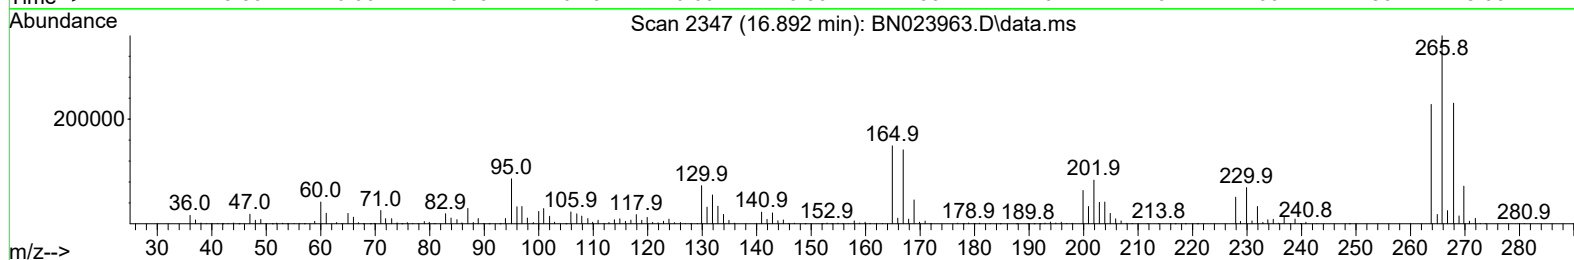


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020723\
 Data File : BN023963.D
 Acq On : 07 Feb 2023 10:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:20:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 08 05:20:21 2023
 Response via : Initial Calibration

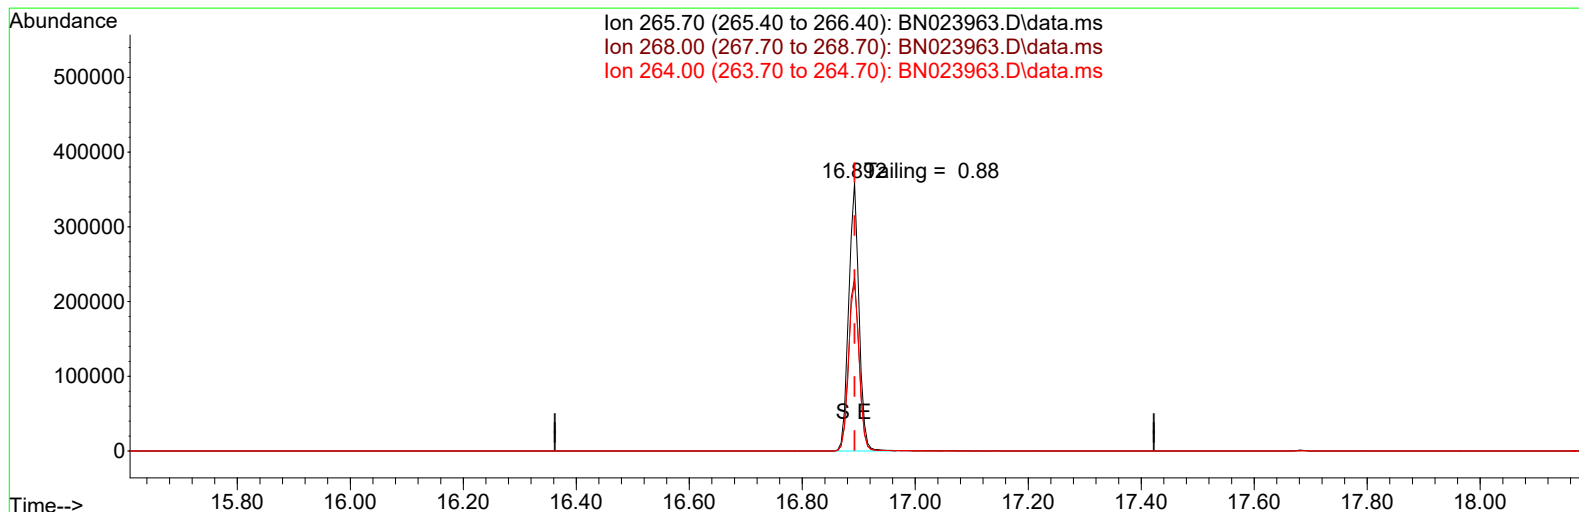

TIC: BN023963.D\data.ms

(70) Pentachlorophenol (C)




16.892min (0.000) 23849.74 ng

response 455751

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.22
264.00	61.60	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020723\
 Data File : BN023963.D
 Acq On : 07 Feb 2023 10:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:20:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 08 05:20:21 2023
 Response via : Initial Calibration

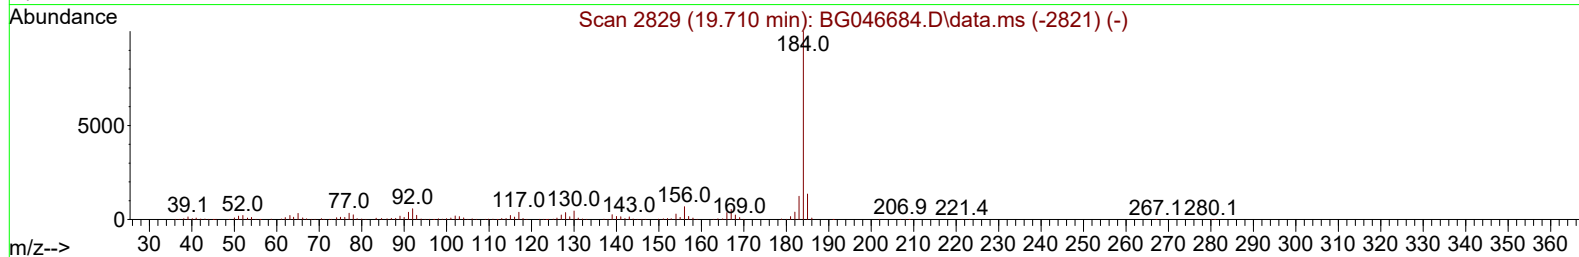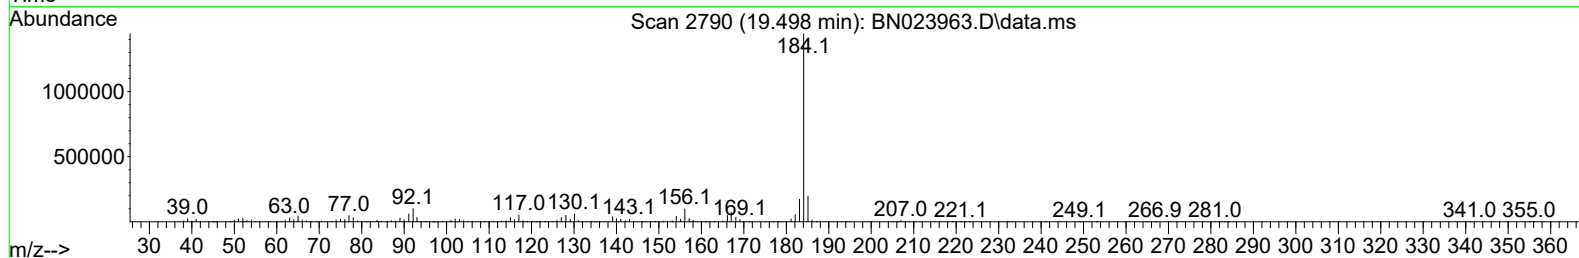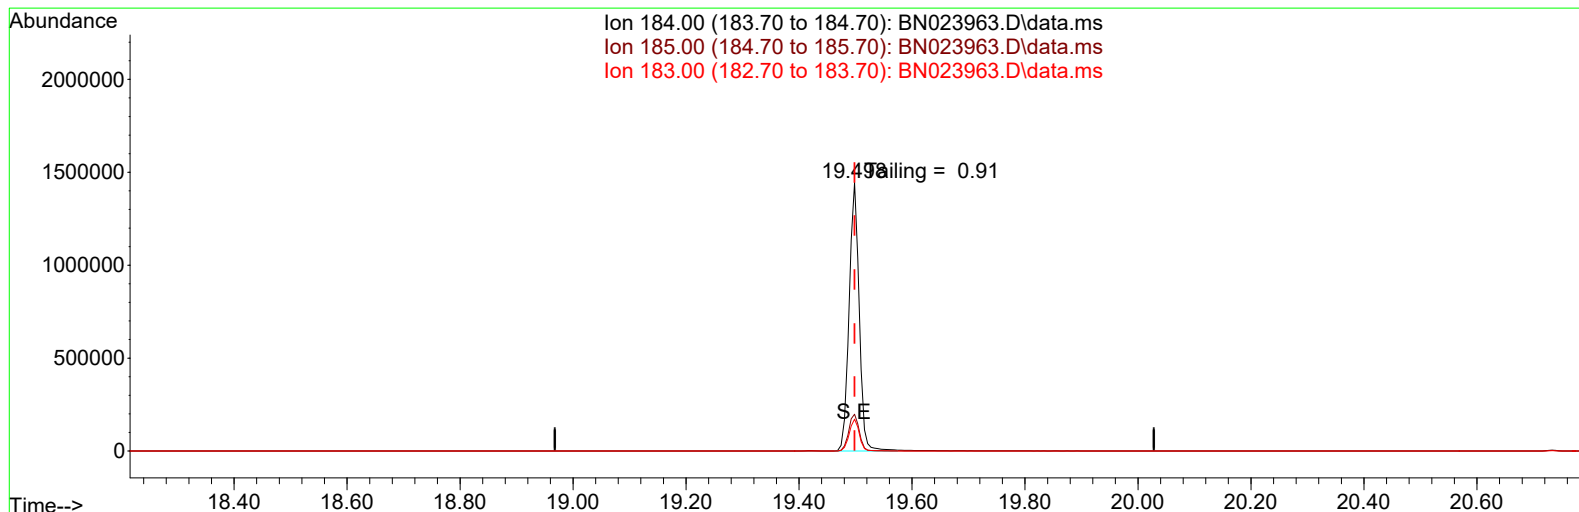

TIC: BN023963.D\data.ms

(77) Benzidine

19.498min (0.000) 201291.43 ng

response 1805621

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.73
183.00	13.20	11.89
0.00	0.00	0.00