
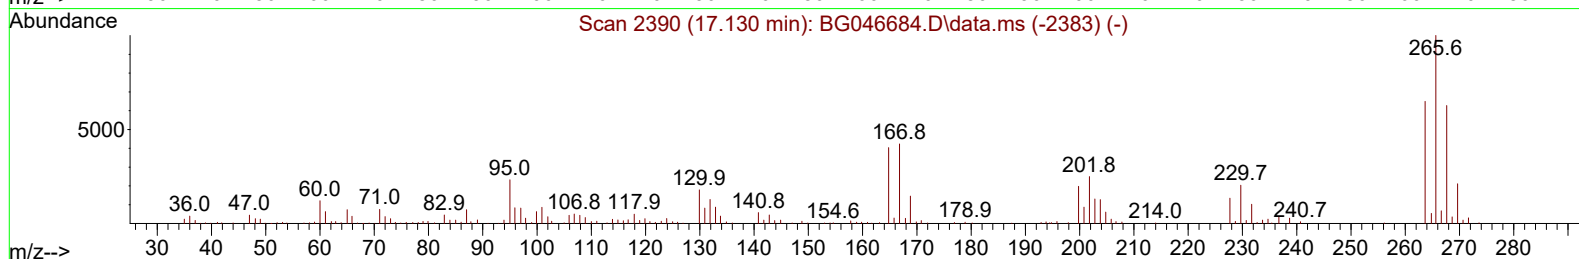
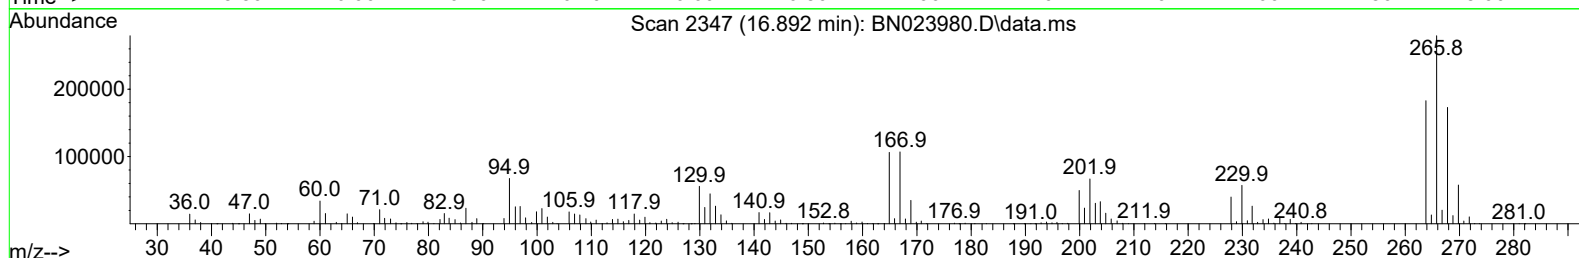


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020723\
Data File : BN023980.D
Acq On : 07 Feb 2023 21:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:21:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 05:20:21 2023
Response via : Initial Calibration

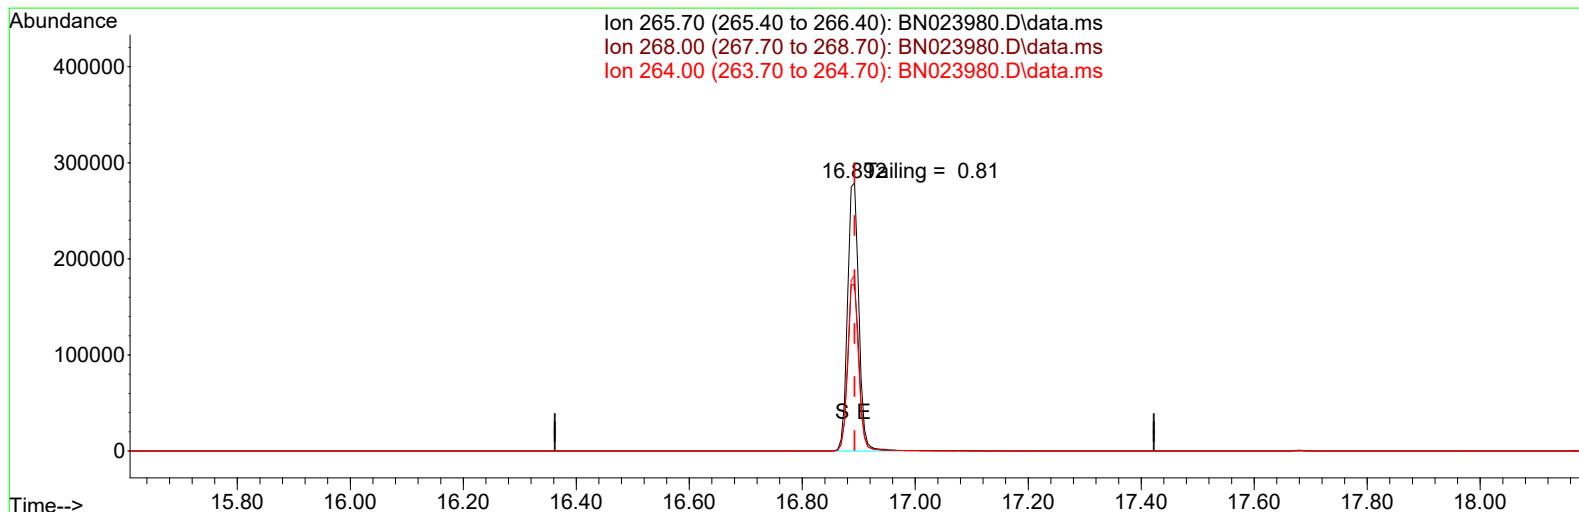

TIC: BN023980.D\data.ms

(70) Pentachlorophenol (C)




16.892min (0.000) 24325.25 ng

response 387333

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.92
264.00	61.60	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020723\
Data File : BN023980.D
Acq On : 07 Feb 2023 21:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:21:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 05:20:21 2023
Response via : Initial Calibration

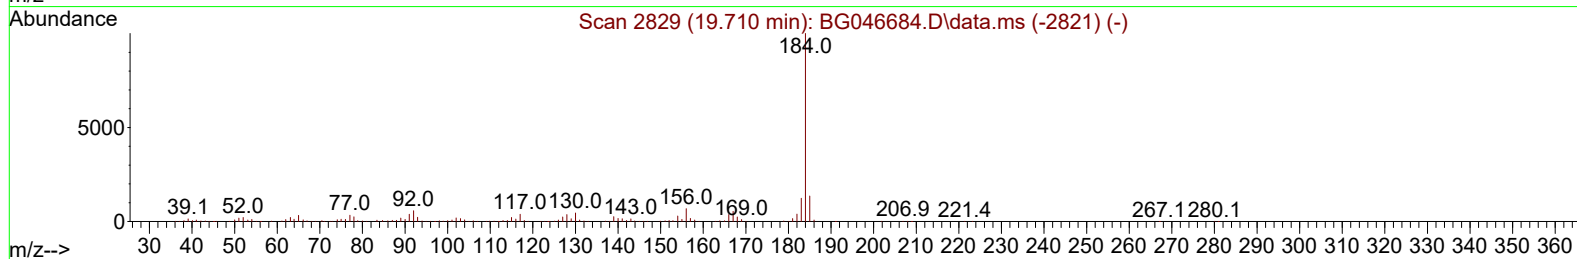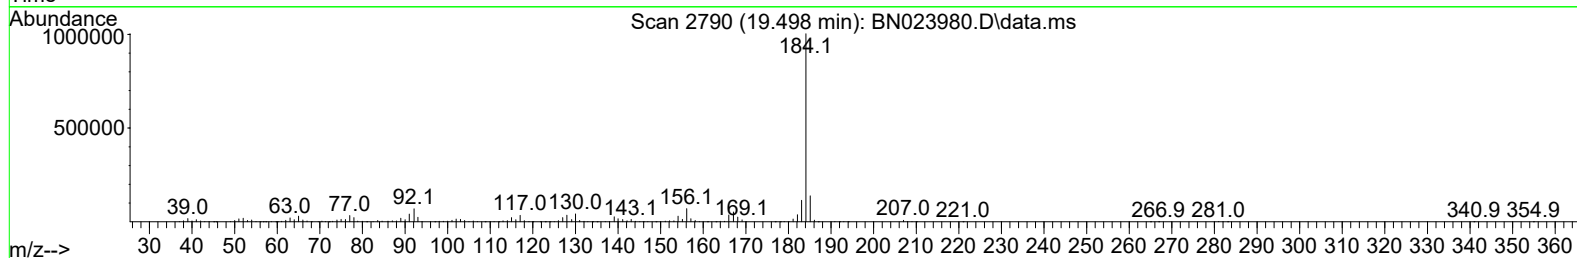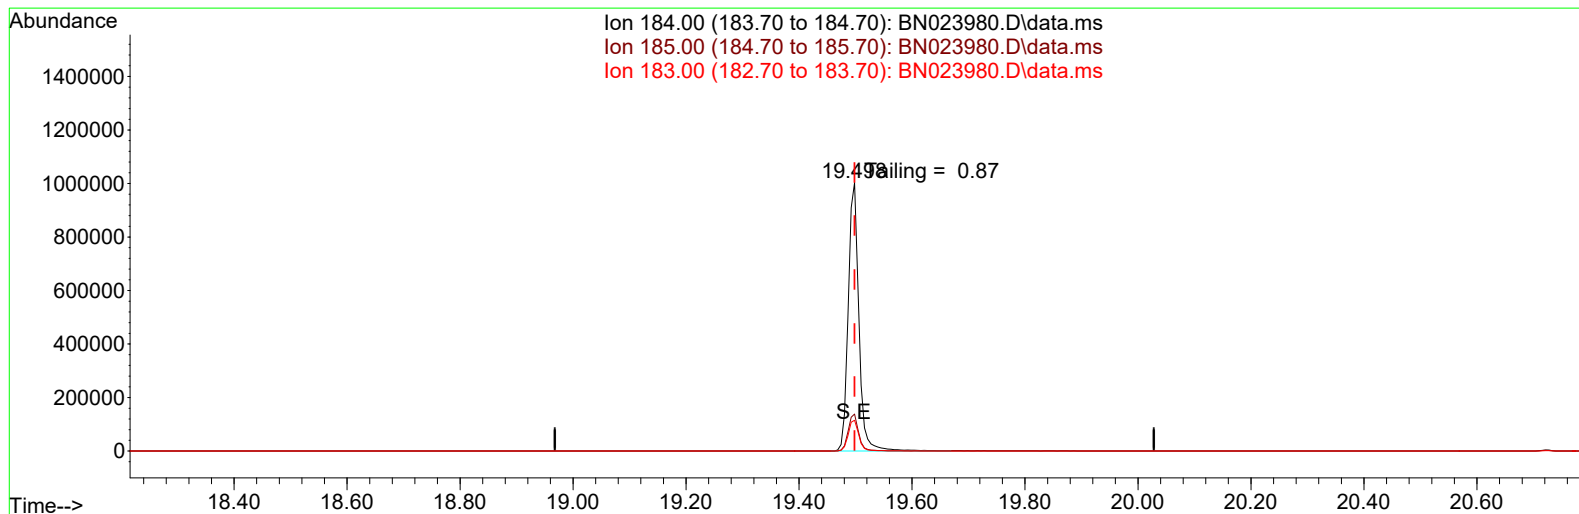

TIC: BN023980.D\data.ms

(77) Benzidine

19.498min (-0.000) 0.00 ng

response 1316435

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.45
0.00	0.00	0.00