
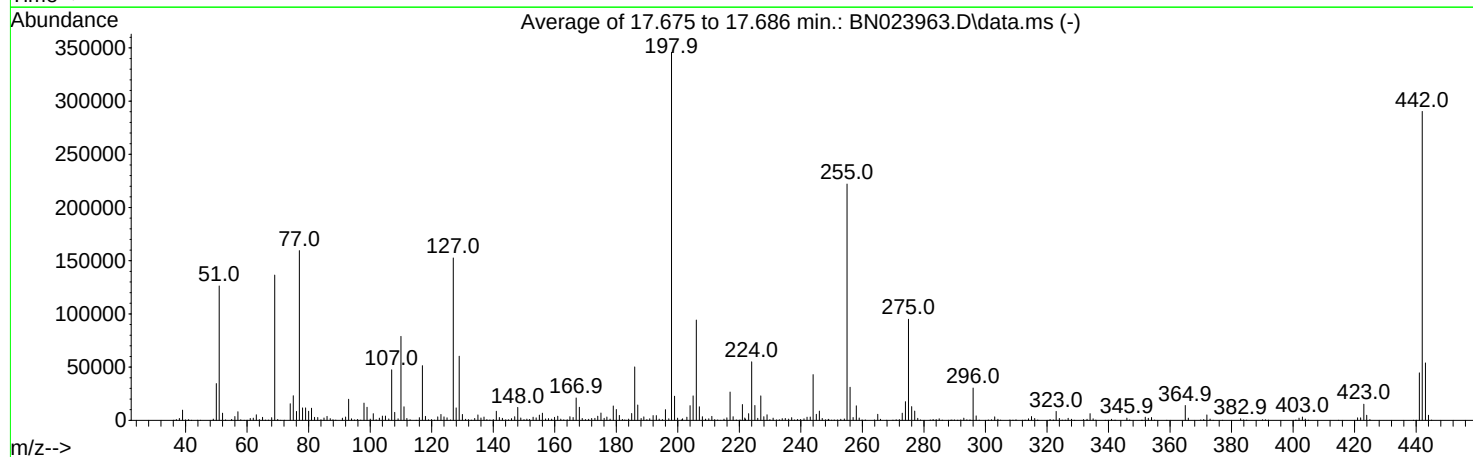


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020723\
Data File : BN023963.D
Acq On : 07 Feb 2023 10:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN020723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 08 02:37:27 2023

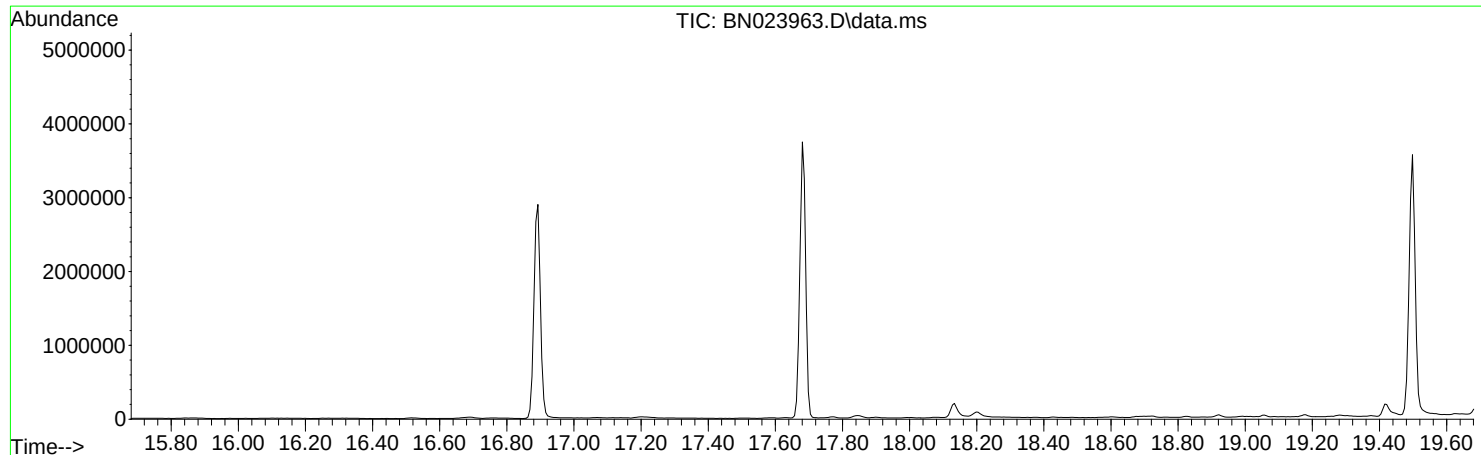




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	126255	PASS
68	69	0.00	2	1.8	2509	PASS
69	198	0.00	100	39.5	136528	PASS
70	69	0.00	2	0.6	845	PASS
127	198	10	80	44.1	152568	PASS
197	198	0.00	2	0.4	1422	PASS
198	198	100	100	100.0	345728	PASS
199	198	5	9	6.6	22656	PASS
275	198	10	60	27.5	94907	PASS
365	198	1	100	4.0	13978	PASS
441	198	0.01	100	12.9	44645	PASS
442	442	50	100	100.0	290325	PASS
443	442	15	24	18.6	53971	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020723\
 Data File : BN023963.D
 Acq On : 07 Feb 2023 10:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Feb 08 05:20:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 08 05:20:21 2023
 Response via : Initial Calibration

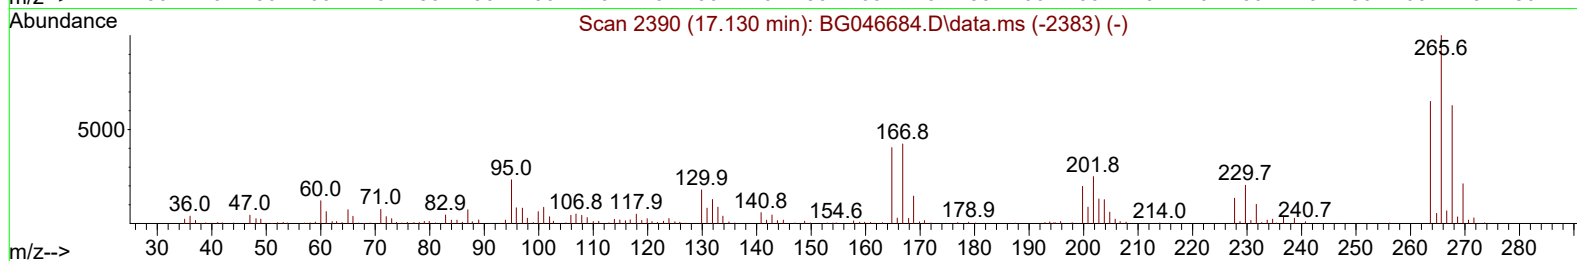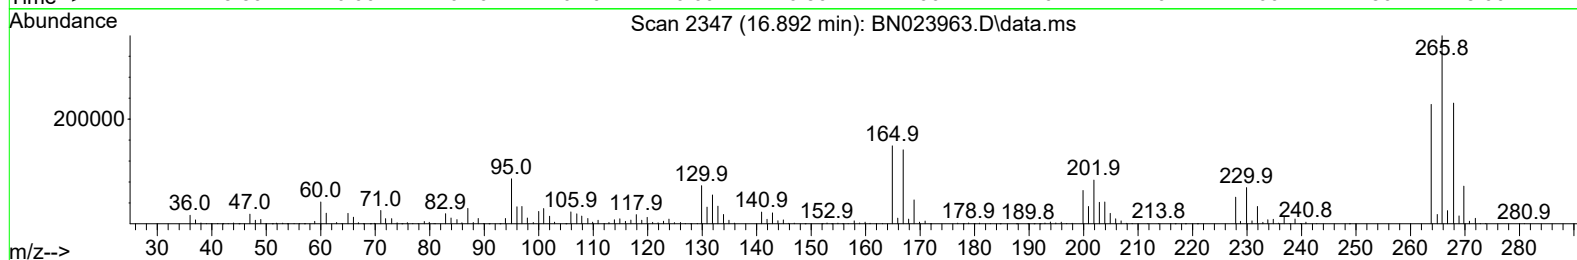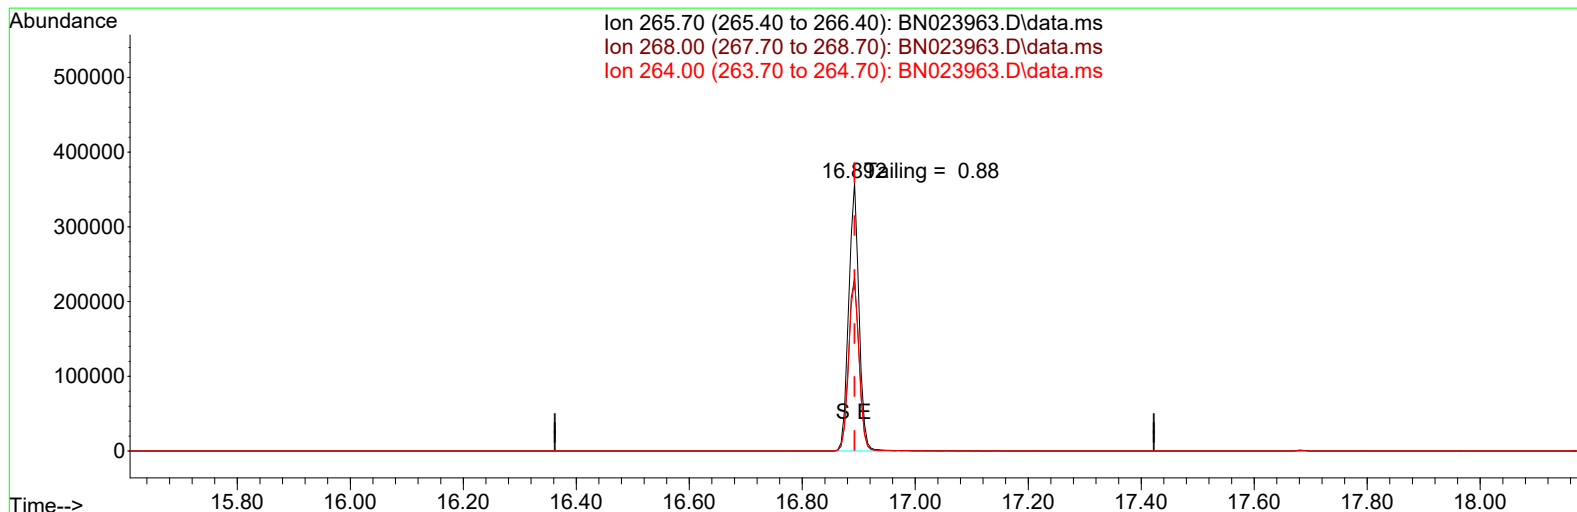

TIC: BN023963.D\data.ms

(70) Pentachlorophenol (C)

16.892min (0.000) 23849.74 ng




response 455751

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.22
264.00	61.60	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020723\
Data File : BN023963.D
Acq On : 07 Feb 2023 10:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 08 05:20:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 05:20:21 2023
Response via : Initial Calibration

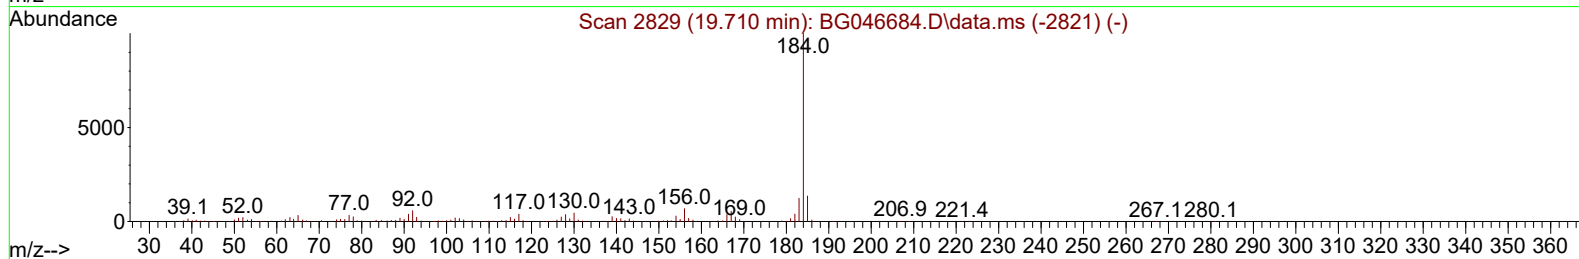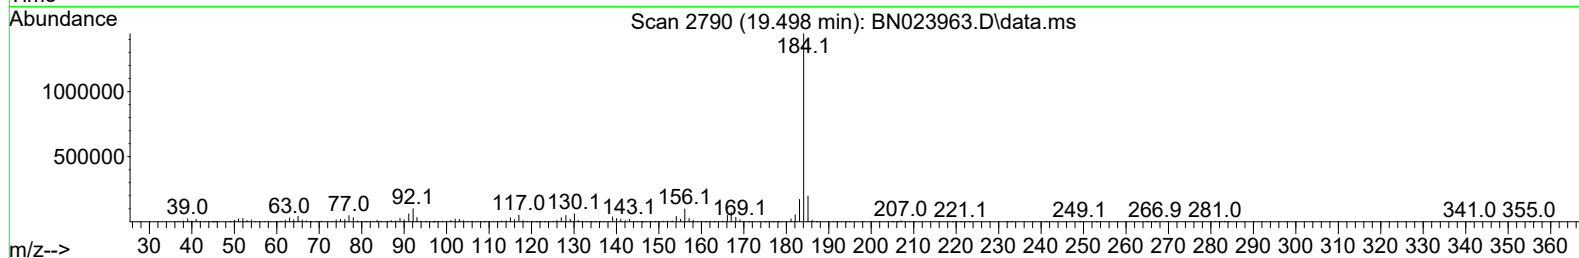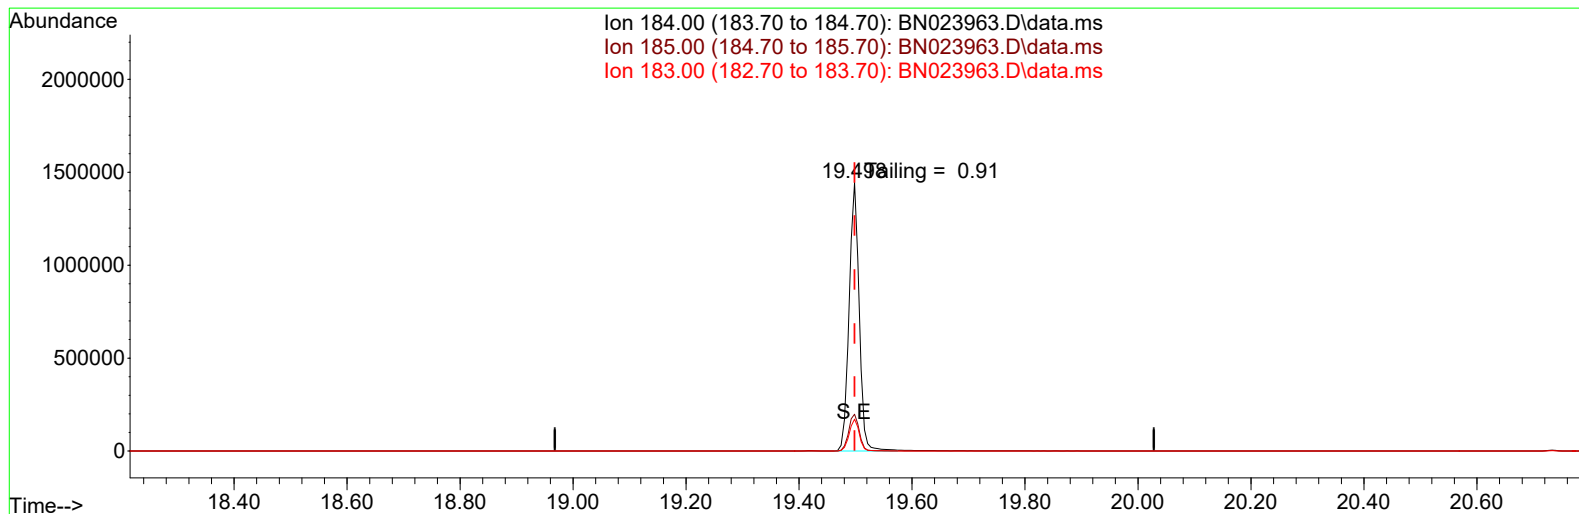

TIC: BN023963.D\data.ms

(77) Benzidine

19.498min (0.000) 201291.43 ng

response 1805621

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.73
183.00	13.20	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/7/2023	BNA_N	<u>BN023963.D</u>
Compound Name	Response	Retention Time
DDT	1092079	20.733
DDD	16814	20.339
DDE	375	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17189	1109268	1.55

Instrument :
BNA_N
ClientSampleId :
DFTPP