
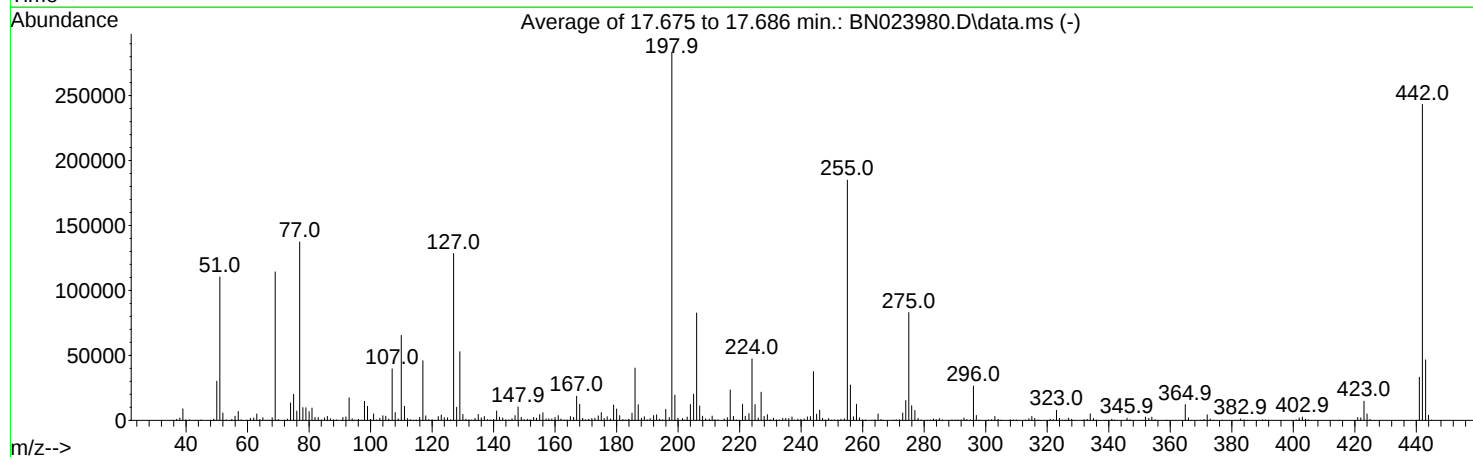


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020723\
Data File : BN023980.D
Acq On : 07 Feb 2023 21:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN020723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 08 02:37:27 2023

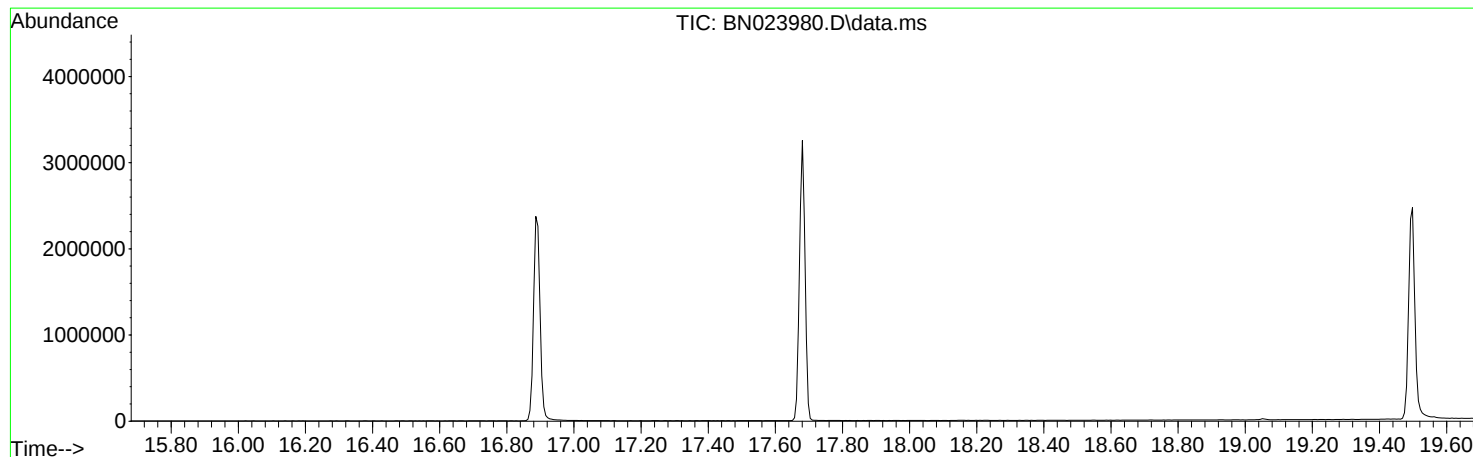




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	110275	PASS
68	69	0.00	2	1.8	2041	PASS
69	198	0.00	100	40.3	114253	PASS
70	69	0.00	2	0.6	680	PASS
127	198	10	80	45.3	128437	PASS
197	198	0.00	2	0.7	2122	PASS
198	198	100	100	100.0	283243	PASS
199	198	5	9	6.9	19464	PASS
275	198	10	60	29.3	82941	PASS
365	198	1	100	4.3	12159	PASS
441	198	0.01	100	11.7	33240	PASS
442	442	50	100	100.0	243200	PASS
443	442	15	24	19.1	46464	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020723\
Data File : BN023980.D
Acq On : 07 Feb 2023 21:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 08 05:21:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 05:20:21 2023
Response via : Initial Calibration

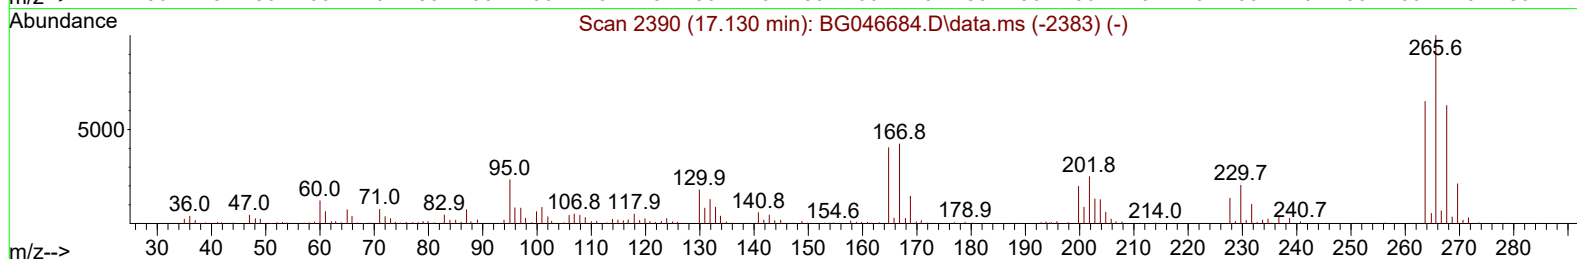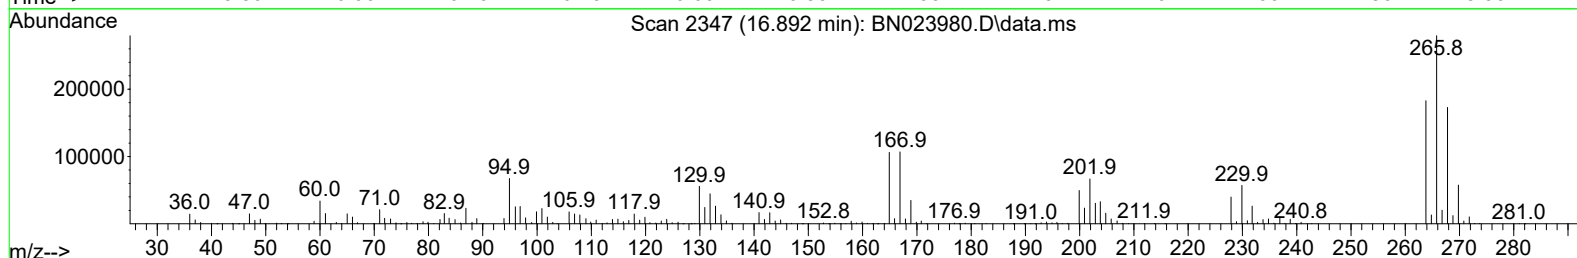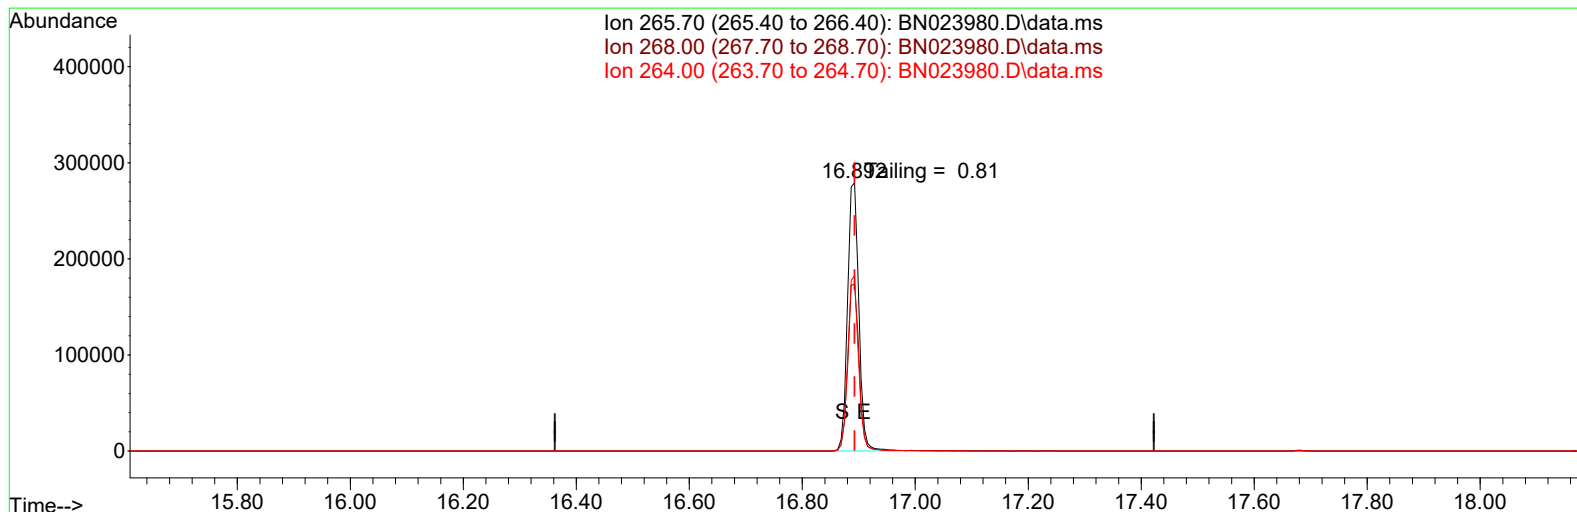

TIC: BN023980.D\data.ms

(70) Pentachlorophenol (C)

16.892min (0.000) 24325.25 ng




response 387333

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.92
264.00	61.60	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020723\
Data File : BN023980.D
Acq On : 07 Feb 2023 21:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 08 05:21:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 05:20:21 2023
Response via : Initial Calibration

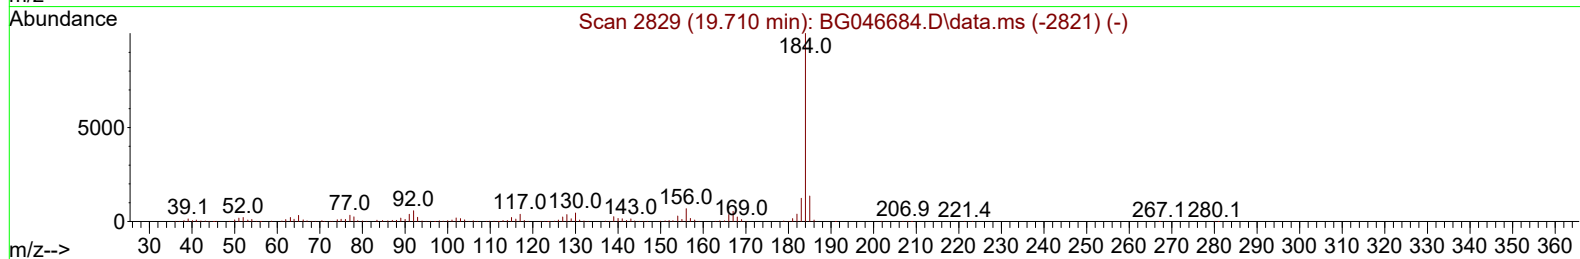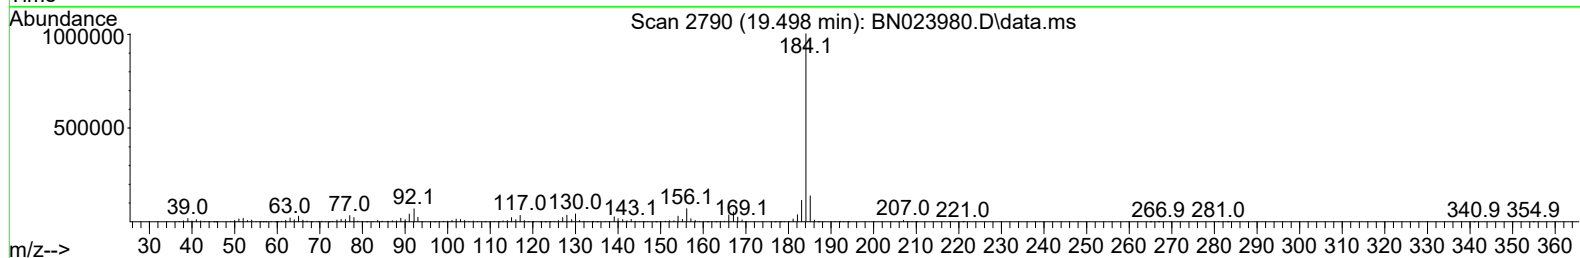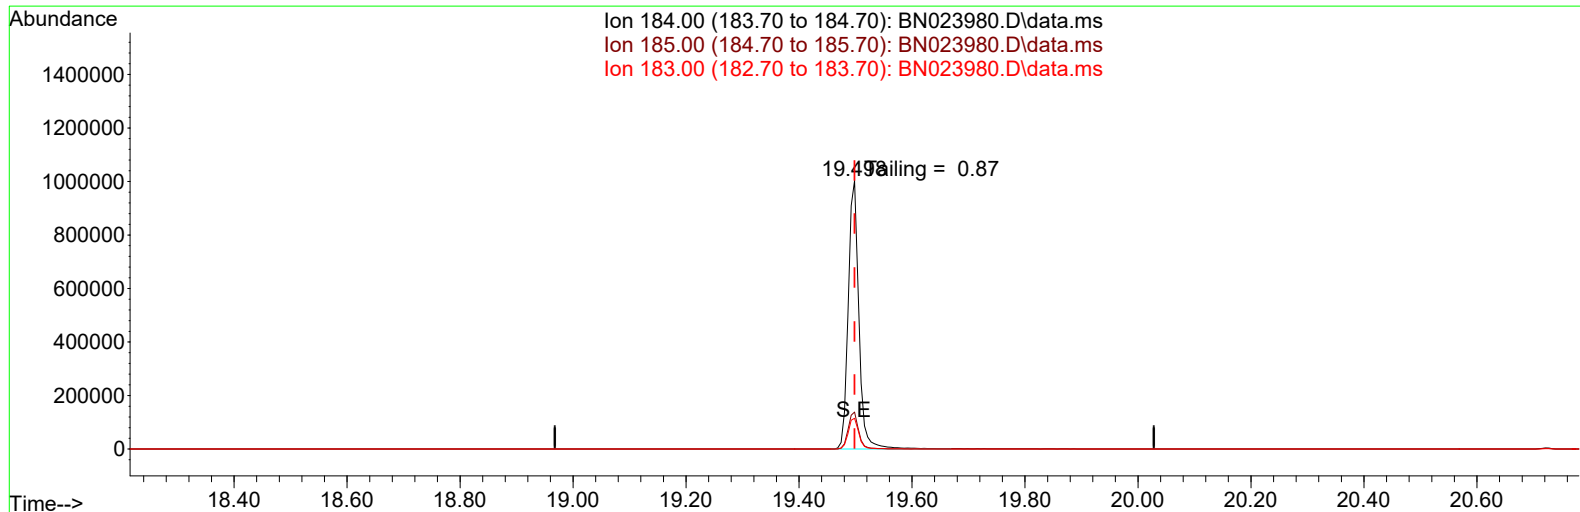

TIC: BN023980.D\data.ms

(77) Benzidine

19.498min (-0.000) 0.00 ng

response 1316435

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/7/2023	BNA_N	<u>BN023980.D</u>
Compound Name	Response	Retention Time
DDT	934781	20.722
DDD	11407	20.333
DDE	434	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11841	946622	1.25

Instrument :
BNA_N
ClientSampleId :
DFTPP