

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
 Data File : BN029549.D
 Acq On : 07 Feb 2024 16:53
 Operator : MA/JU
 Sample : P1303-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FH2

Quant Time: Feb 08 00:50:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	186710	20.000	ng/ul	0.00
20) Naphthalene-d8	10.687	136	758123	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	386214	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.280	188	754704	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	643989	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264	725244	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	29652	5.224	ng/uL	0.00
4) Pyridine-d5	3.740	84	370062	24.445	ng/ul	0.00
7) Phenol-d5	7.046	99	454878	26.047	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	316779	27.179	ng/ul	0.00
11) 2-Chlorophenol-d4	7.410	132	349576	27.623	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	338081	25.958	ng/ul	0.00
21) Nitrobenzene-d5	9.051	128	164423	27.944	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	148036	28.888	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.304	165	281260	27.806	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	455075	26.371	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	831290	28.910	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	986556	28.891	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	115040	21.079	ng/ul	0.00
60) Fluorene-d10	15.522	176	711843	29.101	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	71753	19.512	ng/ul	0.00
73) Anthracene-d10	17.380	188	998193	28.222	ng/ul	0.00
81) Pyrene-d10	19.674	212	1133023	29.318	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1025155	28.249	ng/ul	0.00
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	13.951	165	5638	1.070	ng/ul#	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
Data File : BN029549.D
Acq On : 07 Feb 2024 16:53
Operator : MA/JU
Sample : P1303-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FH2

Quant Time: Feb 08 00:50:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

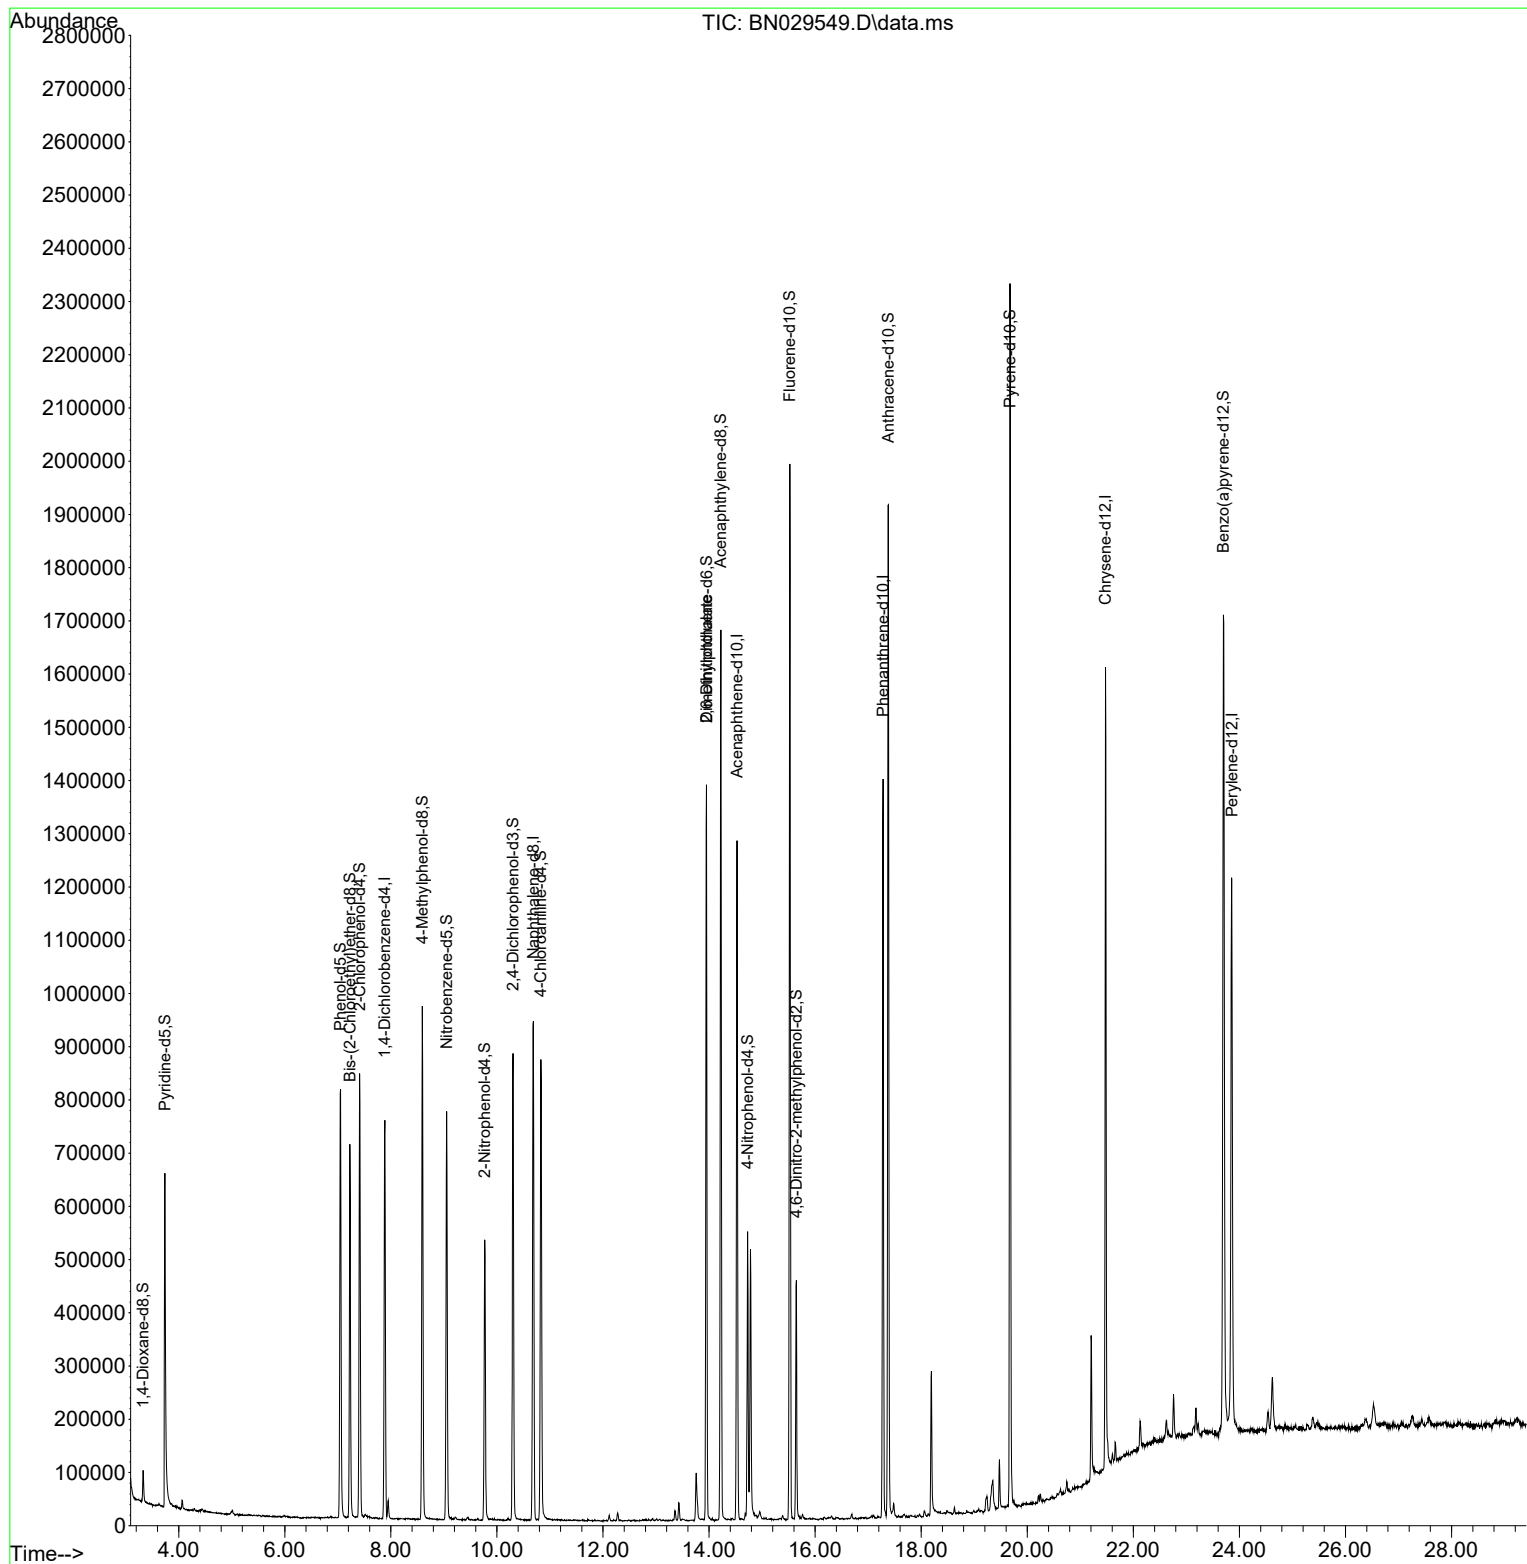

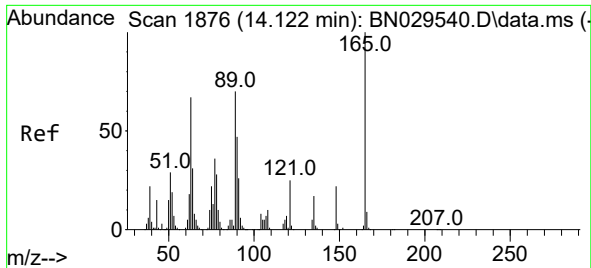

#48
 2,6-Dinitrotoluene
 Concen: 1.070 ng/ul
 RT: 13.951 min Scan# 11
 Delta R.T. -0.171 min
 Lab File: BN029549.D
 Acq: 07 Feb 2024 16:53

Instrument :
 BNA_N
 ClientSampleId :
 C0FH2

Tgt Ion:165 Resp: 5638
 Ion Ratio Lower Upper
 165 100
 89 0.0 55.8 83.8#
 121 45.6 19.8 29.6#

