

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
 Data File : BN029552.D
 Acq On : 07 Feb 2024 18:40
 Operator : MA/JU
 Sample : P1303-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FJ2

Quant Time: Feb 08 00:50:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	191398	20.000	ng/ul	0.00
20) Naphthalene-d8	10.681	136	782329	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.527	164	401742	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.280	188	779914	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	641250	20.000	ng/ul	0.00
88) Perylene-d12	23.850	264	732254	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	26544	4.562	ng/uL	0.00
4) Pyridine-d5	3.740	84	326694	21.052	ng/ul	0.00
7) Phenol-d5	7.045	99	433241	24.200	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	296787	24.840	ng/ul	0.00
11) 2-Chlorophenol-d4	7.410	132	328170	25.296	ng/ul	0.00
15) 4-Methylphenol-d8	8.592	113	326857	24.481	ng/ul	0.00
21) Nitrobenzene-d5	9.051	128	155975	25.688	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	134360	25.408	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.304	165	267366	25.615	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	434821	24.418	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	825032	27.584	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	980225	27.596	ng/ul	0.00
54) 4-Nitrophenol-d4	14.727	143	110216	19.415	ng/ul	0.00
60) Fluorene-d10	15.522	176	721255	28.346	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	68718	18.083	ng/ul	0.00
73) Anthracene-d10	17.380	188	1028367	28.135	ng/ul	0.00
81) Pyrene-d10	19.674	212	1145419	29.765	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.703	264	997313	27.218	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	13.951	165	5783	1.056	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
Data File : BN029552.D
Acq On : 07 Feb 2024 18:40
Operator : MA/JU
Sample : P1303-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FJ2


Quant Time: Feb 08 00:50:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

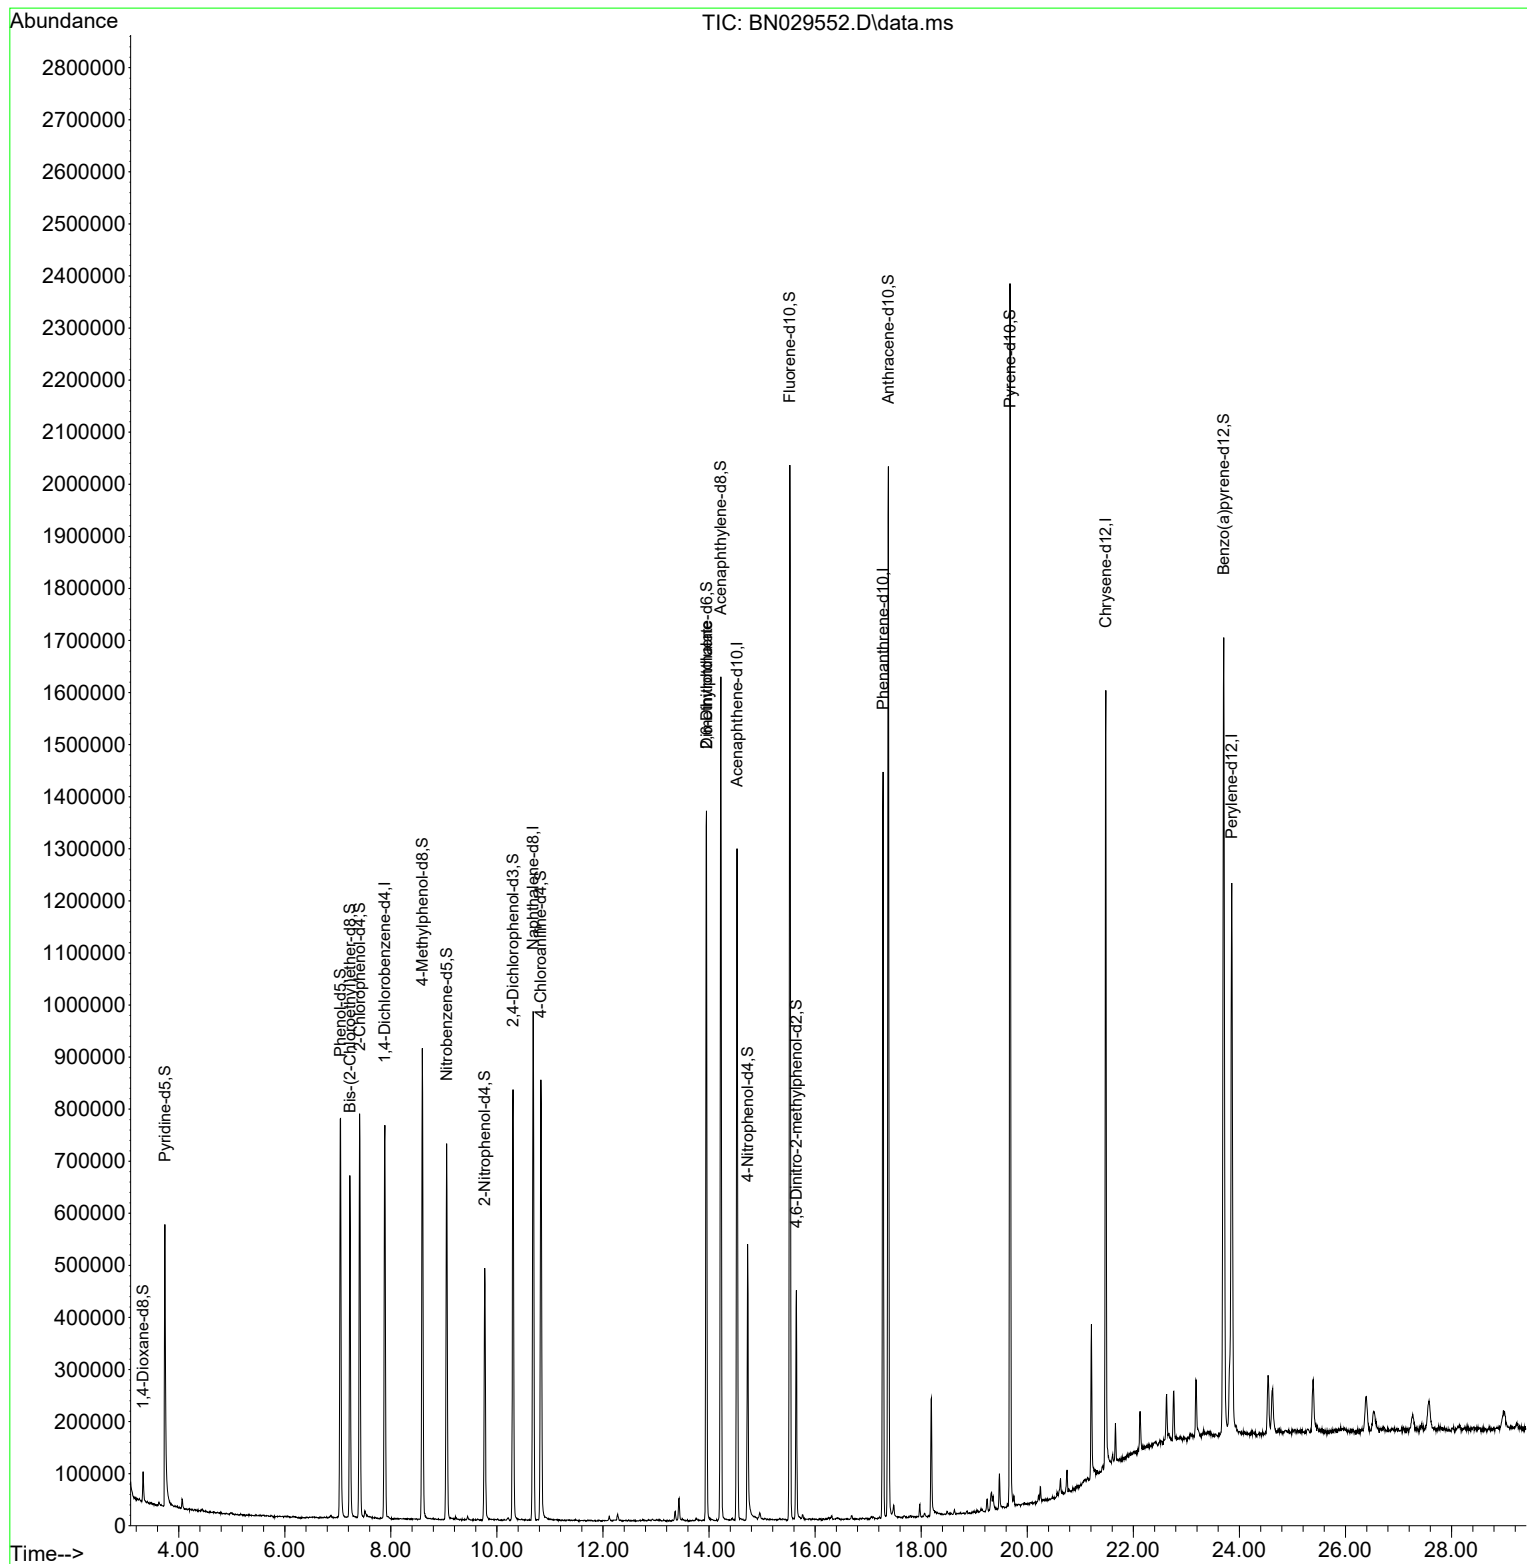

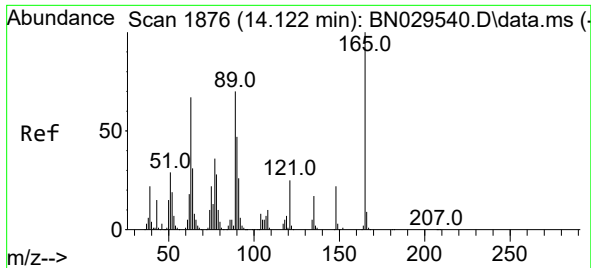

#48
 2,6-Dinitrotoluene
 Concen: 1.056 ng/ul
 RT: 13.951 min Scan# 11
 Delta R.T. -0.171 min
 Lab File: BN029552.D
 Acq: 07 Feb 2024 18:40

Instrument :
 BNA_N
 ClientSampleId :
 C0FJ2

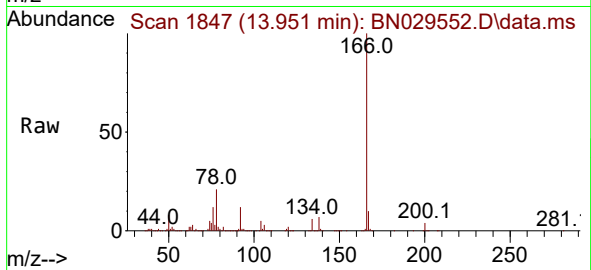

Tgt Ion:	165	Resp:	5783
Ion	Ratio	Lower	Upper
165	100		
89	4.3	55.8	83.8#
121	37.2	19.8	29.6#

