

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
 Data File : BN029555.D
 Acq On : 07 Feb 2024 21:05
 Operator : MA/JU
 Sample : PB158769BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK769

Quant Time: Feb 08 00:51:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	199274	20.000	ng/ul	0.00
20) Naphthalene-d8	10.681	136	854156	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	451670	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	870606	20.000	ng/ul	0.00
79) Chrysene-d12	21.475	240	707032	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264	774279	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.329	96	49420	8.157	ng/uL	0.00
4) Pyridine-d5	3.734	84	654938	40.536	ng/ul	0.00
7) Phenol-d5	7.046	99	762035	40.883	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	517250	41.581	ng/ul	0.00
11) 2-Chlorophenol-d4	7.411	132	576012	42.646	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	574330	41.316	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	282045	42.545	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	259088	44.874	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.305	165	461073	40.458	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	774365	39.829	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	1412594	42.007	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	1664015	41.668	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	229086	35.893	ng/ul	0.00
60) Fluorene-d10	15.522	176	1166717	40.784	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.646	200	149741	35.299	ng/ul	0.00
73) Anthracene-d10	17.375	188	1714553	42.022	ng/ul	0.00
81) Pyrene-d10	19.675	212	1888547	44.510	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	1783821	46.041	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	13.951	165	9780	1.588	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
Data File : BN029555.D
Acq On : 07 Feb 2024 21:05
Operator : MA/JU
Sample : PB158769BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK769


Quant Time: Feb 08 00:51:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

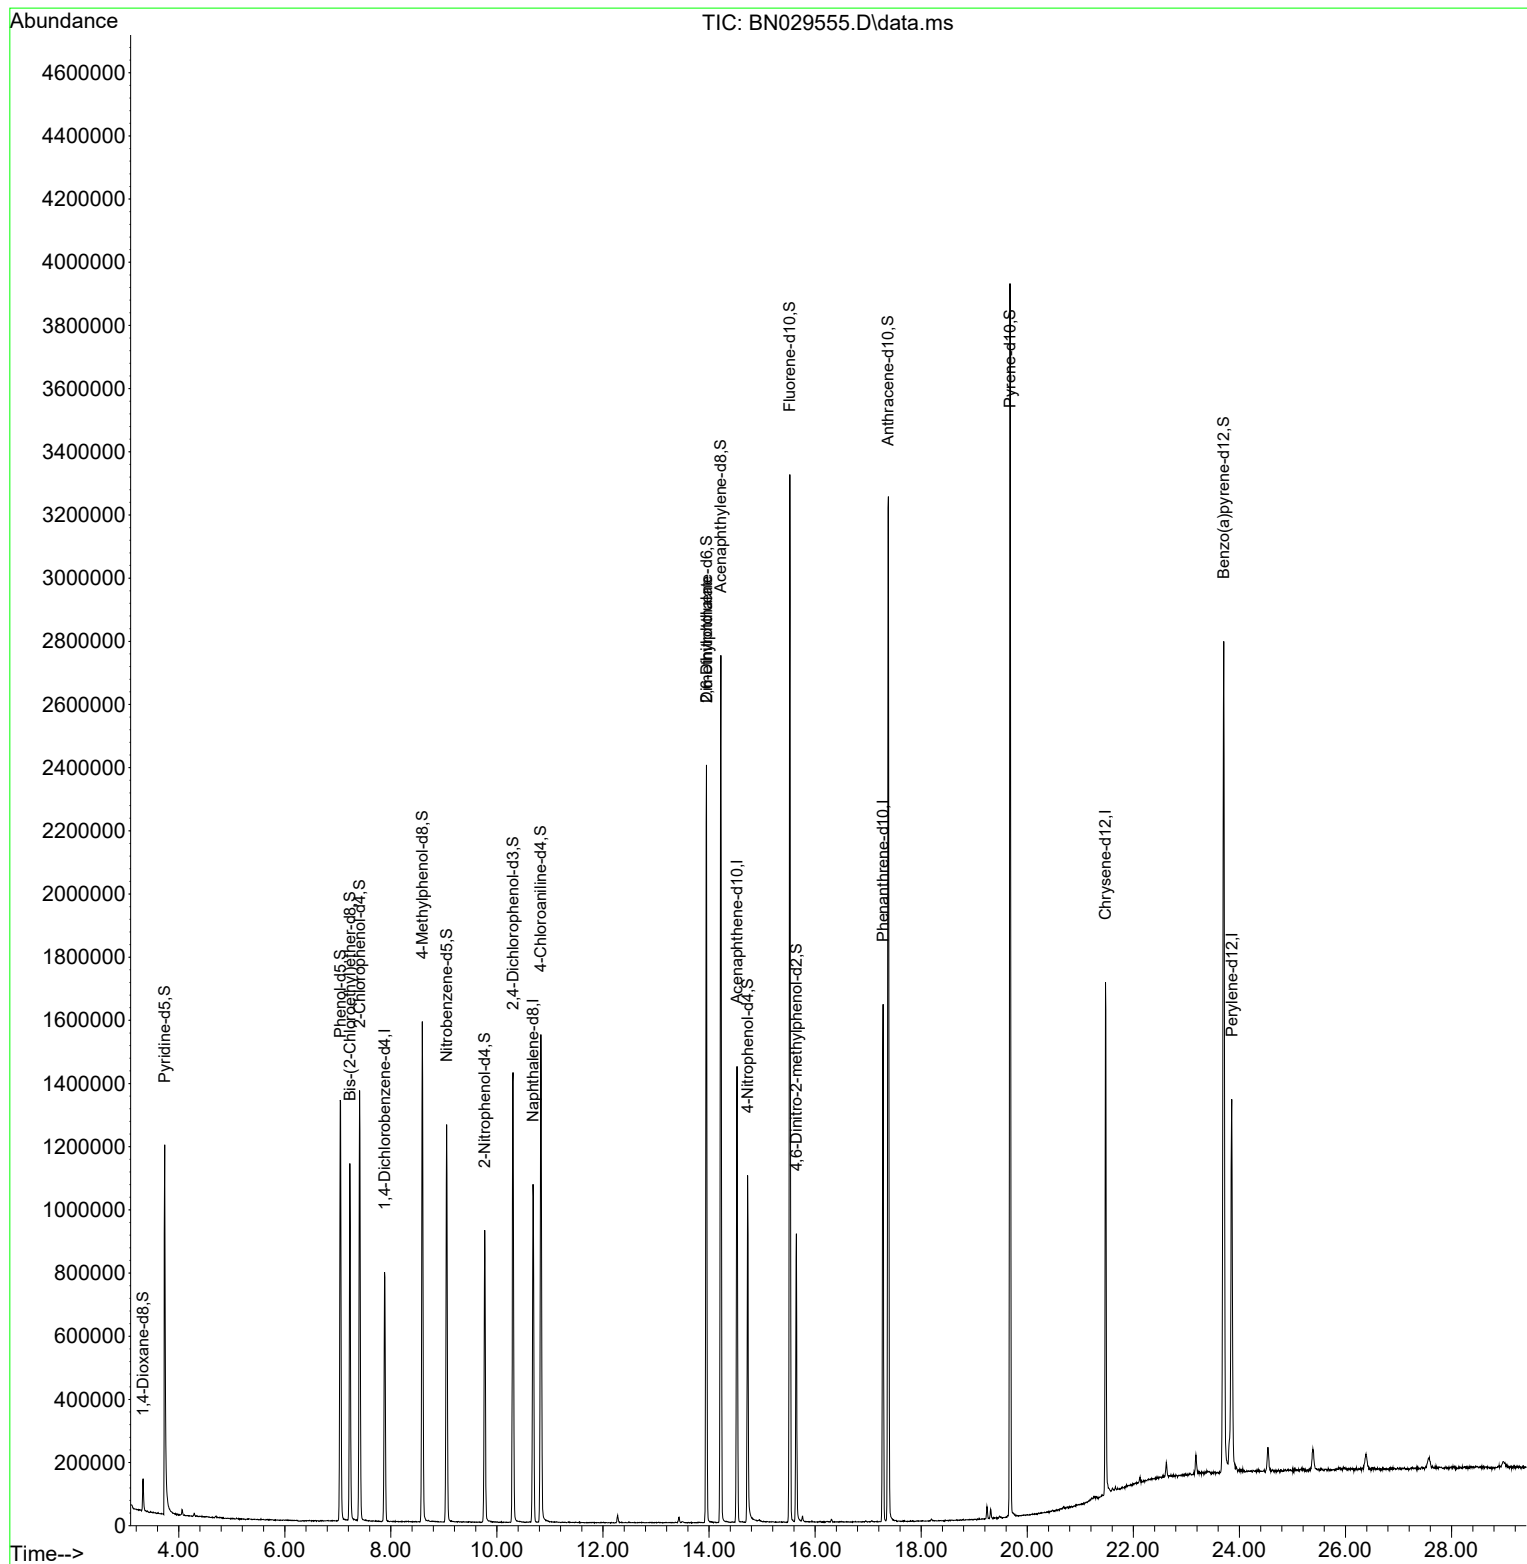

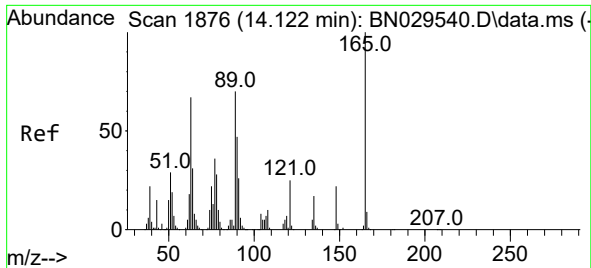

#48
 2,6-Dinitrotoluene
 Concen: 1.588 ng/ul
 RT: 13.951 min Scan# 11
 Delta R.T. -0.170 min
 Lab File: BN029555.D
 Acq: 07 Feb 2024 21:05

Instrument :
 BNA_N
 ClientSampleId :
 SBLK769

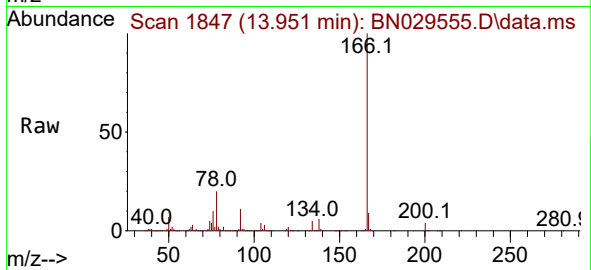

Tgt Ion:	165	Resp:	9780
Ion	Ratio	Lower	Upper
165	100		
89	3.1	55.8	83.8#
121	29.1	19.8	29.6

