

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
 Data File : BN029557.D
 Acq On : 07 Feb 2024 22:17
 Operator : MA/JU
 Sample : P1303-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FJ0

Quant Time: Feb 08 00:51:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	191078	20.000	ng/ul	0.00
20) Naphthalene-d8	10.681	136	786472	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	402996	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	776787	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	650645	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	715621	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	43616	7.508	ng/uL	0.00
4) Pyridine-d5	3.734	84	583872	37.687	ng/ul	0.00
7) Phenol-d5	7.046	99	711377	39.803	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	484525	40.621	ng/ul	0.00
11) 2-Chlorophenol-d4	7.411	132	551067	42.549	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	530036	39.765	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	259621	42.533	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	243574	45.818	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.305	165	436109	41.561	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	698016	38.992	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	1261436	42.043	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	1537784	43.158	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	207326	36.407	ng/ul	0.00
60) Fluorene-d10	15.522	176	1104291	43.264	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	130042	34.358	ng/ul	0.00
73) Anthracene-d10	17.381	188	1598786	43.917	ng/ul	0.00
81) Pyrene-d10	19.675	212	1747907	44.766	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	1591990	44.458	ng/ul	0.00
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	13.951	165	9183	1.671	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
Data File : BN029557.D
Acq On : 07 Feb 2024 22:17
Operator : MA/JU
Sample : P1303-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FJ0


Quant Time: Feb 08 00:51:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

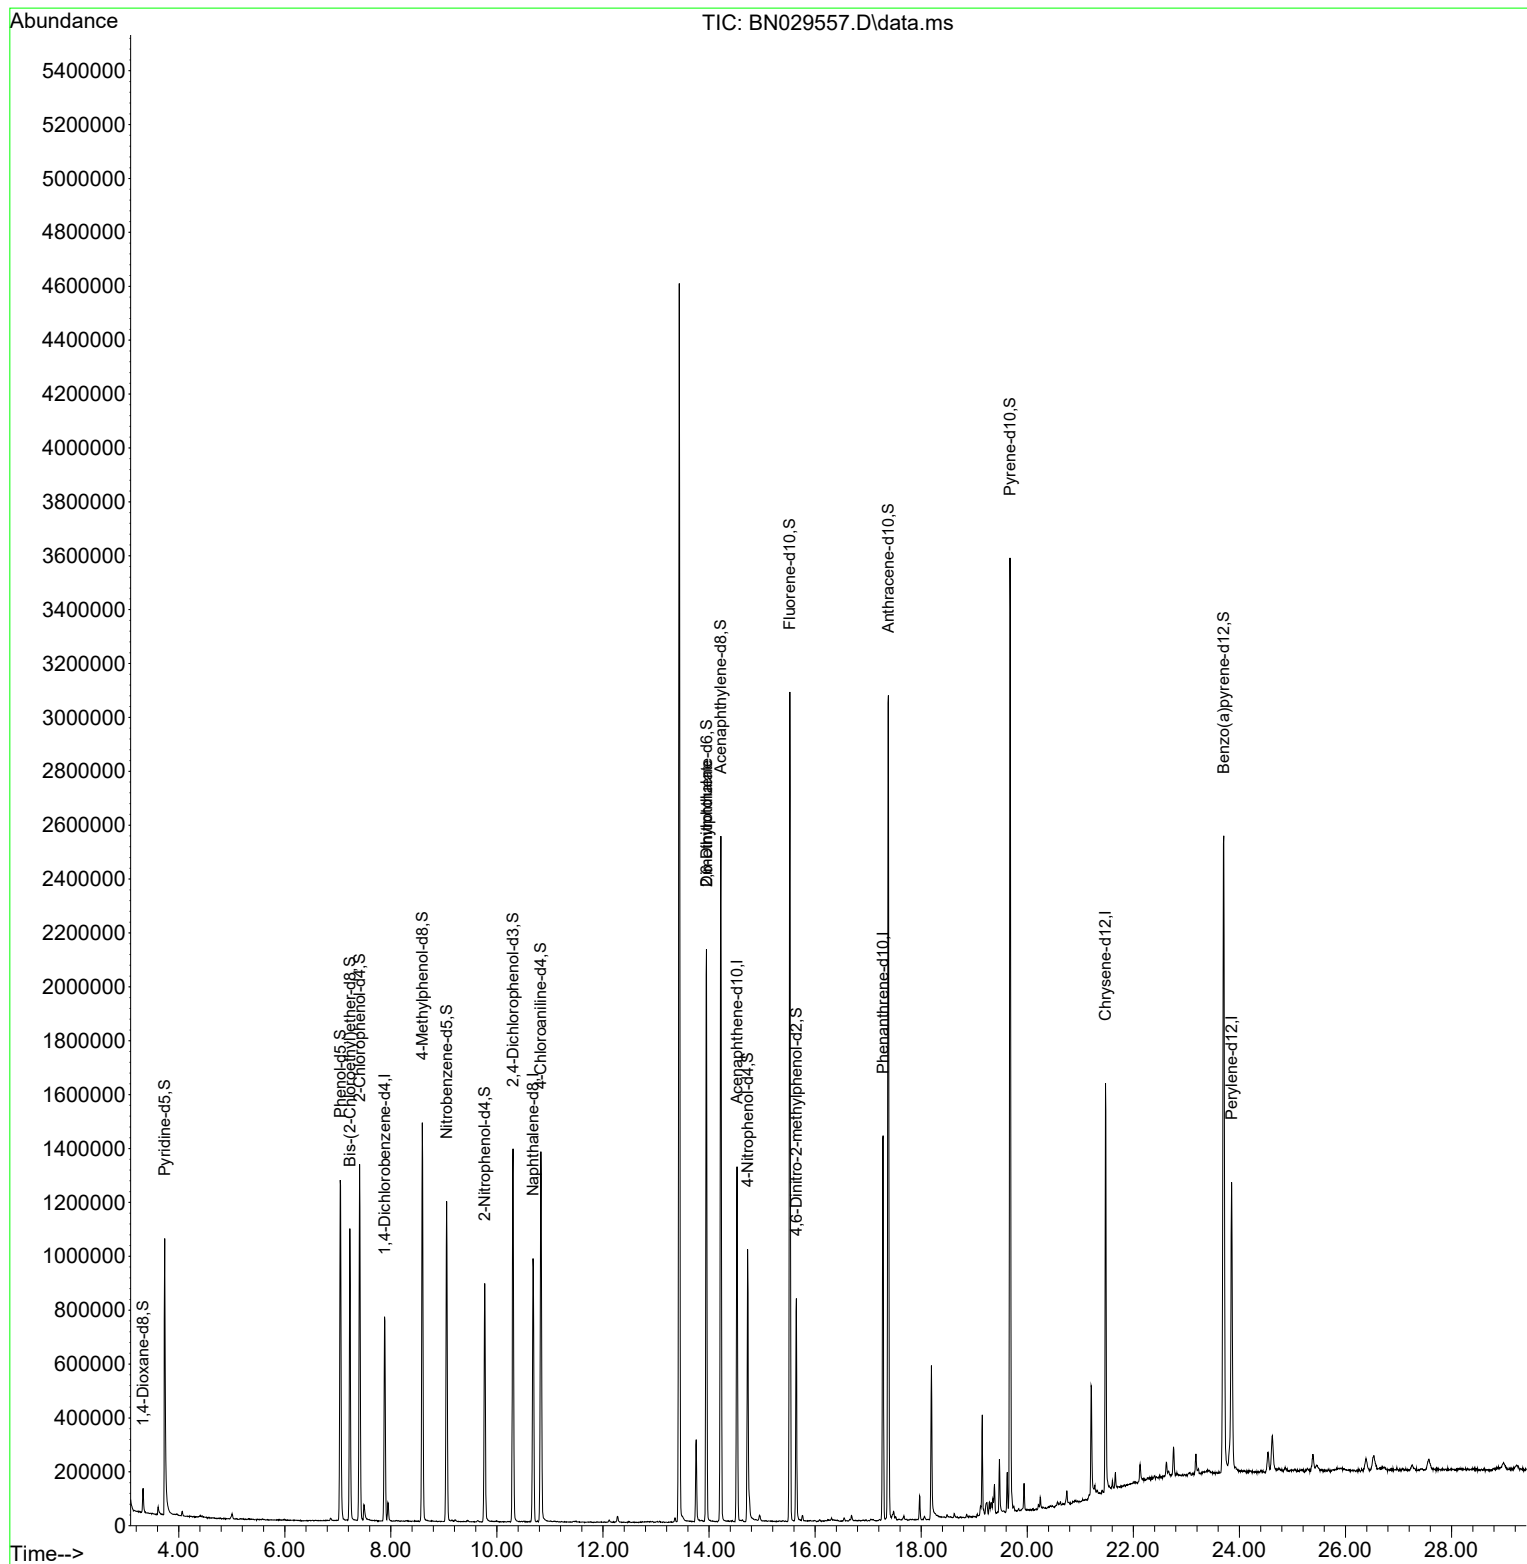

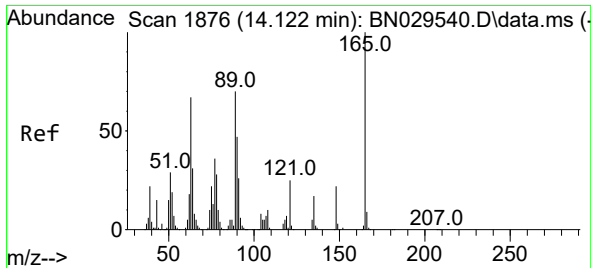

#48
 2,6-Dinitrotoluene
 Concen: 1.671 ng/ul
 RT: 13.951 min Scan# 11
 Delta R.T. -0.170 min
 Lab File: BN029557.D
 Acq: 07 Feb 2024 22:17

Instrument :
 BNA_N
 ClientSampleId :
 C0FJ0

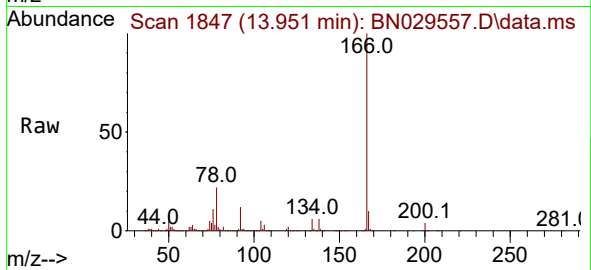

Tgt Ion:	165	Resp:	9183
Ion	Ratio	Lower	Upper
165	100		
89	2.7	55.8	83.8#
121	34.8	19.8	29.6#

