

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
 Data File : BN029562.D
 Acq On : 08 Feb 2024 01:17
 Operator : MA/JU
 Sample : P1303-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FJ4

Quant Time: Feb 08 02:07:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	201336	20.000	ng/ul	0.00
20) Naphthalene-d8	10.686	136	806661	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.527	164	411306	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.280	188	764133	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	618913	20.000	ng/ul	0.00
88) Perylene-d12	23.850	264	689445	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	36948	6.036	ng/uL	0.00
4) Pyridine-d5	3.740	84	251713	15.420	ng/ul	0.00
7) Phenol-d5	7.051	99	655093	34.786	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	447942	35.641	ng/ul	0.00
11) 2-Chlorophenol-d4	7.410	132	498134	36.502	ng/ul	0.00
15) 4-Methylphenol-d8	8.592	113	439984	31.328	ng/ul	0.00
21) Nitrobenzene-d5	9.051	128	243251	38.853	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	221289	40.584	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.304	165	394509	36.656	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	546705	29.775	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	1209119	39.485	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	1425300	39.193	ng/ul	0.00
54) 4-Nitrophenol-d4	14.727	143	192033	33.041	ng/ul	0.00
60) Fluorene-d10	15.521	176	1041108	39.965	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	118644	31.865	ng/ul	0.00
73) Anthracene-d10	17.380	188	1437665	40.145	ng/ul	0.00
81) Pyrene-d10	19.674	212	1655594	44.575	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1515770	43.937	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.716	105	39903	1.785	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
Data File : BN029562.D
Acq On : 08 Feb 2024 01:17
Operator : MA/JU
Sample : P1303-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FJ4

Quant Time: Feb 08 02:07:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

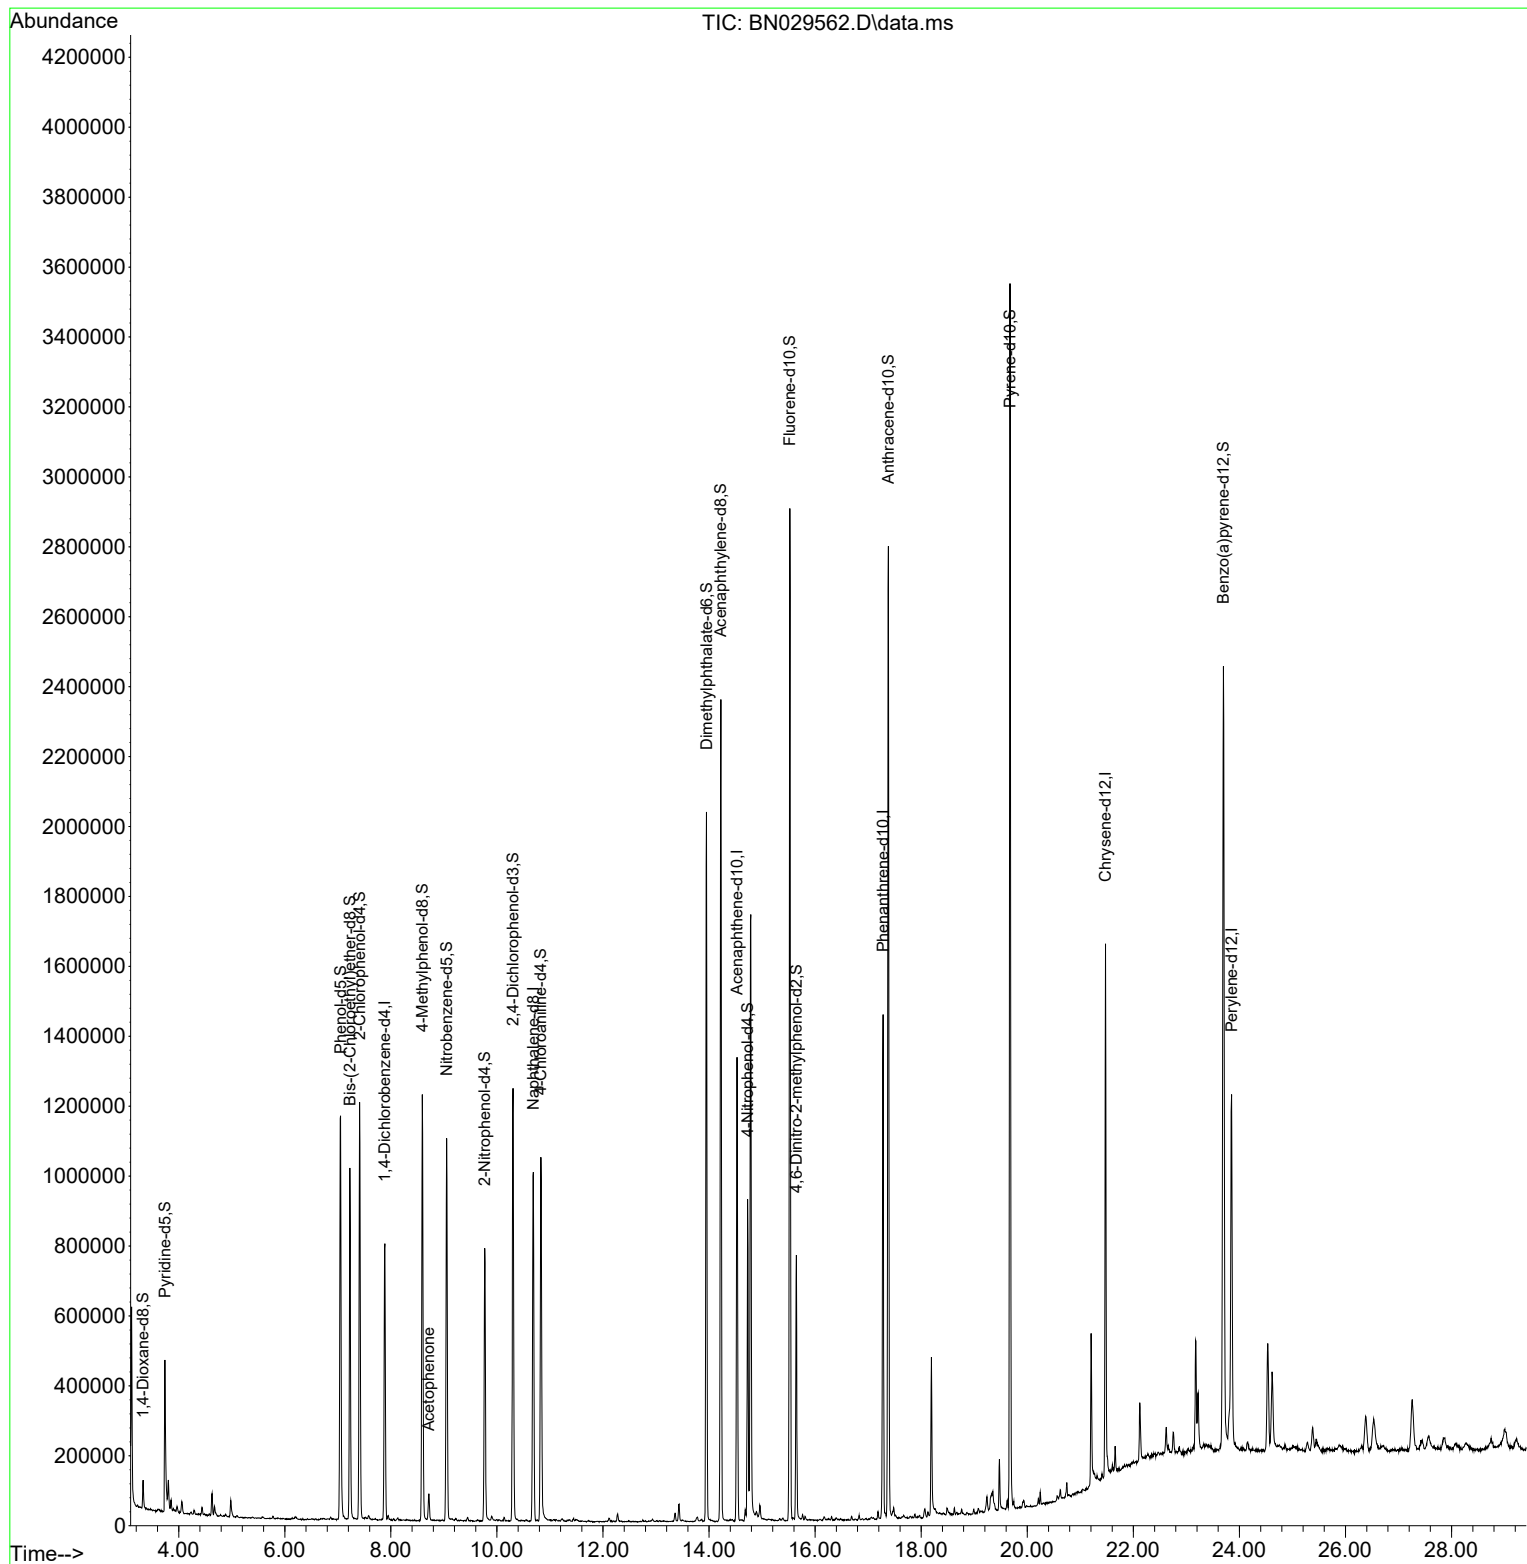

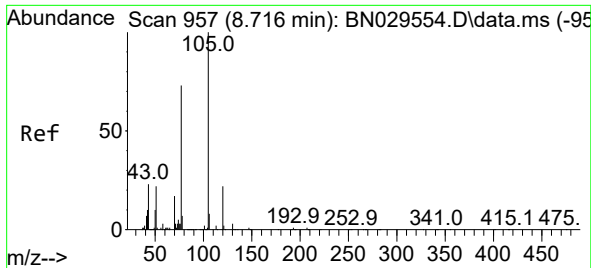

#16
 Acetophenone
 Concen: 1.785 ng/ul
 RT: 8.716 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BN029562.D
 Acq: 08 Feb 2024 01:17

Instrument :
 BNA_N
 ClientSampleId :
 C0FJ4

Tgt Ion:105 Resp: 39903
 Ion Ratio Lower Upper
 105 100
 77 85.2 67.4 101.0
 51 29.7 20.7 31.1

