

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
 Data File : BN029563.D
 Acq On : 08 Feb 2024 01:54
 Operator : MA/JU
 Sample : P1303-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FH3

Quant Time: Feb 08 02:28:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	192729	20.000	ng/ul	0.00
20) Naphthalene-d8	10.681	136	784199	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	401340	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	798136	20.000	ng/ul	0.00
79) Chrysene-d12	21.475	240	634740	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	711636	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.329	96	24064	4.107	ng/uL	0.00
4) Pyridine-d5	3.746	84	92112	5.895	ng/ul	0.00
7) Phenol-d5	7.046	99	412025	22.856	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	287370	23.886	ng/ul	0.00
11) 2-Chlorophenol-d4	7.411	132	318242	24.362	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	285942	21.269	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	150187	24.676	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	133240	25.136	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.305	165	248508	23.751	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	366320	20.522	ng/ul	0.00
46) Dimethylphthalate-d6	13.946	166	817049	27.344	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	914057	25.759	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	107713	18.993	ng/ul	0.00
60) Fluorene-d10	15.522	176	696410	27.397	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.646	200	67087	17.251	ng/ul	0.00
73) Anthracene-d10	17.375	188	979179	26.177	ng/ul	0.00
81) Pyrene-d10	19.675	212	1136059	29.825	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.692	264	1029066	28.899	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.716	105	29895	1.397	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
Data File : BN029563.D
Acq On : 08 Feb 2024 01:54
Operator : MA/JU
Sample : P1303-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FH3

Quant Time: Feb 08 02:28:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

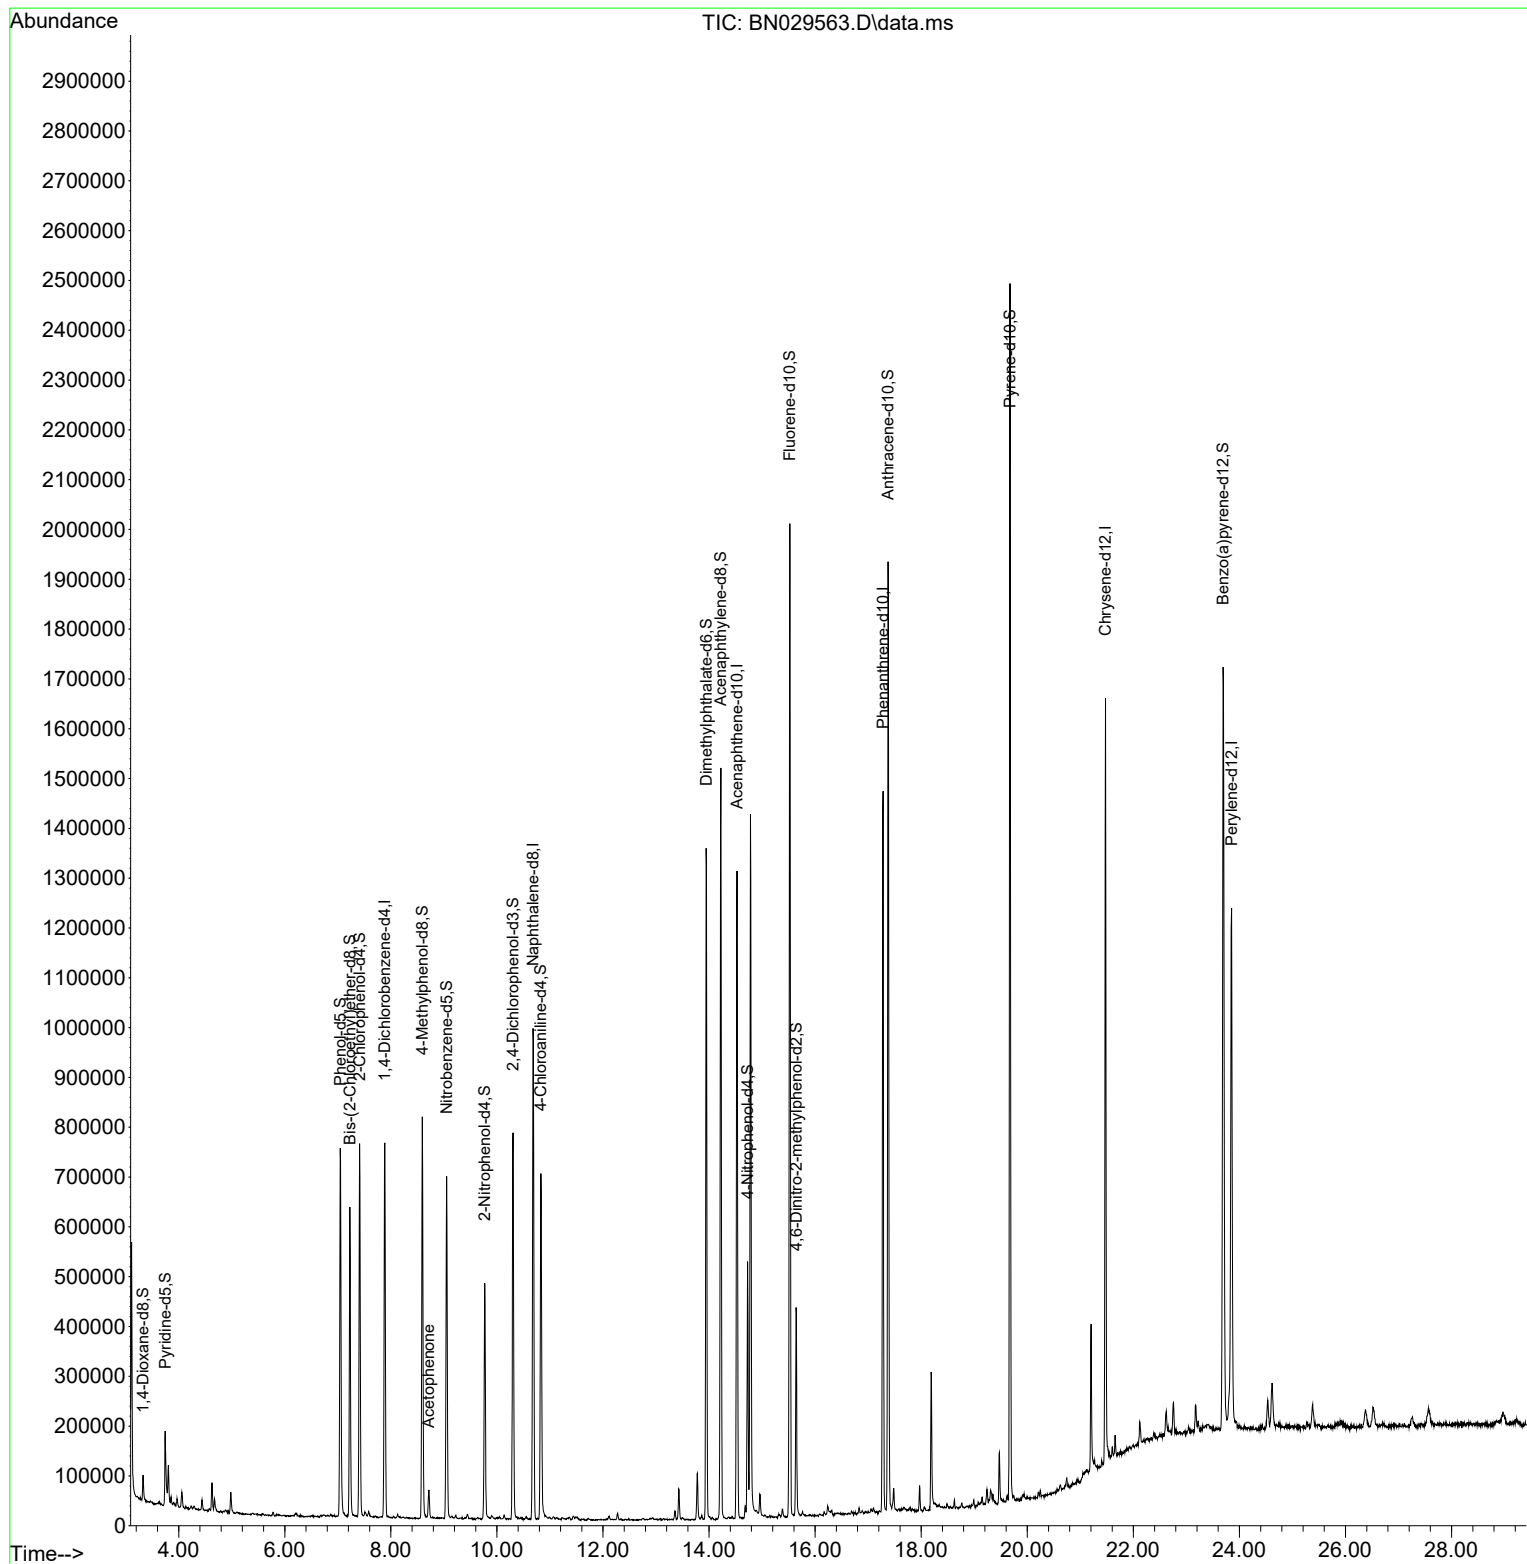

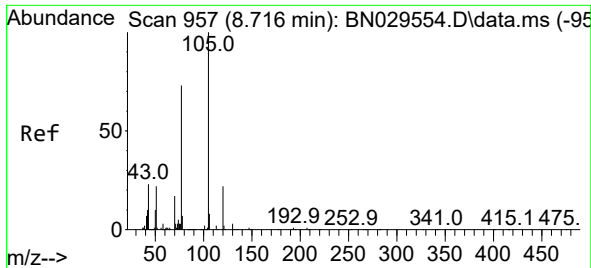

#16
 Acetophenone
 Concen: 1.397 ng/ul
 RT: 8.716 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BN029563.D
 Acq: 08 Feb 2024 01:54

Instrument :
 BNA_N
 ClientSampleId :
 C0FH3

Tgt Ion	Ratio	Lower	Upper
105	100		
77	90.4	67.4	101.0
51	28.8	20.7	31.1

