

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
 Data File : BN029564.D
 Acq On : 08 Feb 2024 02:30
 Operator : MA/JU
 Sample : P1303-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FJ3

Quant Time: Feb 08 03:46:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	197924	20.000	ng/ul	0.00
20) Naphthalene-d8	10.681	136	801360	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	410578	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	789543	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	621092	20.000	ng/ul	0.00
88) Perylene-d12	23.845	264	715120	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	22957	3.815	ng/uL	0.00
4) Pyridine-d5	3.746	84	57404	3.577	ng/ul	0.00
7) Phenol-d5	7.046	99	425019	22.958	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	301781	24.425	ng/ul	0.00
11) 2-Chlorophenol-d4	7.411	132	321450	23.961	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	293035	21.224	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	156321	25.134	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	131939	24.357	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.304	165	248498	23.242	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	339882	18.633	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	761795	24.921	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	925146	25.485	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	95214	16.411	ng/ul	0.00
60) Fluorene-d10	15.522	176	715403	27.511	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	59687	15.515	ng/ul	0.00
73) Anthracene-d10	17.381	188	1011774	27.343	ng/ul	0.00
81) Pyrene-d10	19.675	212	1171688	31.436	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1079527	30.168	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.716	105	30893	1.406	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020724\
Data File : BN029564.D
Acq On : 08 Feb 2024 02:30
Operator : MA/JU
Sample : P1303-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FJ3

Quant Time: Feb 08 03:46:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

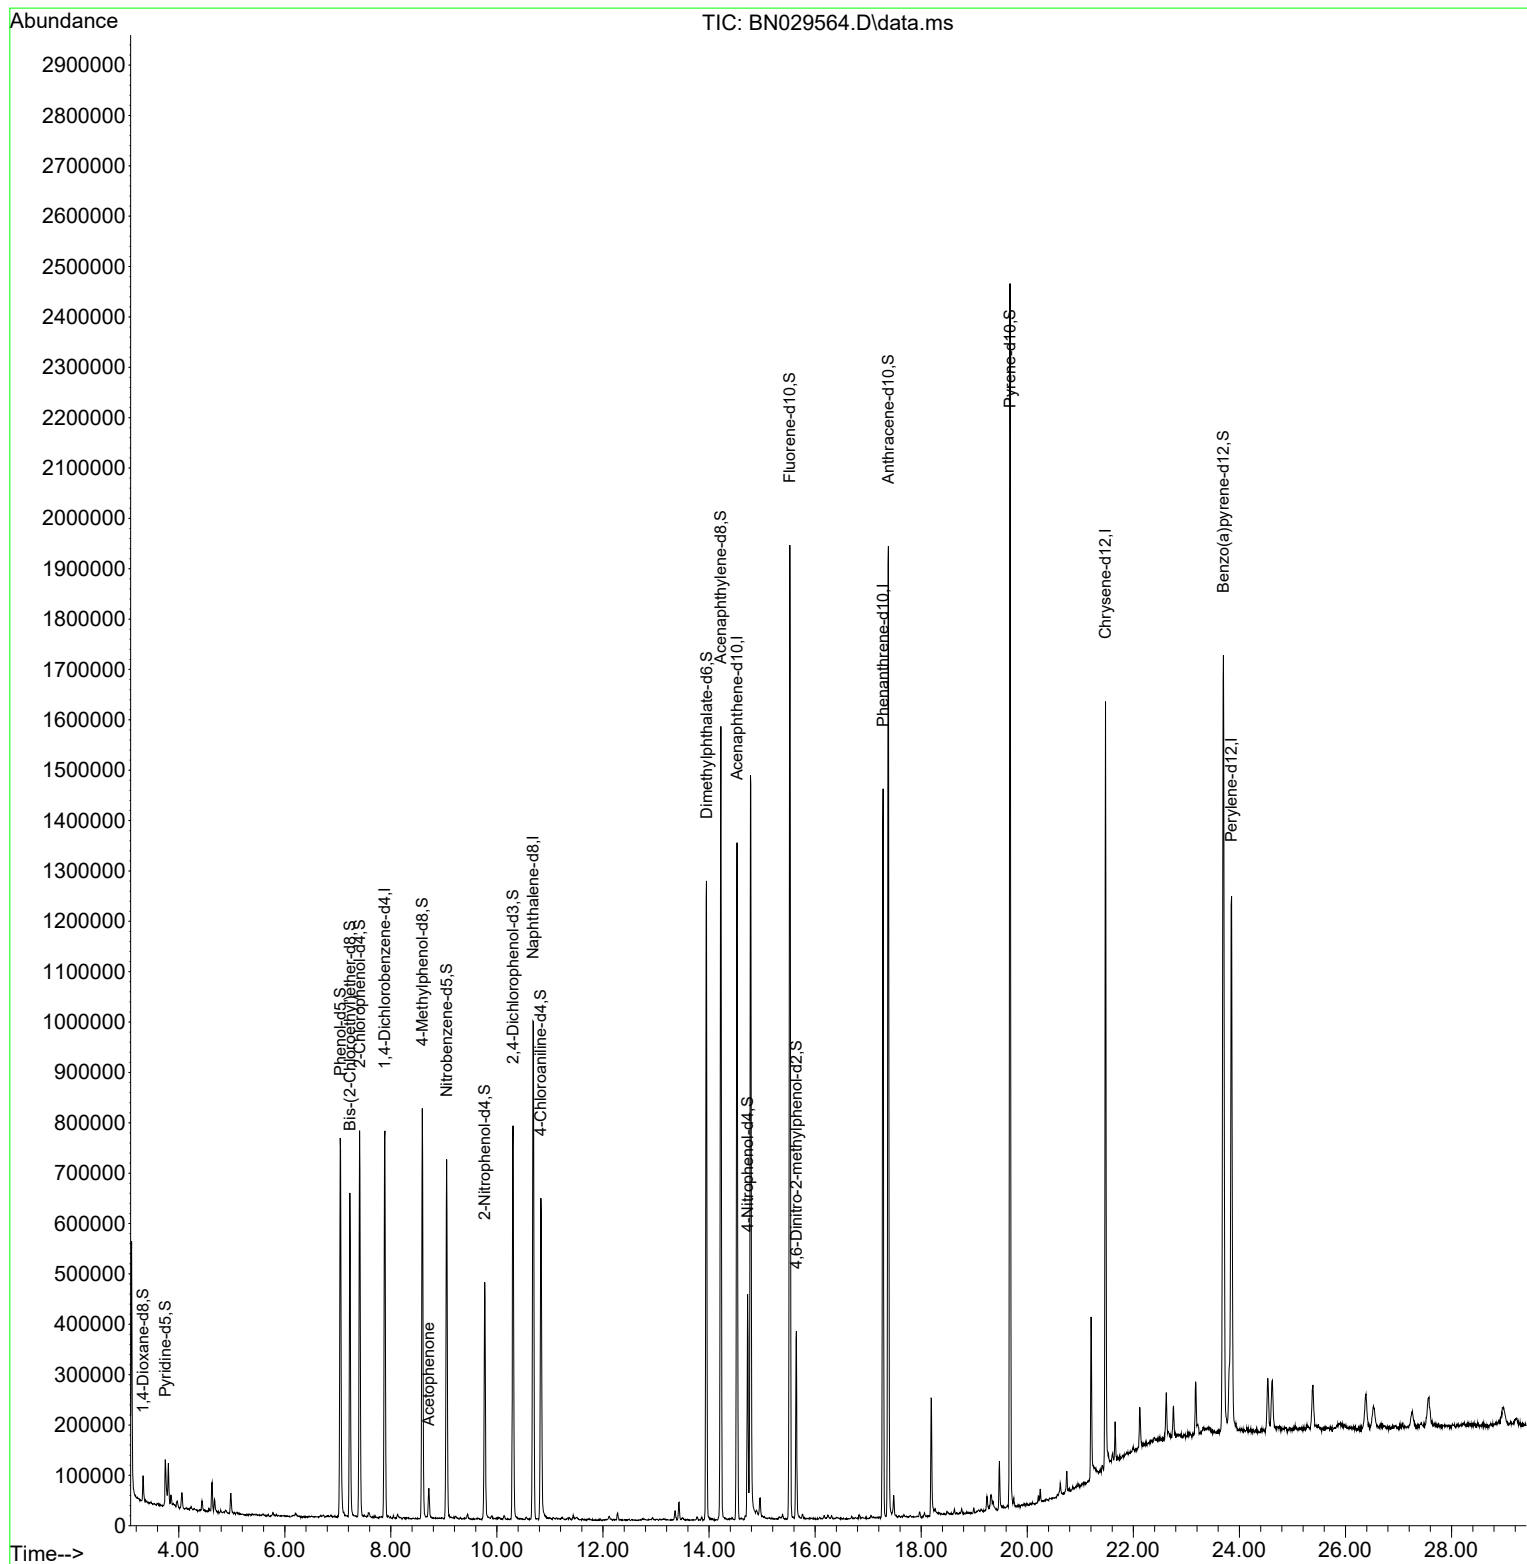

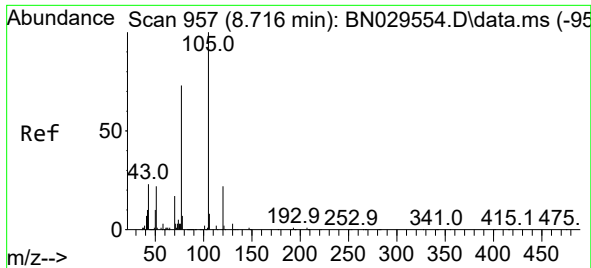

#16
 Acetophenone
 Concen: 1.406 ng/ul
 RT: 8.716 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BN029564.D
 Acq: 08 Feb 2024 02:30

Instrument :
 BNA_N
 ClientSampleId :
 C0FJ3

Tgt Ion:105 Resp: 30893
 Ion Ratio Lower Upper
 105 100
 77 89.9 67.4 101.0
 51 29.8 20.7 31.1

