

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
 Data File : BN029582.D
 Acq On : 08 Feb 2024 17:47
 Operator : MA/JU
 Sample : P1303-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FH4

Quant Time: Feb 08 23:58:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 07 02:17:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.889	152	5415	0.400	ng/ul	0.00
4) Naphthalene-d8	10.683	136	14762	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.525	164	6725	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.276	188	12847	0.400	ng/ul	0.00
17) Chrysene-d12	21.476	240	9657	0.400	ng/ul	0.00
23) Perylene-d12	23.849	264	12616	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.332	96	48832	7.232	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.278	152	8208	0.437	ng/ul	0.00
18) Fluoranthene-d10	19.309	212	13958	0.440	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.524	166	2481	0.095	ng/ul#	15
20) Pyrene	19.676	202	2183	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.697	252	4621	0.104	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
Data File : BN029582.D
Acq On : 08 Feb 2024 17:47
Operator : MA/JU
Sample : P1303-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FH4

Quant Time: Feb 08 23:58:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 02:17:13 2024
Response via : Initial Calibration




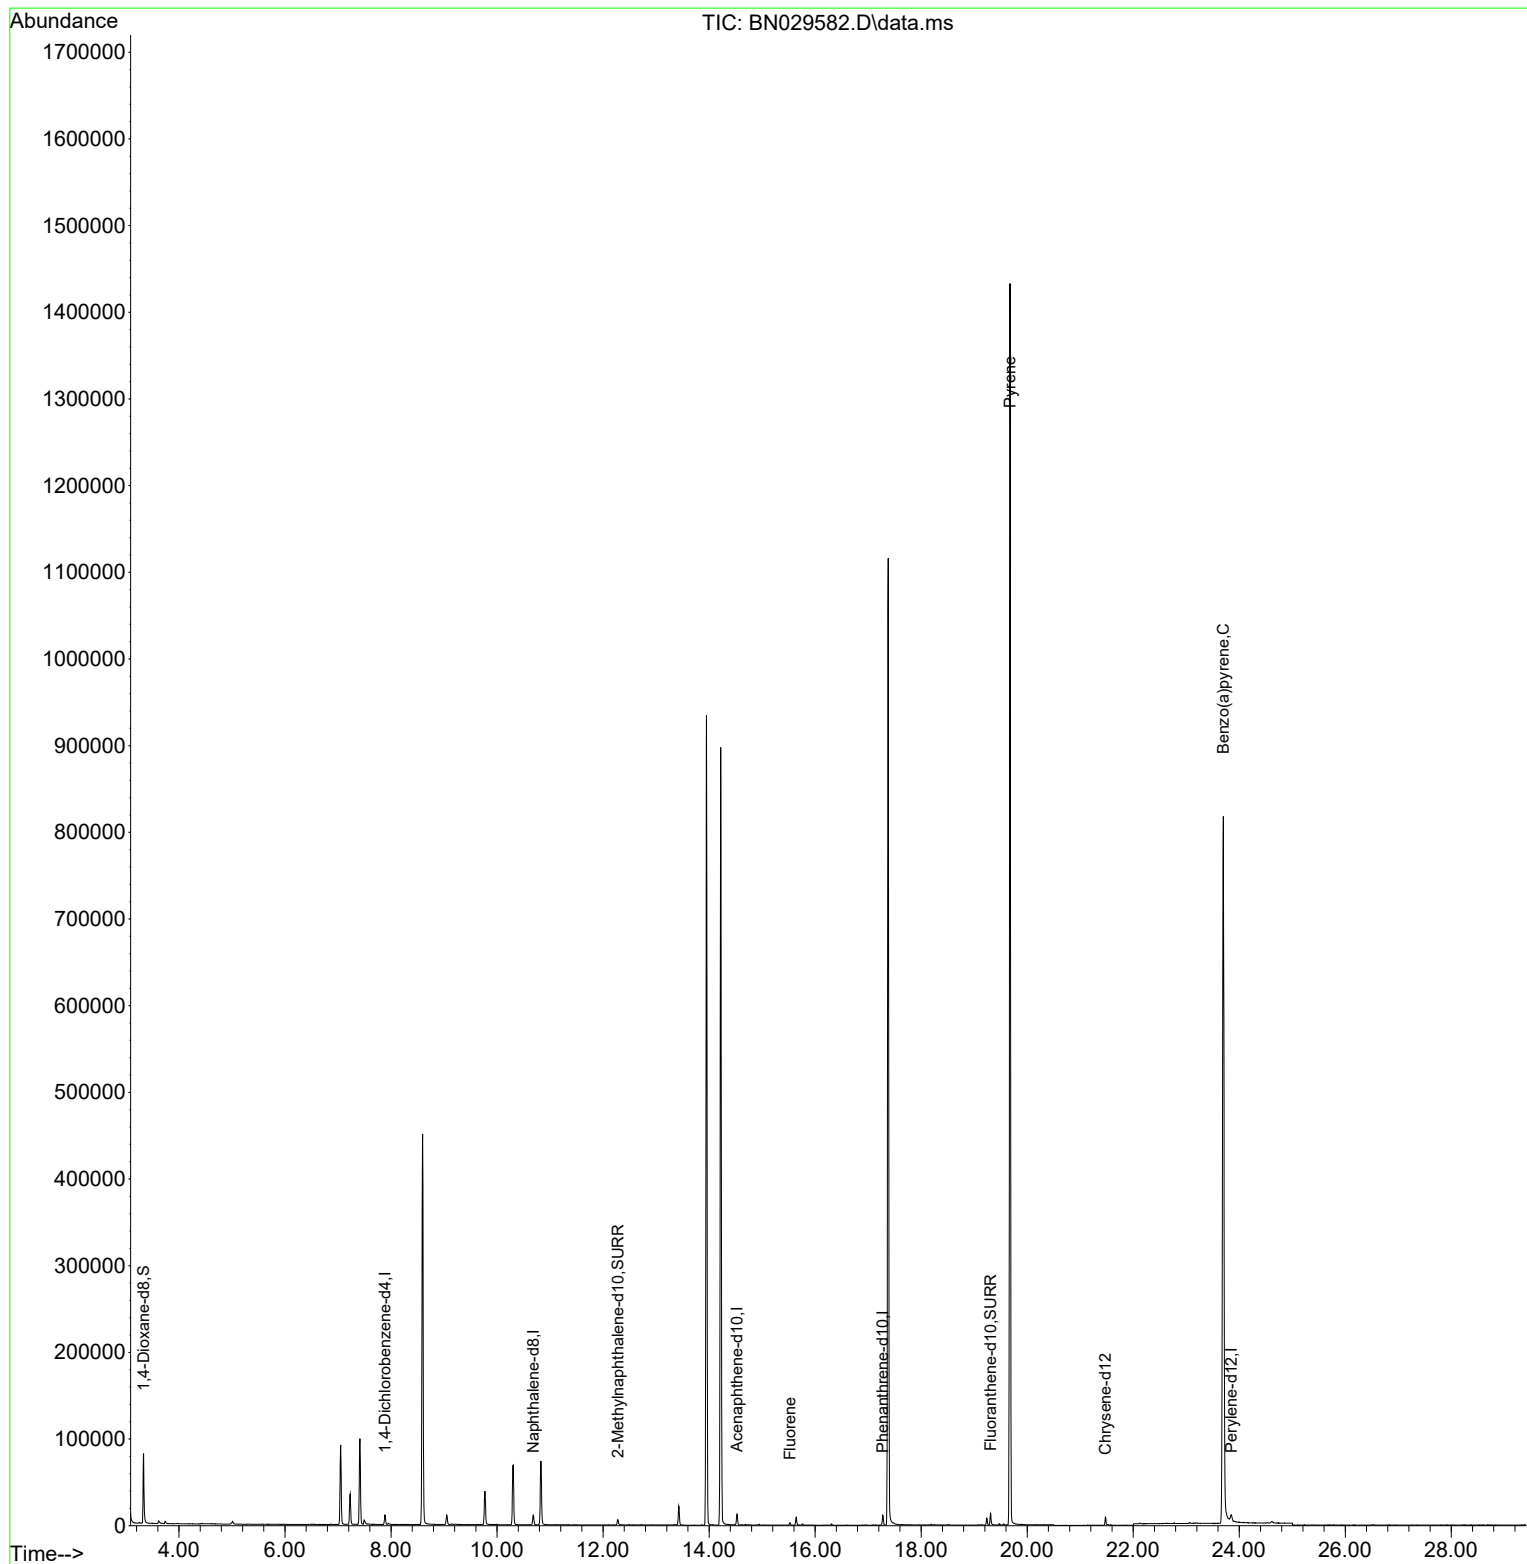


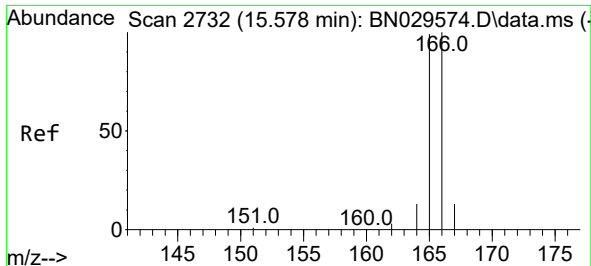

#12
Fluorene
Concen: 0.095 ng/ul
RT: 15.524 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN029582.D
Acq: 08 Feb 2024 17:47




Instrument :
BNA_N
ClientSampleId :
C0FH4


Tgt Ion:166 Resp: 2481
Ion Ratio Lower Upper
166 100
165 9.2 78.6 117.8#
167 35.7 11.5 17.3#

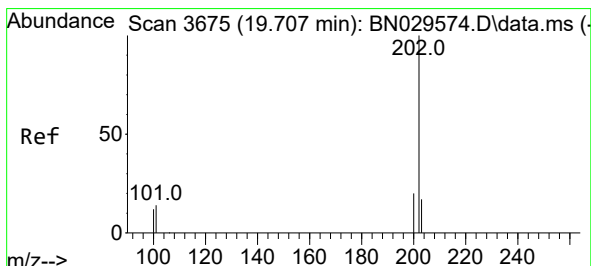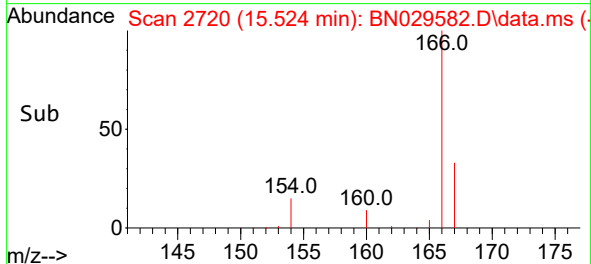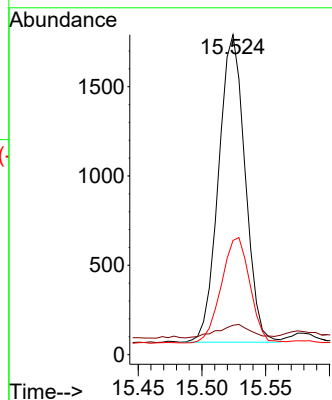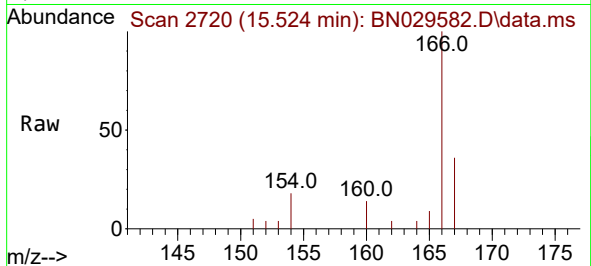

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.676 min Scan# 3668
Delta R.T. -0.032 min
Lab File: BN029582.D
Acq: 08 Feb 2024 17:47


Tgt Ion:202 Resp: 2183
Ion Ratio Lower Upper
202 100
101 191.5 12.5 18.7#
100 1405.3 10.0 15.0#

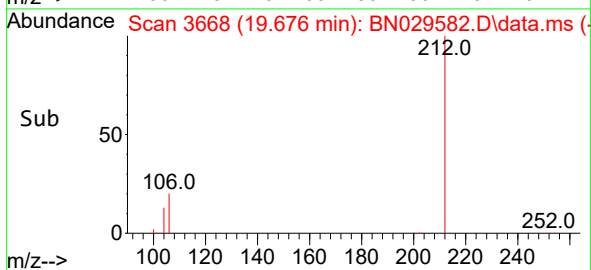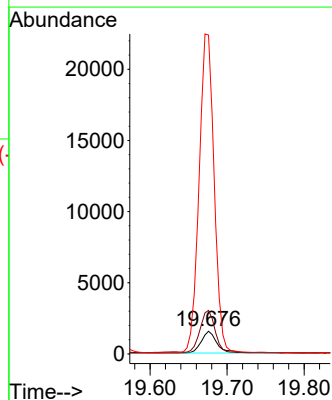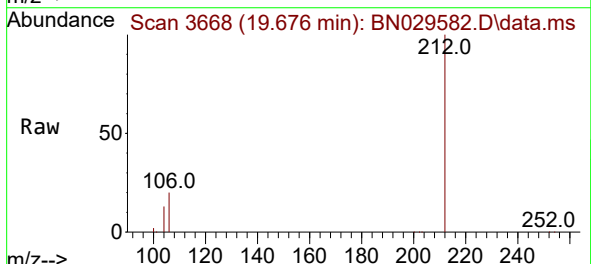

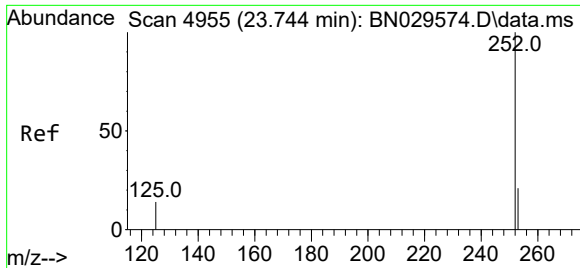

#26
Benzo(a)pyrene
Concen: 0.104 ng/ul
RT: 23.697 min Scan# 4939
Delta R.T. -0.055 min
Lab File: BN029582.D
Acq: 08 Feb 2024 17:47

Instrument :
BNA_N
ClientSampleId :
C0FH4

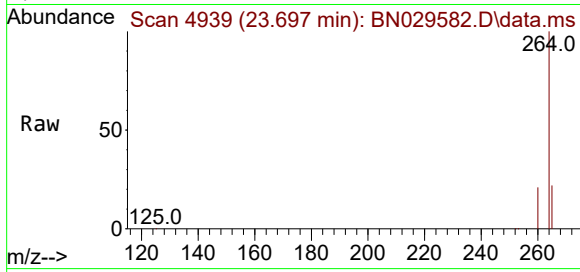

Tgt Ion:252 Resp: 4621
Ion Ratio Lower Upper
252 100
253 55.5 25.4 38.0#
125 40.4 16.0 24.0#

