

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
 Data File : BN029584.D
 Acq On : 08 Feb 2024 18:59
 Operator : MA/JU
 Sample : P1303-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FJ0

Quant Time: Feb 08 23:59:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 07 02:17:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.884	152	5688	0.400	ng/ul	0.00
4) Naphthalene-d8	10.683	136	15514	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.525	164	7286	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.276	188	14456	0.400	ng/ul	0.00
17) Chrysene-d12	21.479	240	10951	0.400	ng/ul	0.00
23) Perylene-d12	23.849	264	14194	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.332	96	53786	7.584	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.278	152	8456	0.428	ng/ul	0.00
18) Fluoranthene-d10	19.309	212	15181	0.422	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Anthracene	17.378	178	819	0.022	ng/ul#	1
20) Pyrene	19.676	202	2369	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.700	252	4735	0.094	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
Data File : BN029584.D
Acq On : 08 Feb 2024 18:59
Operator : MA/JU
Sample : P1303-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FJ0

Quant Time: Feb 08 23:59:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 02:17:13 2024
Response via : Initial Calibration




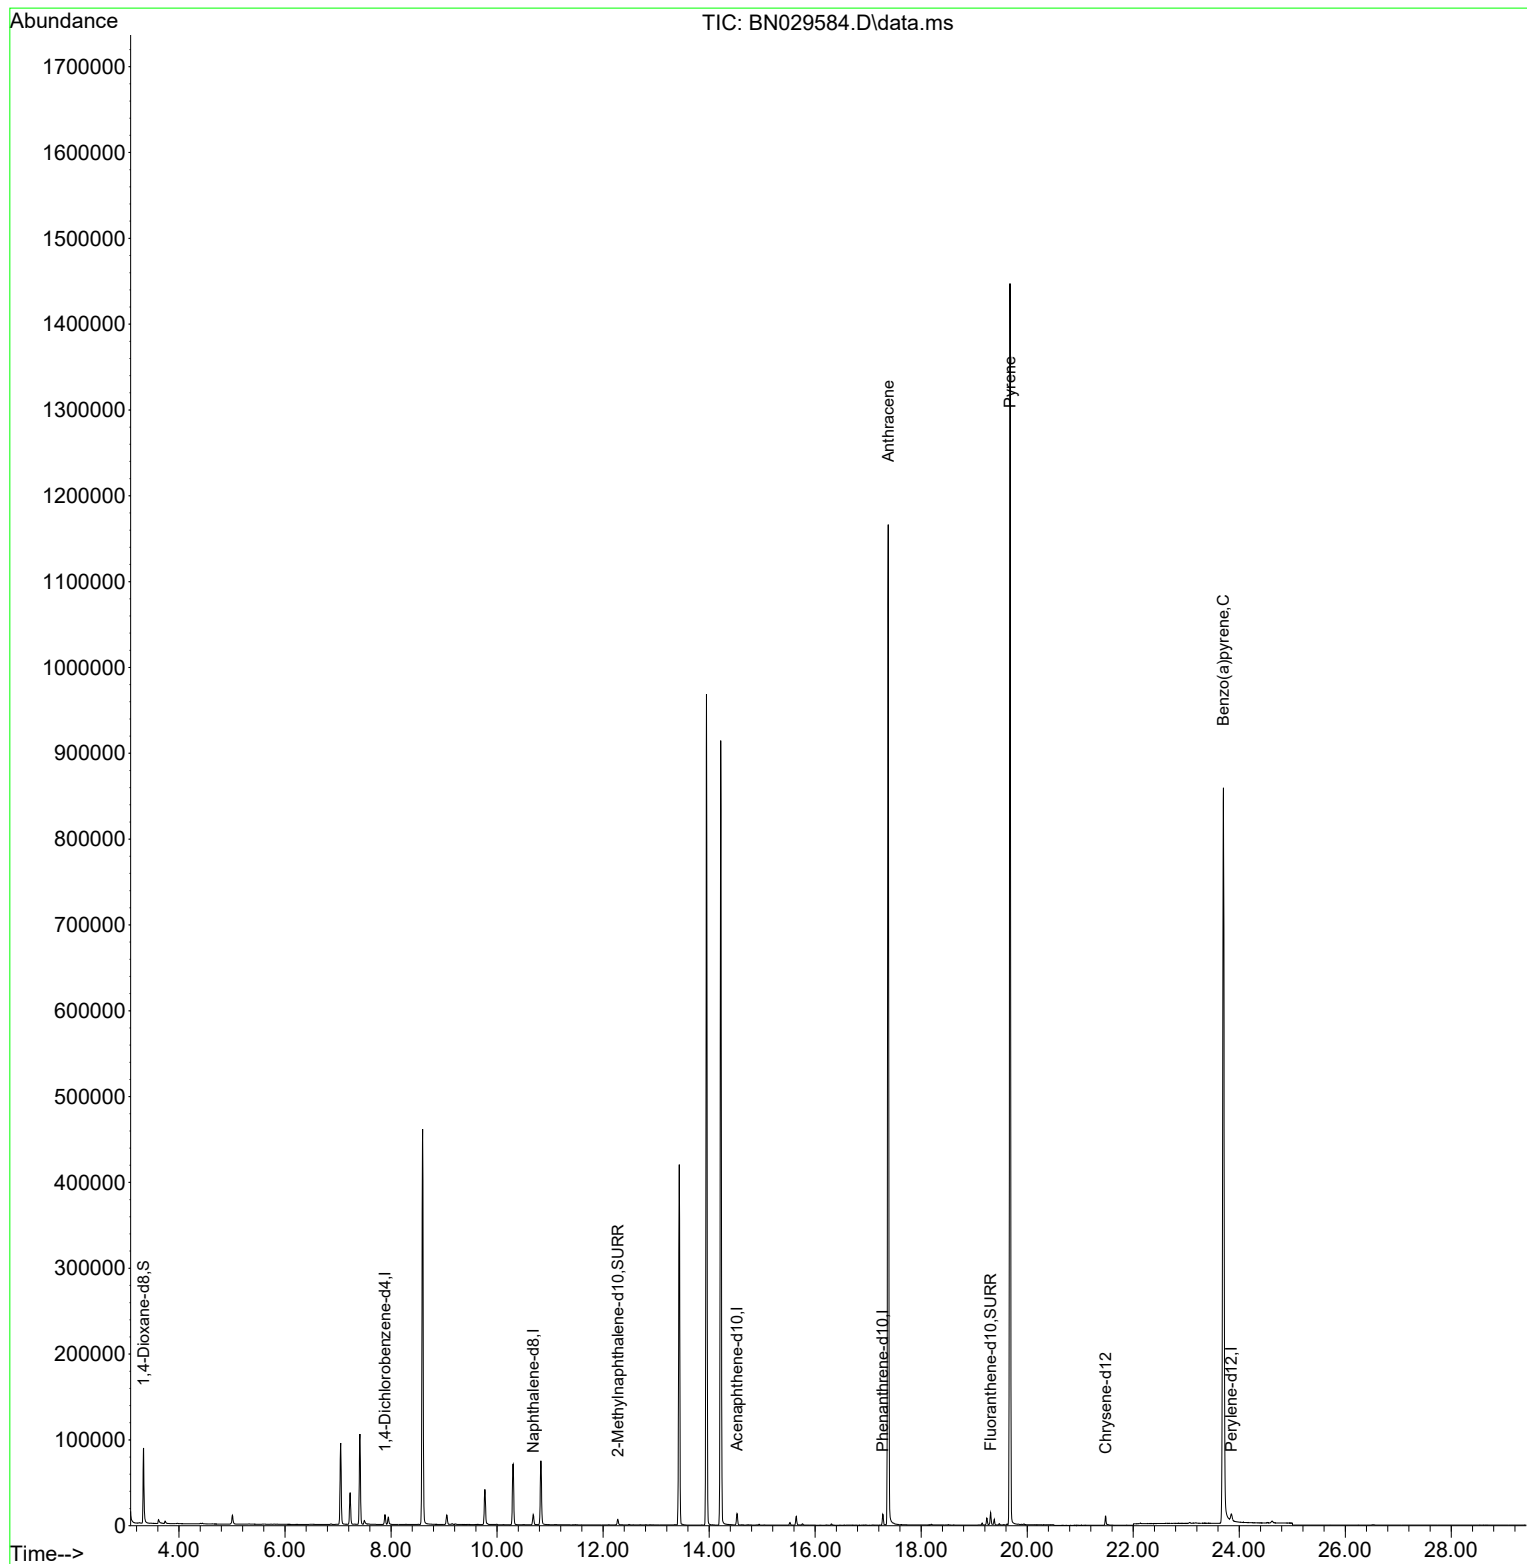


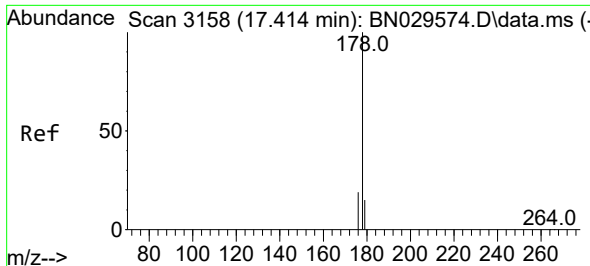

#16
Anthracene
Concen: 0.022 ng/ul
RT: 17.378 min Scan# 3158
Delta R.T. -0.038 min
Lab File: BN029584.D
Acq: 08 Feb 2024 18:59




Instrument :
BNA_N
ClientSampleId :
C0FJ0


Tgt Ion:178 Resp: 819
Ion Ratio Lower Upper
178 100
179 214.7 12.9 19.3#
176 19.7 15.8 23.8

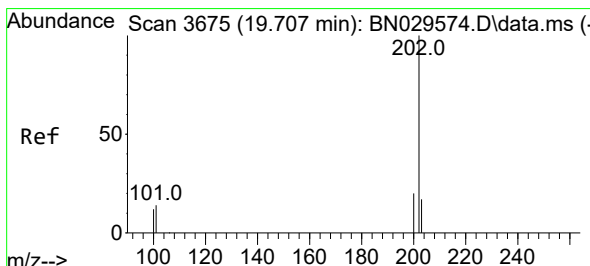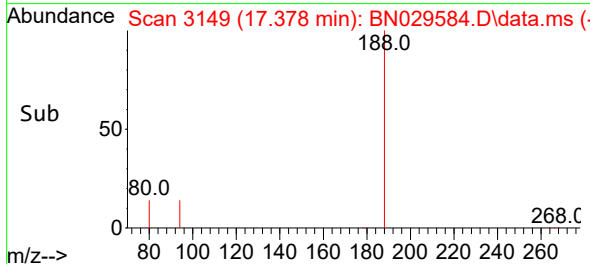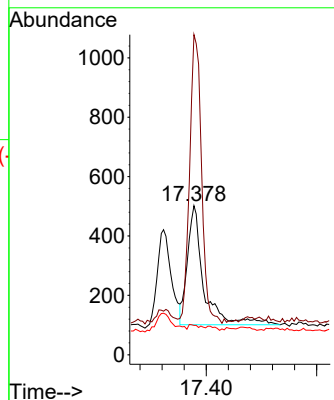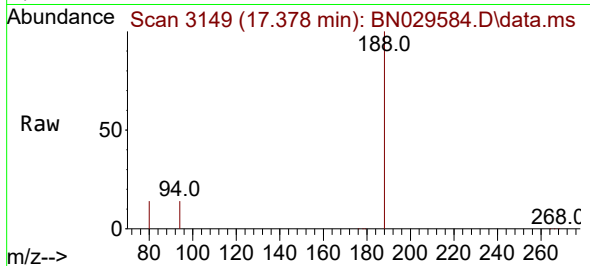

#20
Pyrene
Concen: 0.046 ng/ul
RT: 19.676 min Scan# 3668
Delta R.T. -0.032 min
Lab File: BN029584.D
Acq: 08 Feb 2024 18:59


Tgt Ion:202 Resp: 2369
Ion Ratio Lower Upper
202 100
101 204.8 12.5 18.7#
100 1515.4 10.0 15.0#

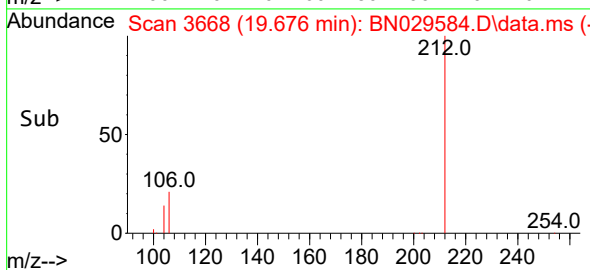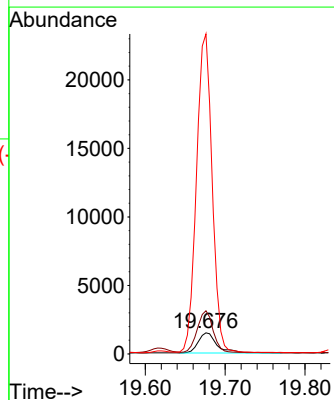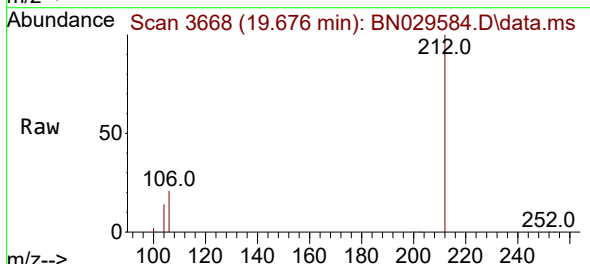

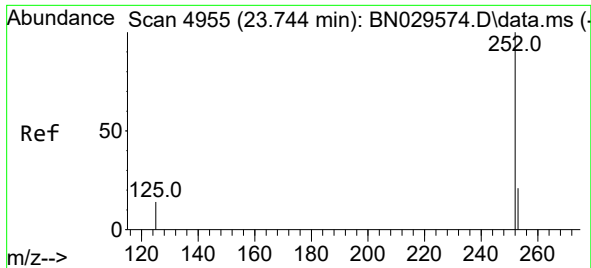

#26
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.700 min Scan# 4940
Delta R.T. -0.052 min
Lab File: BN029584.D
Acq: 08 Feb 2024 18:59

Instrument :
BNA_N
ClientSampleId :
C0FJ0

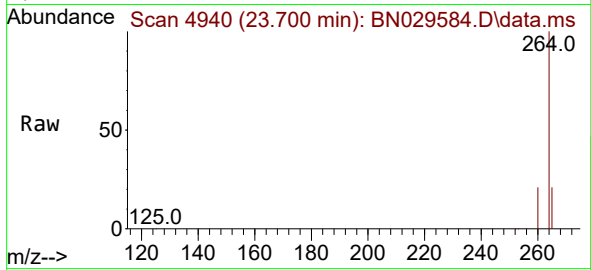

Tgt Ion:252 Resp: 4735
Ion Ratio Lower Upper
252 100
253 54.4 25.4 38.0#
125 41.2 16.0 24.0#

