

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
 Data File : BN029587.D
 Acq On : 08 Feb 2024 21:24
 Operator : MA/JU
 Sample : PB158770BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK770

Quant Time: Feb 08 23:59:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 07 02:17:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.888	152	6191	0.400	ng/ul	0.00
4) Naphthalene-d8	10.683	136	17025	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.526	164	7835	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.277	188	14626	0.400	ng/ul	0.00
17) Chrysene-d12	21.479	240	9594	0.400	ng/ul	0.00
23) Perylene-d12	23.847	264	13530	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.332	96	66877	8.663	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.278	152	9506	0.439	ng/ul	0.00
18) Fluoranthene-d10	19.309	212	14369	0.456	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.677	202	2489	0.055	ng/ul#	1
26) Benzo(a)pyrene	23.698	252	5230	0.109	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
Data File : BN029587.D
Acq On : 08 Feb 2024 21:24
Operator : MA/JU
Sample : PB158770BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK770

Quant Time: Feb 08 23:59:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 02:17:13 2024
Response via : Initial Calibration

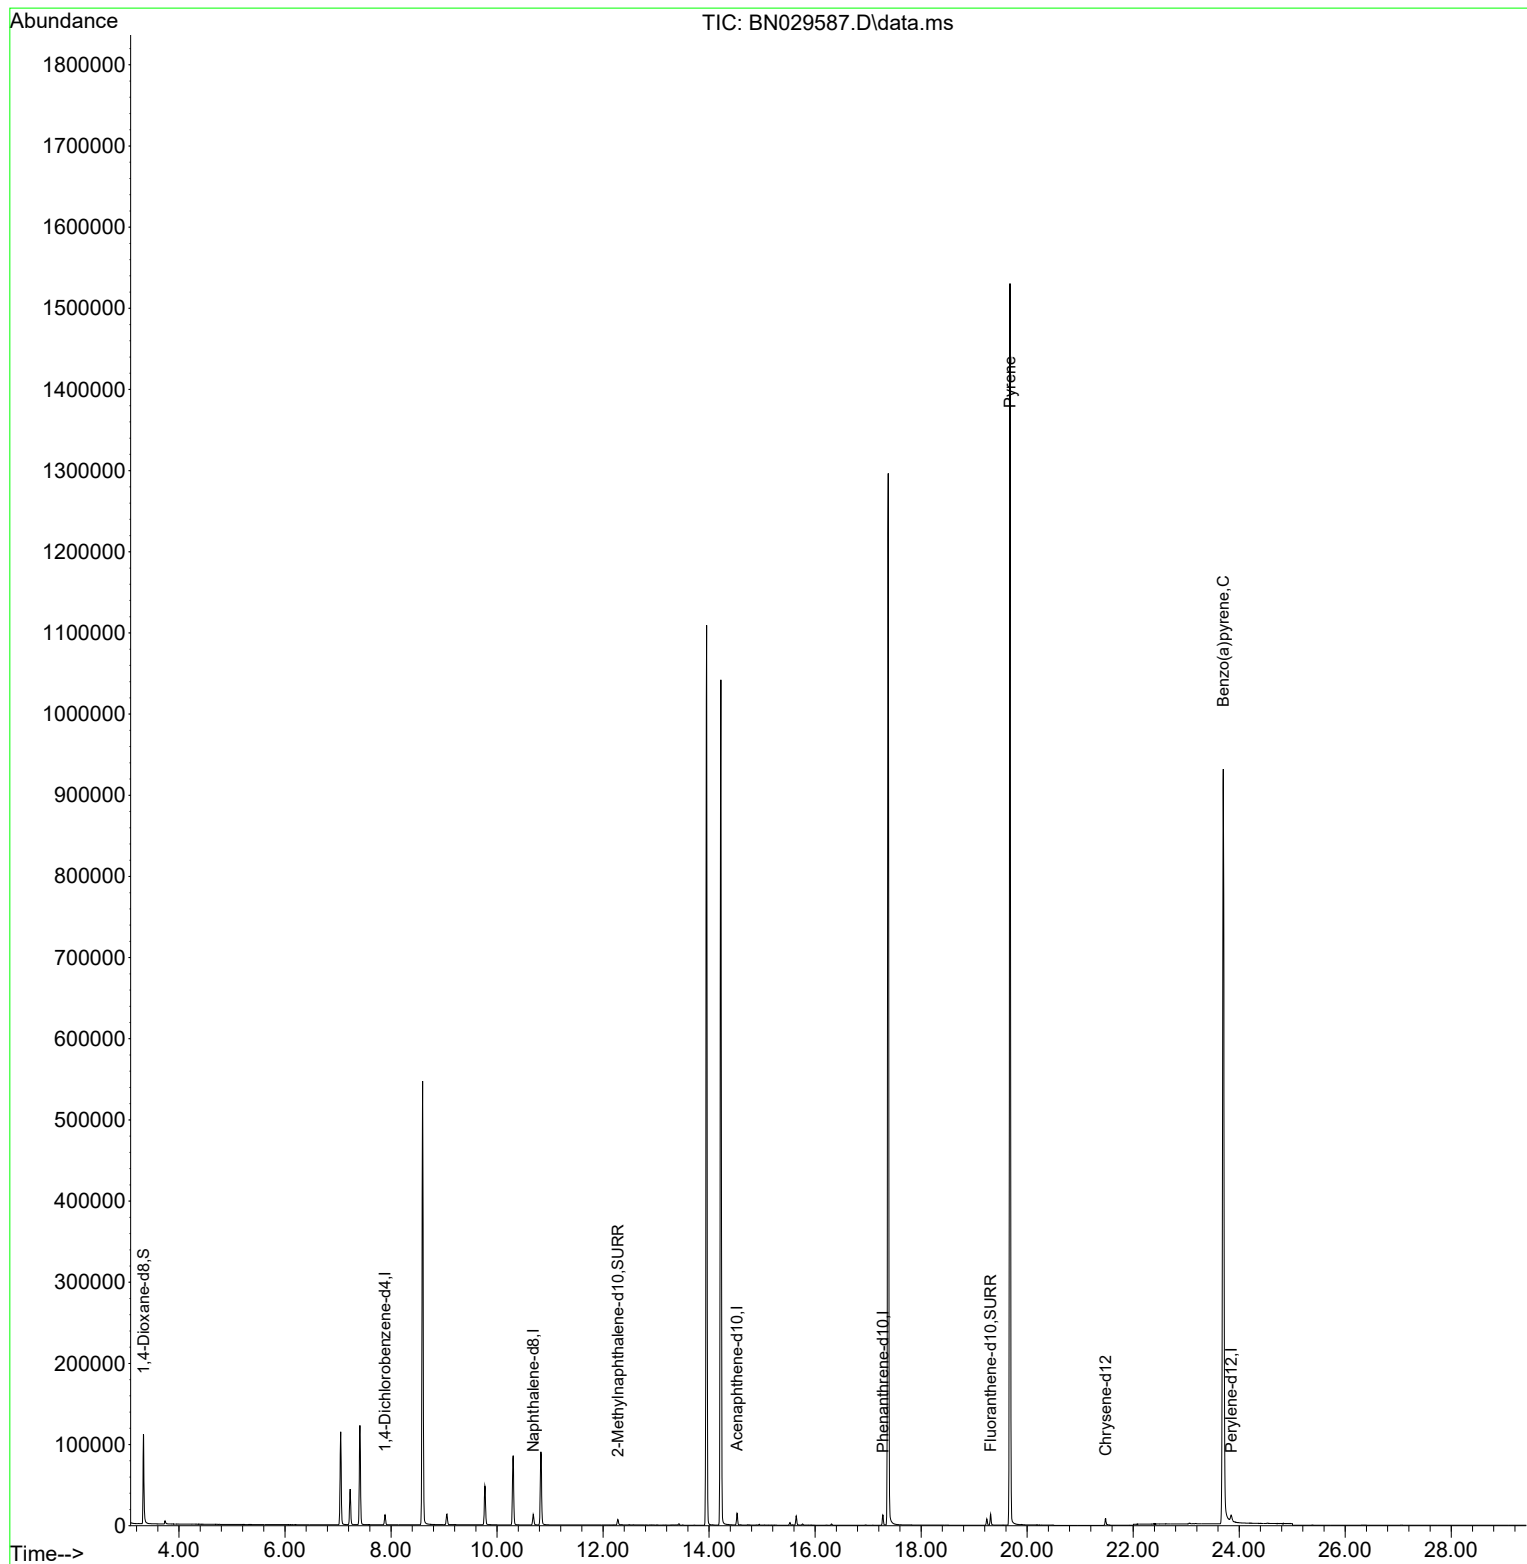

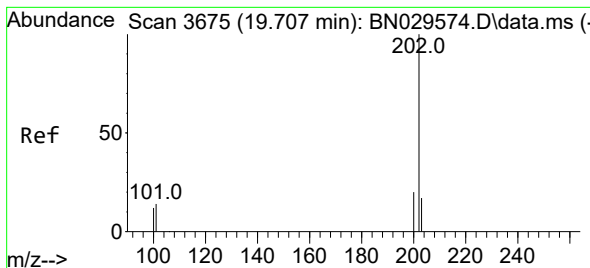

#20

Pyrene

Concen: 0.055 ng/ul

RT: 19.677 min Scan# 3

Delta R.T. -0.032 min

Lab File: BN029587.D

Acq: 08 Feb 2024 21:24

Instrument :





BNA_N

ClientSampleId :

SBLK770

Tgt Ion:202 Resp: 2489

Ion	Ratio	Lower	Upper
202	100		
101	200.5	12.5	18.7#
100	1480.4	10.0	15.0#

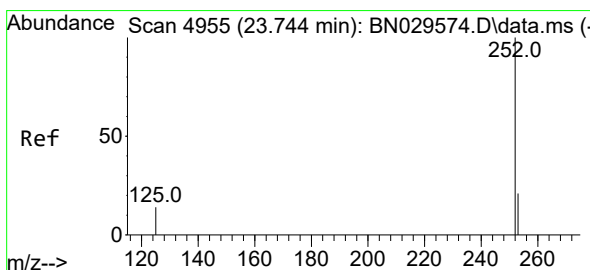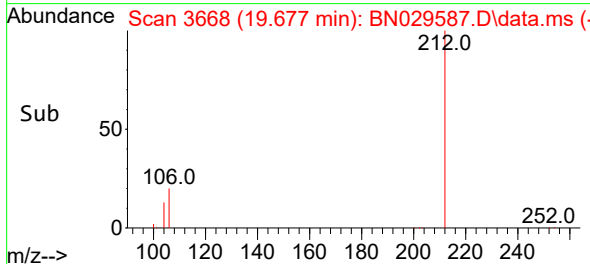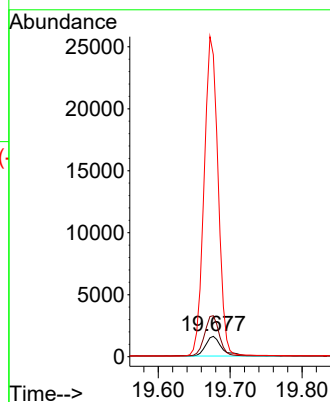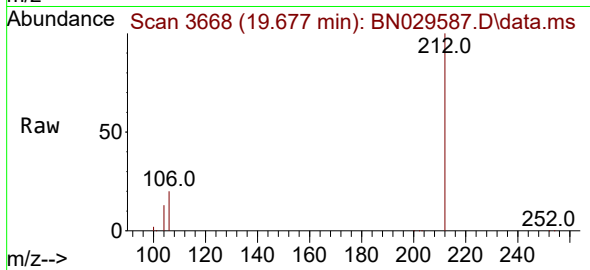

#26

Benzo(a)pyrene

Concen: 0.109 ng/ul

RT: 23.698 min Scan# 4939

Delta R.T. -0.055 min

Lab File: BN029587.D

Acq: 08 Feb 2024 21:24

Tgt Ion:252 Resp: 5230

Ion	Ratio	Lower	Upper
252	100		
253	48.7	25.4	38.0#
125	38.4	16.0	24.0#

