

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
 Data File : BN029588.D
 Acq On : 08 Feb 2024 22:00
 Operator : MA/JU
 Sample : P1303-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FH5

Quant Time: Feb 08 23:59:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 07 02:17:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.884	152	5551	0.400	ng/ul	0.00
4) Naphthalene-d8	10.683	136	15151	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.525	164	7208	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.276	188	14087	0.400	ng/ul	0.00
17) Chrysene-d12	21.476	240	10961	0.400	ng/ul	0.00
23) Perylene-d12	23.846	264	14128	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.332	96	52438	7.576	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.278	152	8199	0.425	ng/ul	0.00
18) Fluoranthene-d10	19.309	212	14474	0.402	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Anthracene	17.378	178	763	0.021	ng/ul#	1
20) Pyrene	19.676	202	2424	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.694	252	4772	0.095	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
Data File : BN029588.D
Acq On : 08 Feb 2024 22:00
Operator : MA/JU
Sample : P1303-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FH5

Quant Time: Feb 08 23:59:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 02:17:13 2024
Response via : Initial Calibration




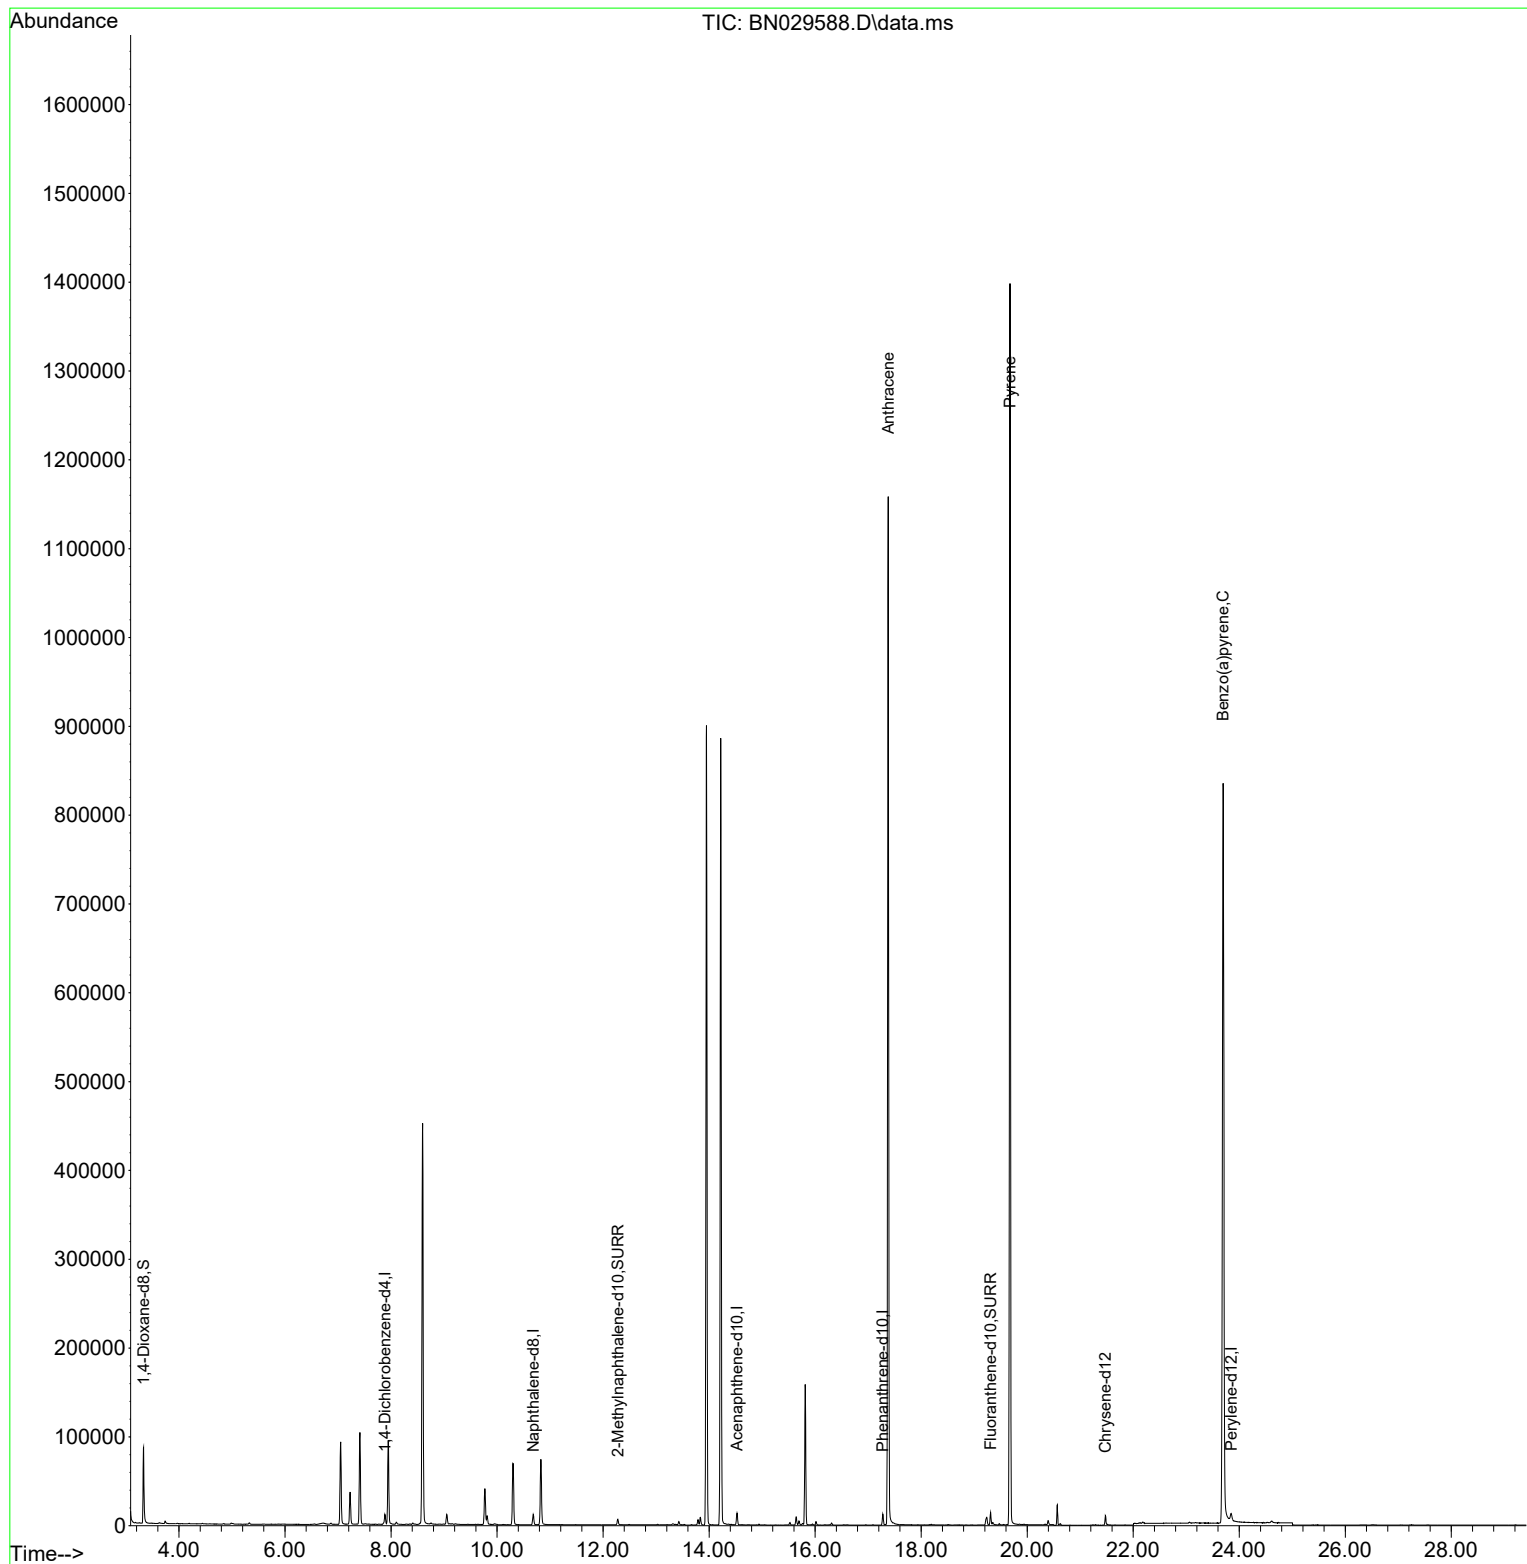


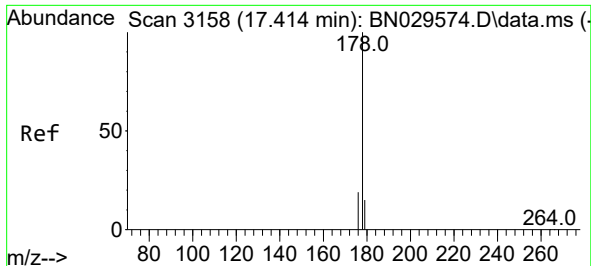

#16
 Anthracene
 Concen: 0.021 ng/ul
 RT: 17.378 min Scan# 3158
 Delta R.T. -0.038 min
 Lab File: BN029588.D
 Acq: 08 Feb 2024 22:00




Instrument :
 BNA_N
 ClientSampleId :
 C0FH5


Tgt Ion:178 Resp: 763
 Ion Ratio Lower Upper
 178 100
 179 205.3 12.9 19.3#
 176 35.9 15.8 23.8#

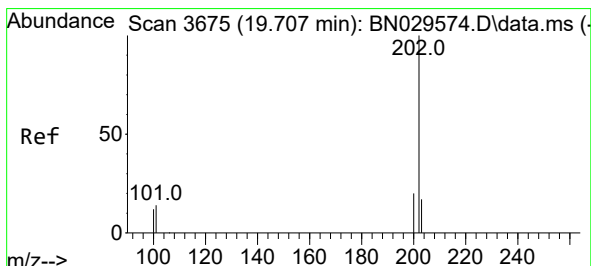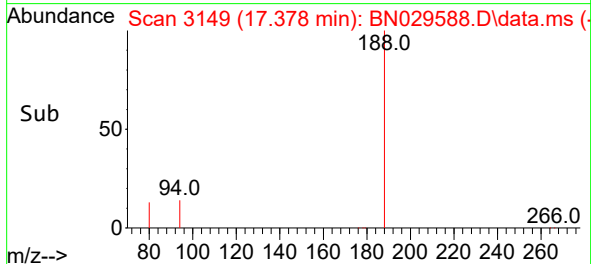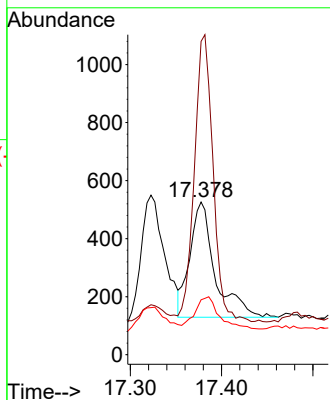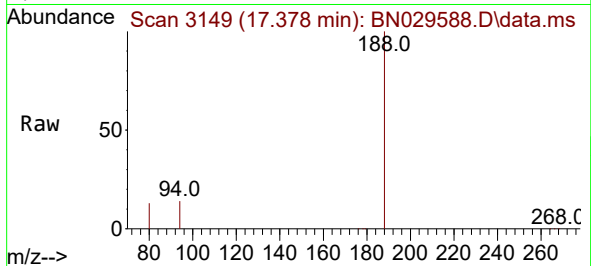

#20
 Pyrene
 Concen: 0.047 ng/ul
 RT: 19.676 min Scan# 3668
 Delta R.T. -0.032 min
 Lab File: BN029588.D
 Acq: 08 Feb 2024 22:00


Tgt Ion:202 Resp: 2424
 Ion Ratio Lower Upper
 202 100
 101 199.9 12.5 18.7#
 100 1467.4 10.0 15.0#

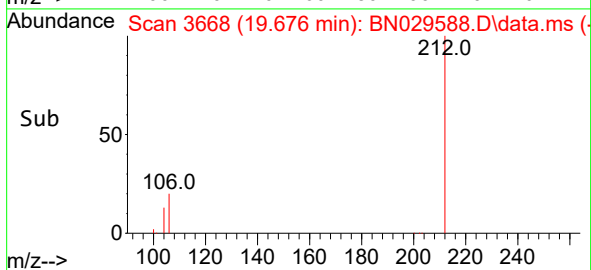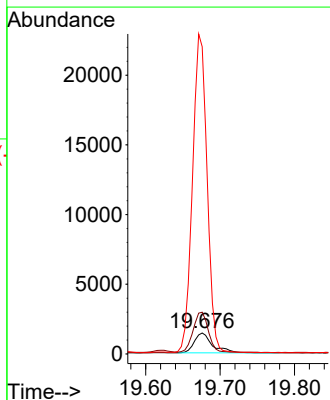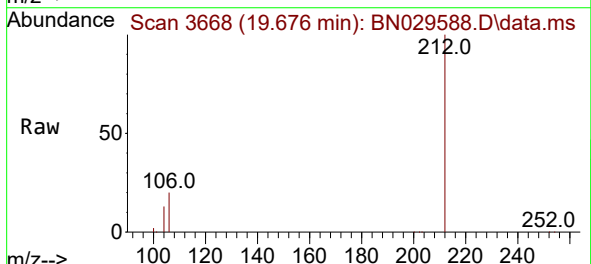

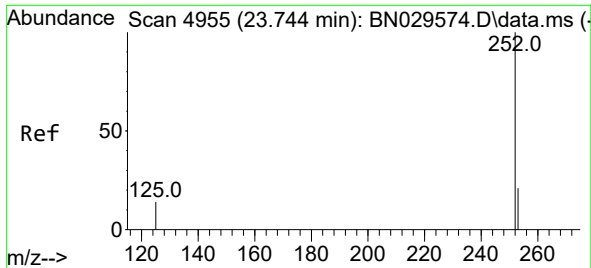

#26
Benzo(a)pyrene
Concen: 0.095 ng/ul
RT: 23.694 min Scan# 4938
Delta R.T. -0.058 min
Lab File: BN029588.D
Acq: 08 Feb 2024 22:00

Instrument :
BNA_N
ClientSampleId :
C0FH5

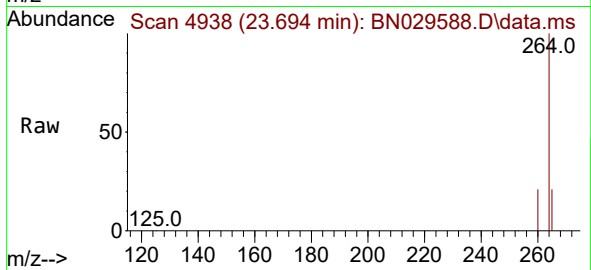

Tgt Ion:252 Resp: 4772
Ion Ratio Lower Upper
252 100
253 58.2 25.4 38.0#
125 40.2 16.0 24.0#

