

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
 Data File : BN029590.D
 Acq On : 08 Feb 2024 23:11
 Operator : MA/JU
 Sample : P1303-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FJ5

Quant Time: Feb 08 23:59:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 07 02:17:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.888	152	5732	0.400	ng/ul	0.00
4) Naphthalene-d8	10.683	136	15909	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.529	164	7241	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.280	188	13208	0.400	ng/ul	0.00
17) Chrysene-d12	21.474	240	9326	0.400	ng/ul	0.00
23) Perylene-d12	23.845	264	12017	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.332	96	54119	7.572	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.278	152	9269	0.458	ng/ul	0.00
18) Fluoranthene-d10	19.309	212	13559	0.442	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.341	202	1028	0.024	ng/ul#	Qvalue 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
Data File : BN029590.D
Acq On : 08 Feb 2024 23:11
Operator : MA/JU
Sample : P1303-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FJ5

Quant Time: Feb 08 23:59:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 02:17:13 2024
Response via : Initial Calibration

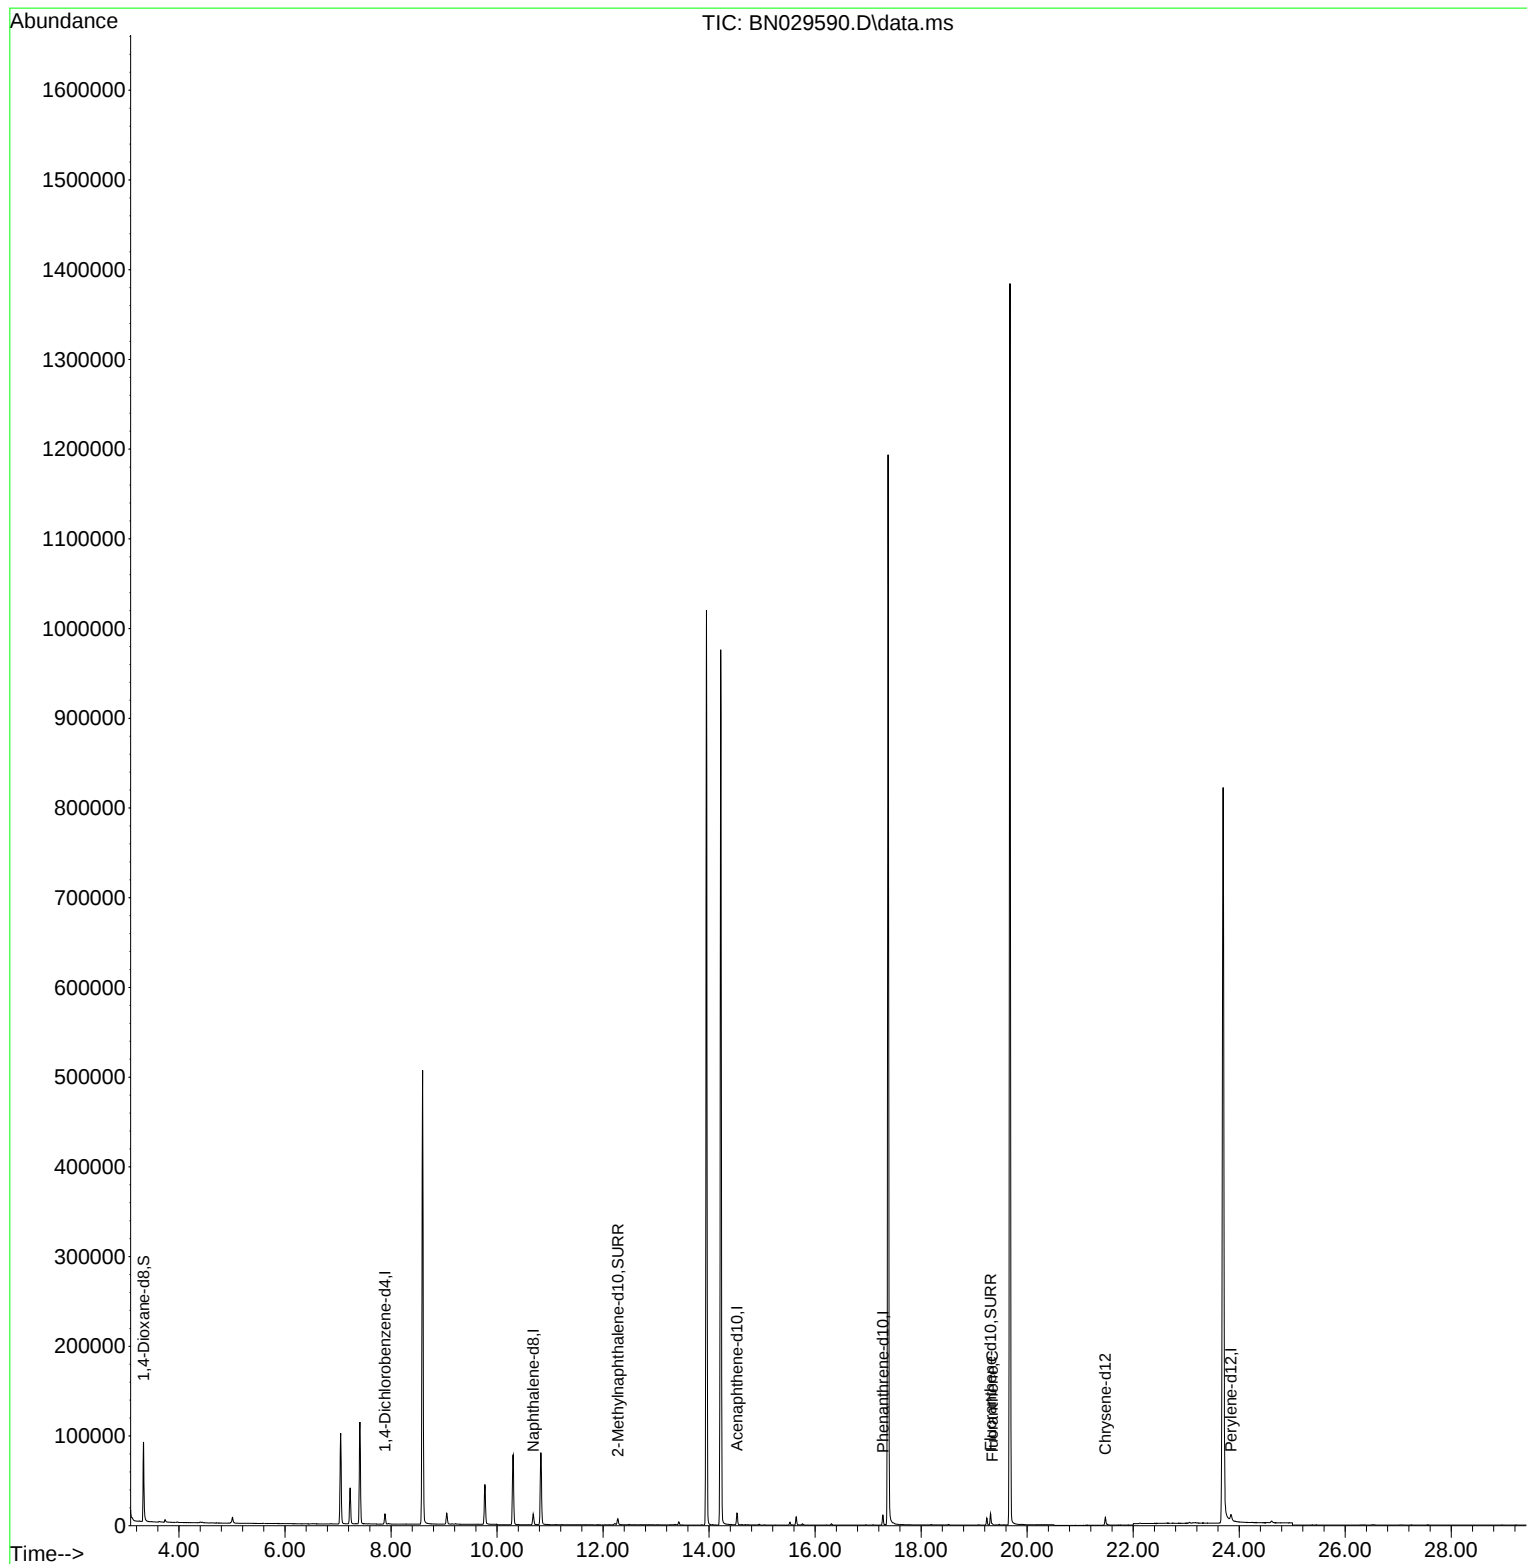

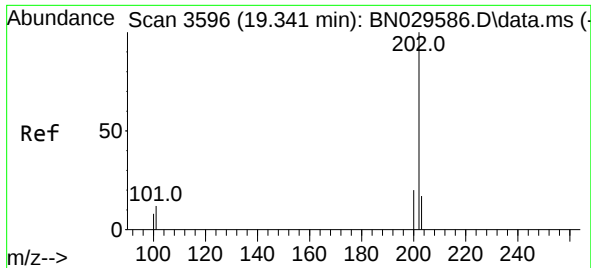

#19

Fluoranthene

Concen: 0.024 ng/ul

RT: 19.341 min Scan# 31

Delta R.T. -0.005 min

Lab File: BN029590.D


Acq: 08 Feb 2024 23:11

Instrument :

BNA_N

ClientSampleId :

C0FJ5

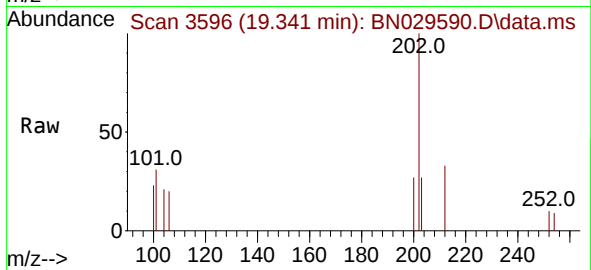

Tgt Ion:202 Resp: 1028

Ion Ratio Lower Upper

202 100

101 31.0 10.4 15.6#

100 22.7 8.5 12.7#

