

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
 Data File : BN029593.D
 Acq On : 09 Feb 2024 00:59
 Operator : MA/JU
 Sample : P1303-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0FH3

Quant Time: Feb 09 01:47:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 07 02:17:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.888	152	5985	0.400	ng/ul	0.00
4) Naphthalene-d8	10.683	136	16394	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.525	164	7432	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.276	188	14047	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.474	240	9750	0.400	ng/ul	0.00
23) Perylene-d12	23.845	264	12247	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.332	96	31498	4.221	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.278	152	5446	0.261	ng/ul	0.00
18) Fluoranthene-d10	19.308	212	9247	0.289	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.318	178	1007	0.023	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020824\
Data File : BN029593.D
Acq On : 09 Feb 2024 00:59
Operator : MA/JU
Sample : P1303-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0FH3


Quant Time: Feb 09 01:47:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 02:17:13 2024
Response via : Initial Calibration

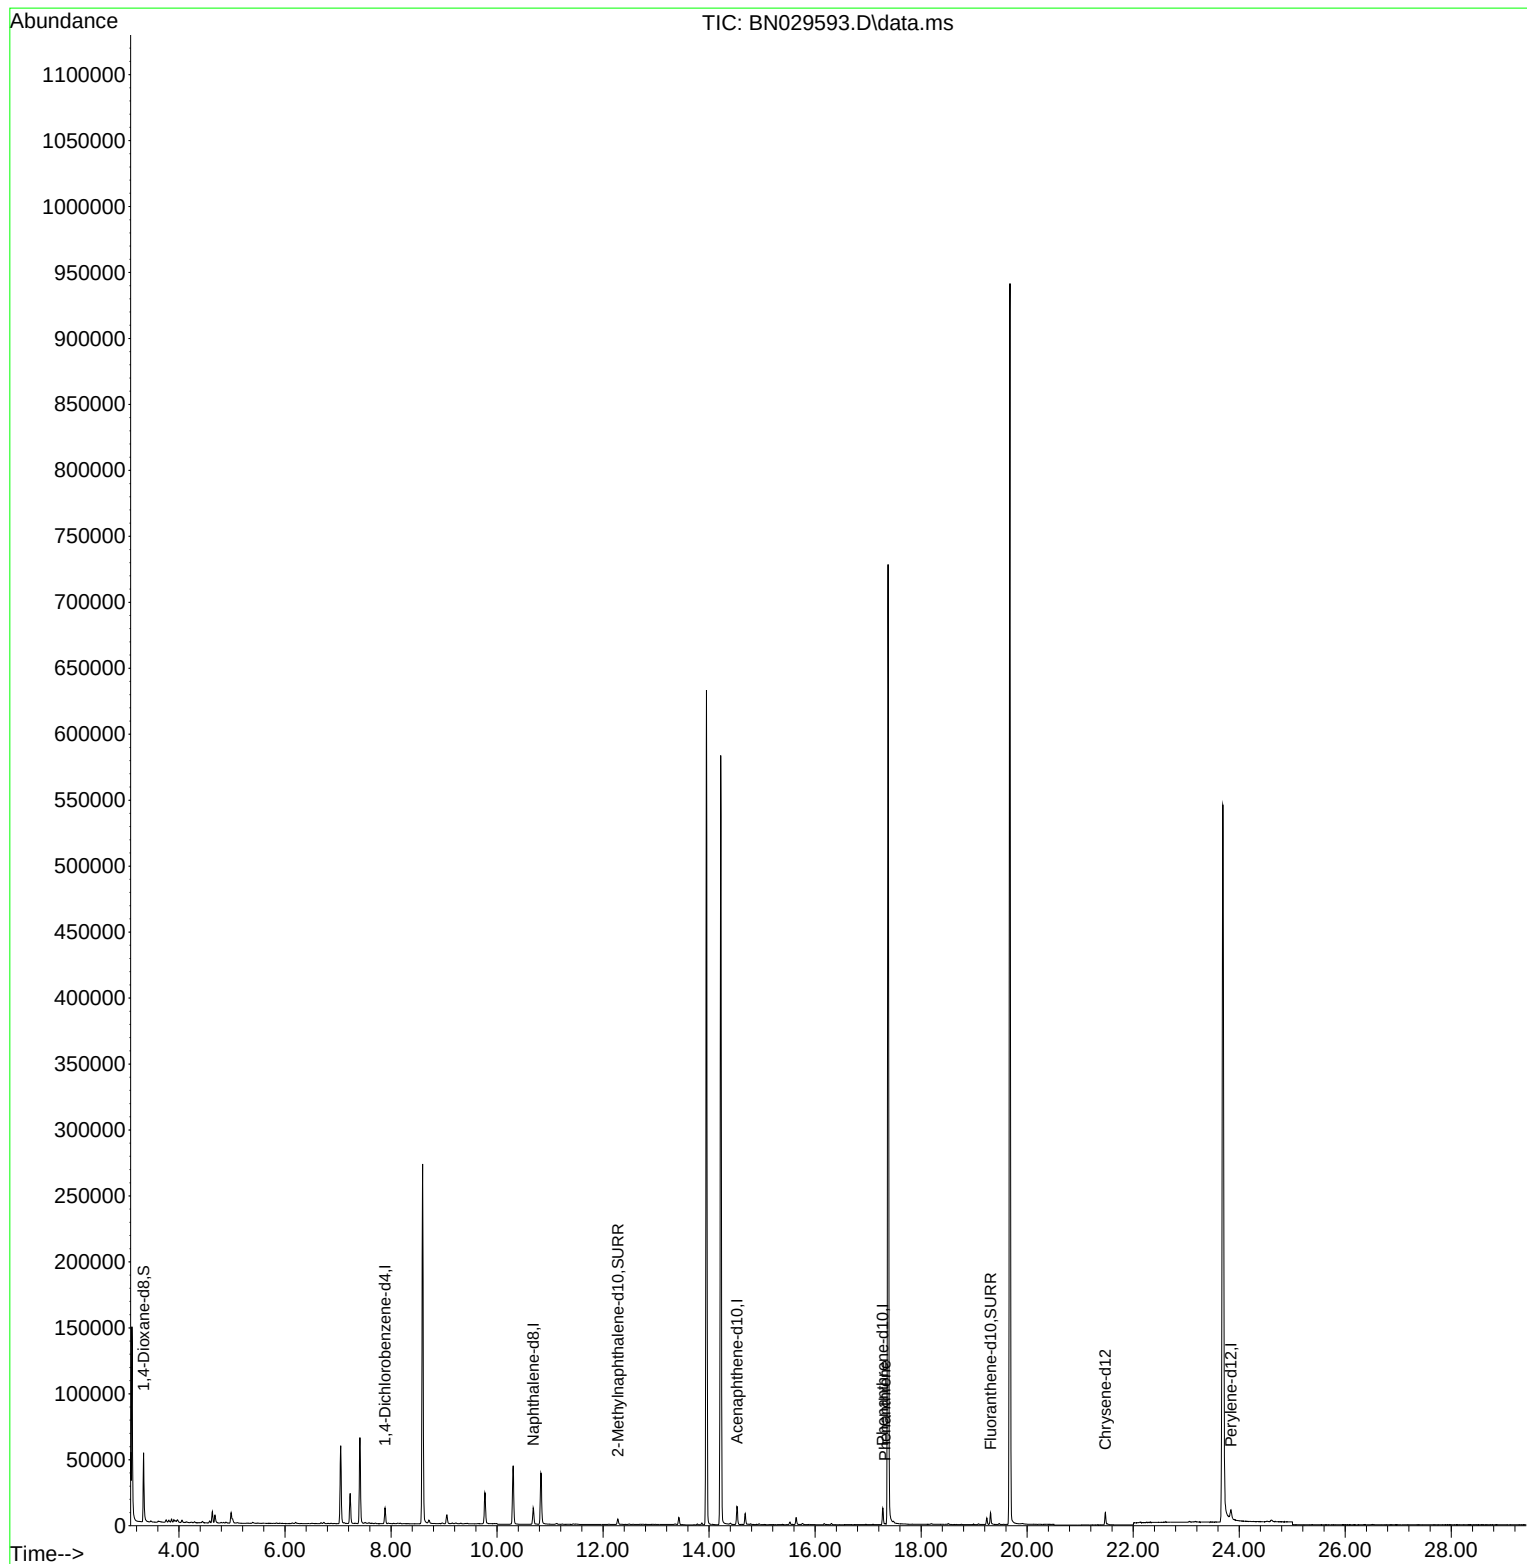

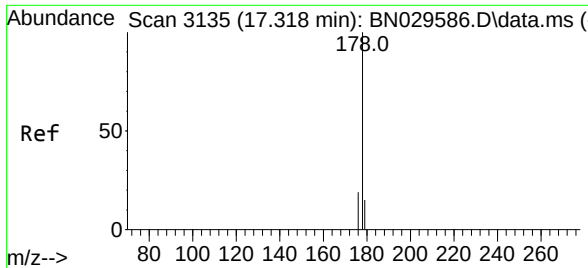

#15
Phenanthrene
Concen: 0.023 ng/ul
RT: 17.318 min Scan# 3135
Delta R.T. -0.009 min
Lab File: BN029593.D
Acq: 09 Feb 2024 00:59

Instrument :
BNA_N
ClientSampleId :
C0FH3

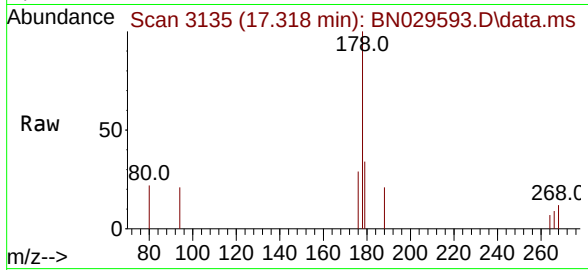

Tgt Ion:178 Resp: 1007
Ion Ratio Lower Upper
178 100
179 34.2 12.6 18.8#
176 29.4 15.7 23.5#

