


Data Path : Z:\HPCHEM1\BNA N\Data\BN020918\
 Data File : BN000049.D
 Acq On : 09 Feb 2018 09:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 18:24:45 2018

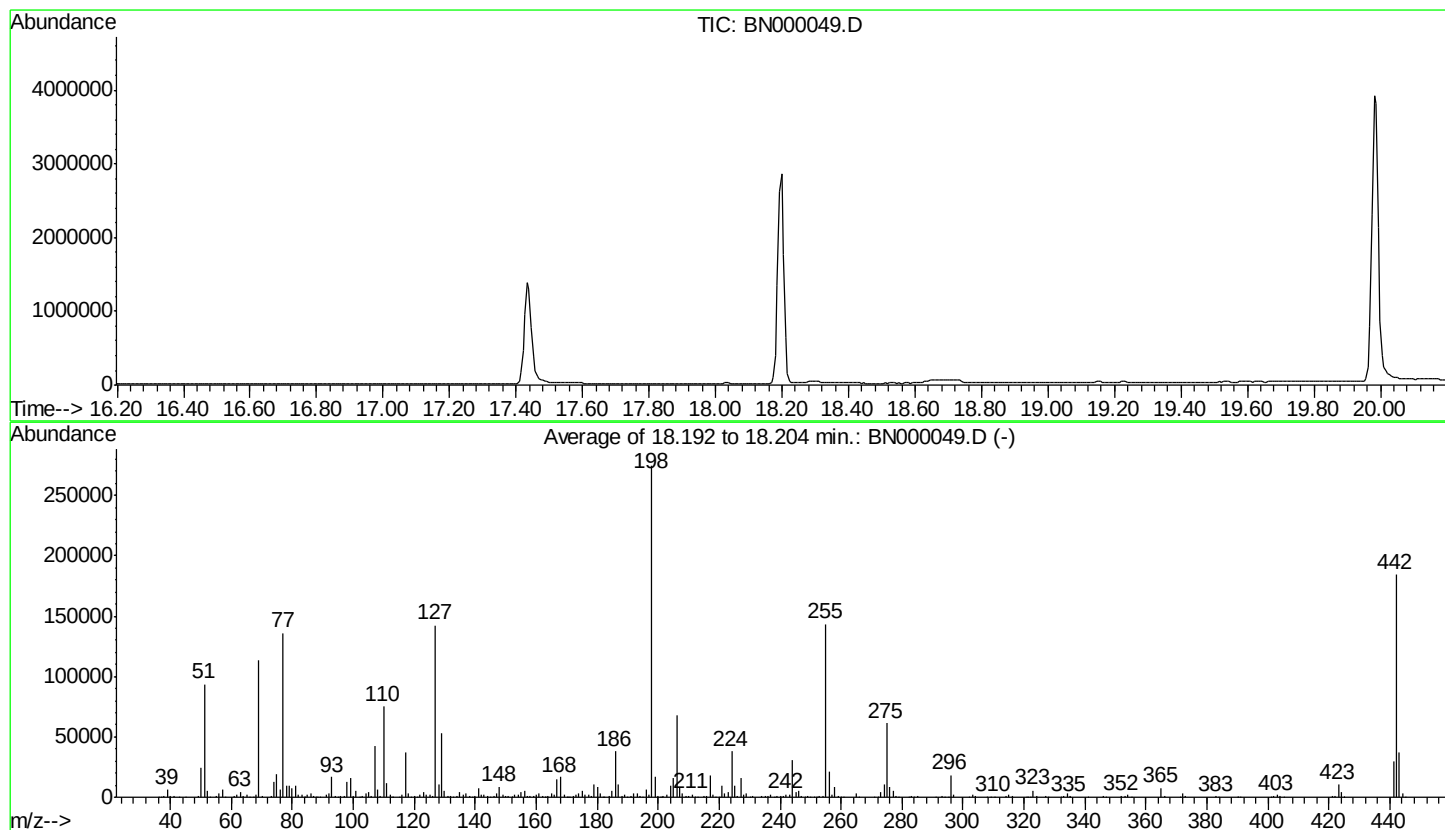

AutoFind: Scans 2585, 2586, 2587; Background Corrected with Scan 2578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	93602	PASS
68	69	0.00	2	1.9	2170	PASS
69	198	0.00	100	41.4	113712	PASS
70	69	0.00	2	0.6	654	PASS
127	198	10	80	51.9	142645	PASS
197	198	0.00	2	0.6	1779	PASS
198	198	100	100	100.0	274730	PASS
199	198	5	9	6.4	17532	PASS
275	198	10	60	22.2	61093	PASS
365	198	1	100	2.8	7807	PASS
441	443	0.01	100	81.1	29714	PASS
442	198	50	100	67.1	184448	PASS
443	442	15	24	19.9	36653	PASS