

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029619.D
 Acq On : 09 Feb 2024 20:32
 Operator : MA/JU
 Sample : P1398-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG0

Quant Time: Feb 09 21:44:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	197503	20.000	ng/ul	0.00
20) Naphthalene-d8	10.675	136	784651	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.522	164	372817	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.275	188	648477	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	537493	20.000	ng/ul	0.00
88) Perylene-d12	23.845	264	617104	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	24113	4.016	ng/uL	0.00
4) Pyridine-d5	3.740	84	170494	10.647	ng/ul	0.00
7) Phenol-d5	7.046	99	129732	7.023	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	466679	37.852	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	395191	29.521	ng/ul	-0.01
15) 4-Methylphenol-d8	8.587	113	238598	17.318	ng/ul	-0.01
21) Nitrobenzene-d5	9.046	128	246786	40.524	ng/ul	0.00
24) 2-Nitrophenol-d4	9.763	143	214467	40.436	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.299	165	359086	34.300	ng/ul	0.00
31) 4-Chloroaniline-d4	10.822	131	566629	31.726	ng/ul	-0.01
46) Dimethylphthalate-d6	13.945	166	1120242	40.360	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	1360988	41.288	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	17580	3.337	ng/ul	-0.01
60) Fluorene-d10	15.516	176	934281	39.566	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200	96400	30.509	ng/ul	0.00
73) Anthracene-d10	17.375	188	1360437	44.764	ng/ul	0.00
81) Pyrene-d10	19.669	212	1425756	44.202	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.692	264	1388005	44.950	ng/ul	-0.01
Target Compounds						
48) 2,6-Dinitrotoluene	13.945	165	7622	1.499	ng/ul#	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029619.D
Acq On : 09 Feb 2024 20:32
Operator : MA/JU
Sample : P1398-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG0


Quant Time: Feb 09 21:44:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

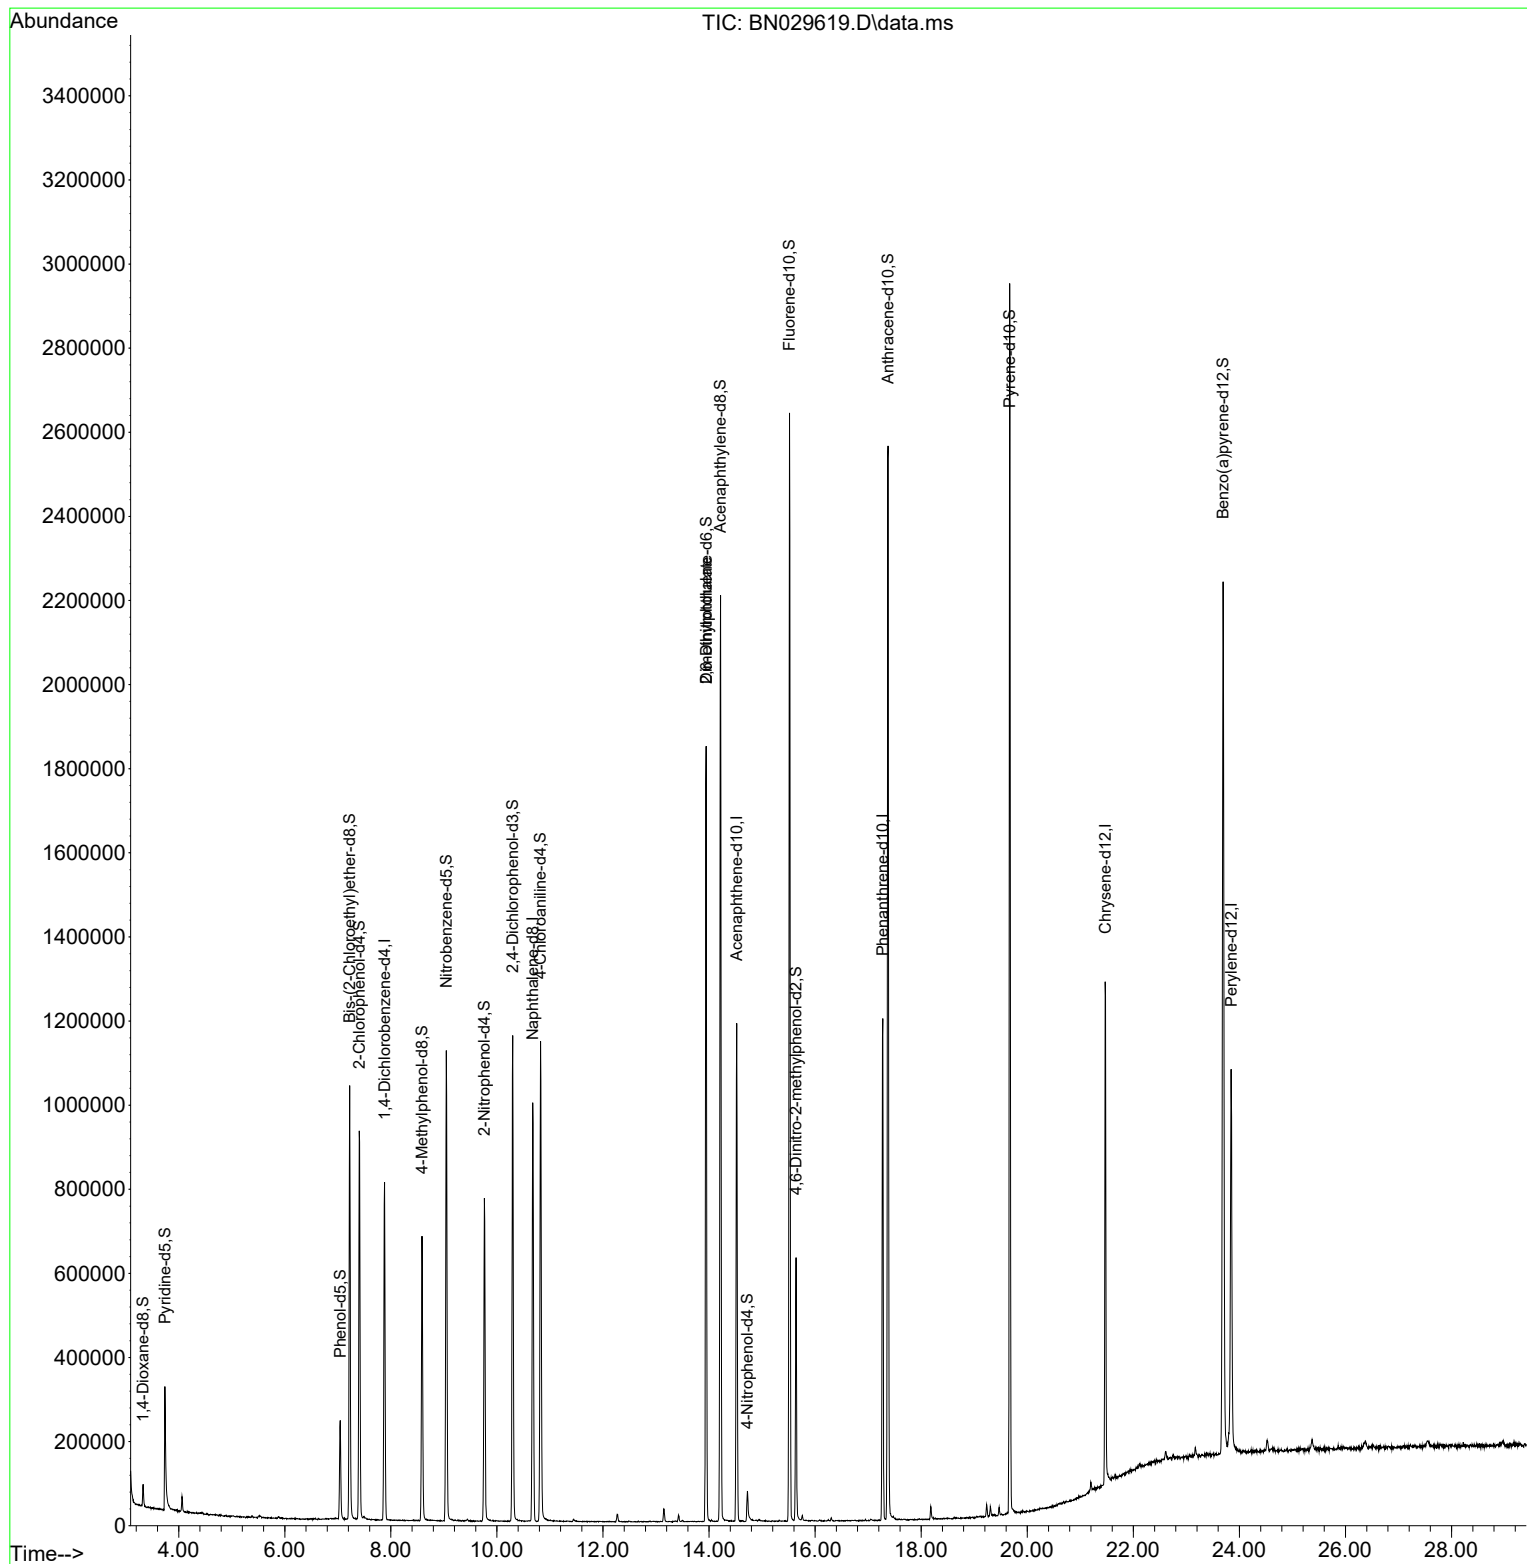

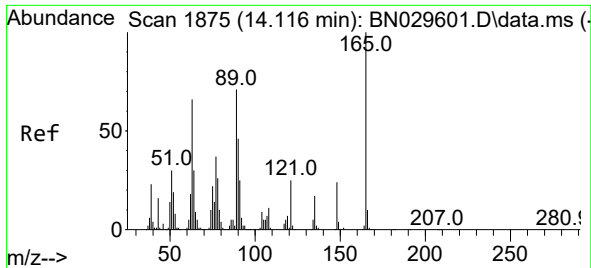

#48
 2,6-Dinitrotoluene
 Concen: 1.499 ng/ul
 RT: 13.945 min Scan# 11
 Delta R.T. -0.176 min
 Lab File: BN029619.D
 Acq: 09 Feb 2024 20:32

Instrument :
 BNA_N
 ClientSampleId :
 C0AG0

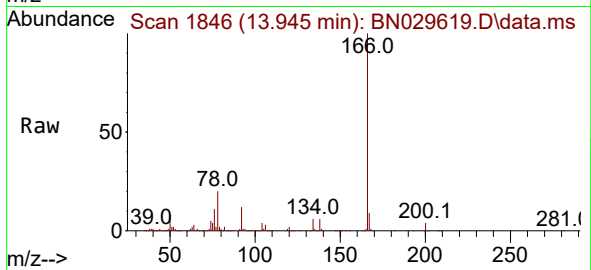

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	55.8	83.8#
121	34.9	19.8	29.6#

