

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029634.D
 Acq On : 10 Feb 2024 06:09
 Operator : MA/JU
 Sample : P1398-18
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH2

Quant Time: Feb 11 22:09:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	210501	20.000	ng/ul	0.00
20) Naphthalene-d8	10.681	136	833755	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	405500	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.275	188	729262	20.000	ng/ul	0.00
79) Chrysene-d12	21.469	240	554870	20.000	ng/ul	-0.01
88) Perylene-d12	23.845	264	656684	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	25687	4.014	ng/uL	0.00
4) Pyridine-d5	3.740	84	117064	6.859	ng/ul	0.00
7) Phenol-d5	7.046	99	126098	6.404	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	467741	35.595	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	400483	28.069	ng/ul	-0.01
15) 4-Methylphenol-d8	8.587	113	233502	15.902	ng/ul	-0.01
21) Nitrobenzene-d5	9.046	128	254062	39.262	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	227111	40.298	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.299	165	363941	32.716	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	550932	29.030	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	1122986	37.197	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	1334824	37.231	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	17508	3.056	ng/ul	0.00
60) Fluorene-d10	15.516	176	934243	36.376	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200	102778	28.924	ng/ul	0.00
73) Anthracene-d10	17.375	188	1325448	38.781	ng/ul	0.00
81) Pyrene-d10	19.669	212	1365130	40.997	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.698	264	1320304	40.180	ng/ul	0.00
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	13.945	165	8004	1.447	ng/ul#	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029634.D
Acq On : 10 Feb 2024 06:09
Operator : MA/JU
Sample : P1398-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH2


Quant Time: Feb 11 22:09:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

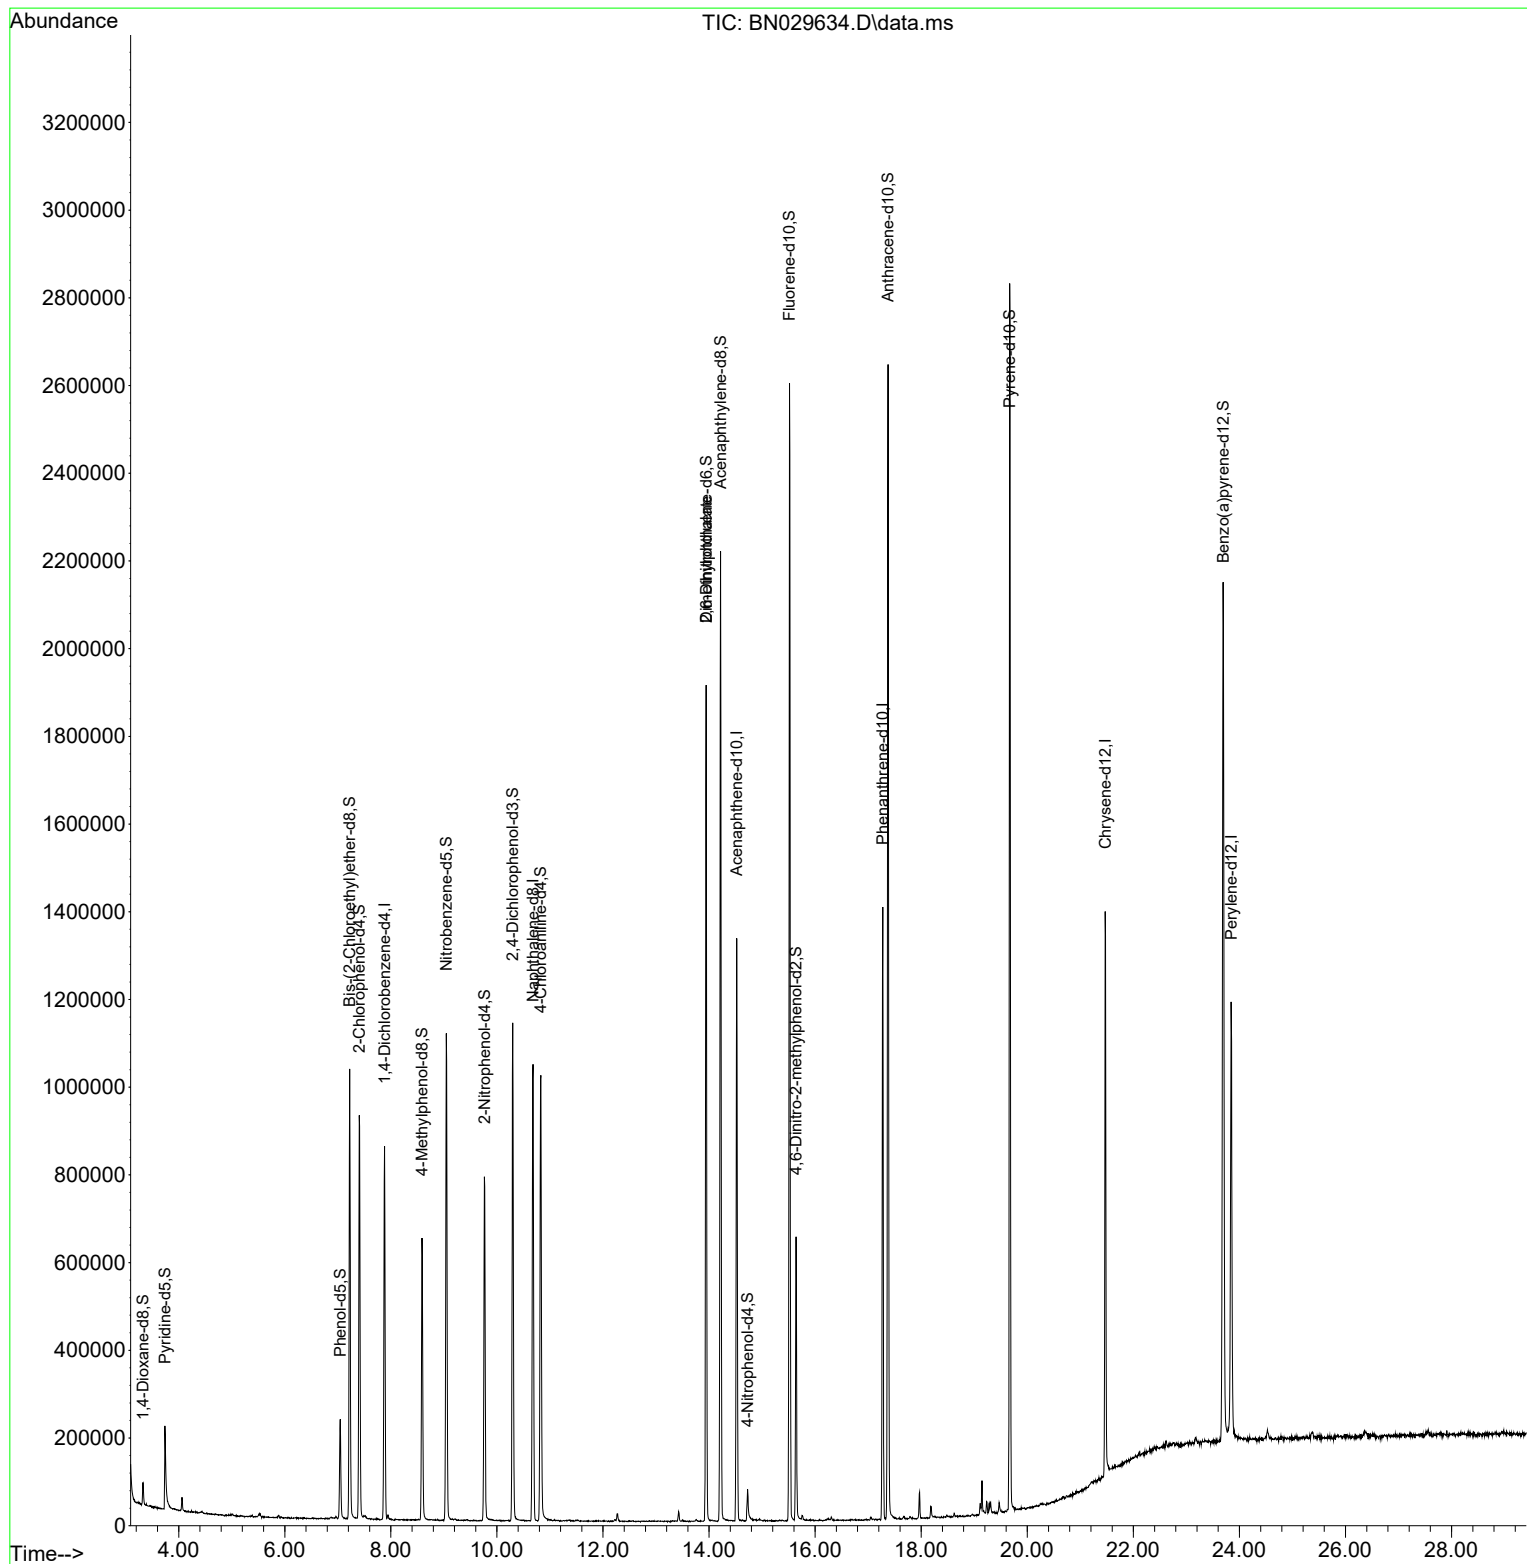

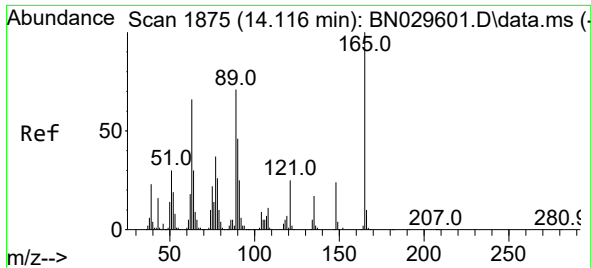

#48
 2,6-Dinitrotoluene
 Concen: 1.447 ng/ul
 RT: 13.945 min Scan# 11
 Delta R.T. -0.176 min
 Lab File: BN029634.D
 Acq: 10 Feb 2024 06:09

Instrument :
 BNA_N
 ClientSampleId :
 C0AH2

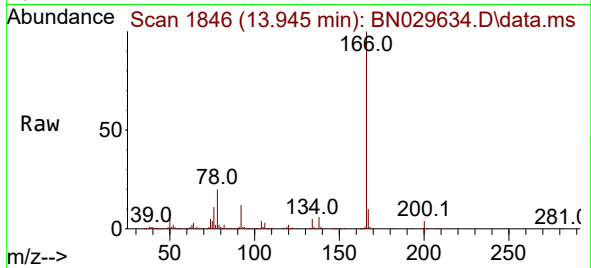

Tgt Ion:	165	Resp:	8004
Ion	Ratio	Lower	Upper
165	100		
89	3.4	55.8	83.8#
121	41.7	19.8	29.6#

