

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029652.D
 Acq On : 10 Feb 2024 17:36
 Operator : MA/JU
 Sample : P1399-10
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ3

Quant Time: Feb 11 22:13:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	220564	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.675	136	893776	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.522	164	427104	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.269	188	750506	20.000	ng/ul	-0.01
79) Chrysene-d12	21.469	240	536363	20.000	ng/ul	-0.01
88) Perylene-d12	23.845	264	639542	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	30091	4.487	ng/uL	0.00
4) Pyridine-d5	3.746	84	99534	5.566	ng/ul	0.00
7) Phenol-d5	7.046	99	193575	9.383	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	576092	41.841	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	512437	34.277	ng/ul	-0.01
15) 4-Methylphenol-d8	8.587	113	325001	21.123	ng/ul	-0.01
21) Nitrobenzene-d5	9.046	128	308598	44.487	ng/ul	0.00
24) 2-Nitrophenol-d4	9.763	143	285110	47.192	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.293	165	468001	39.246	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.822	131	620239	30.487	ng/ul	-0.01
46) Dimethylphthalate-d6	13.940	166	1412652	44.425	ng/ul	-0.01
49) Acenaphthylene-d8	14.210	160	1679624	44.478	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.722	143	27130	4.495	ng/ul	-0.01
60) Fluorene-d10	15.516	176	1143020	42.254	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.640	200	125530	34.327	ng/ul	0.00
73) Anthracene-d10	17.369	188	1598461	45.445	ng/ul	-0.01
81) Pyrene-d10	19.669	212	1595638	49.573	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.692	264	1509955	47.183	ng/ul	-0.01
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	13.945	165	9653	1.657	ng/ul#	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029652.D
Acq On : 10 Feb 2024 17:36
Operator : MA/JU
Sample : P1399-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ3


Quant Time: Feb 11 22:13:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

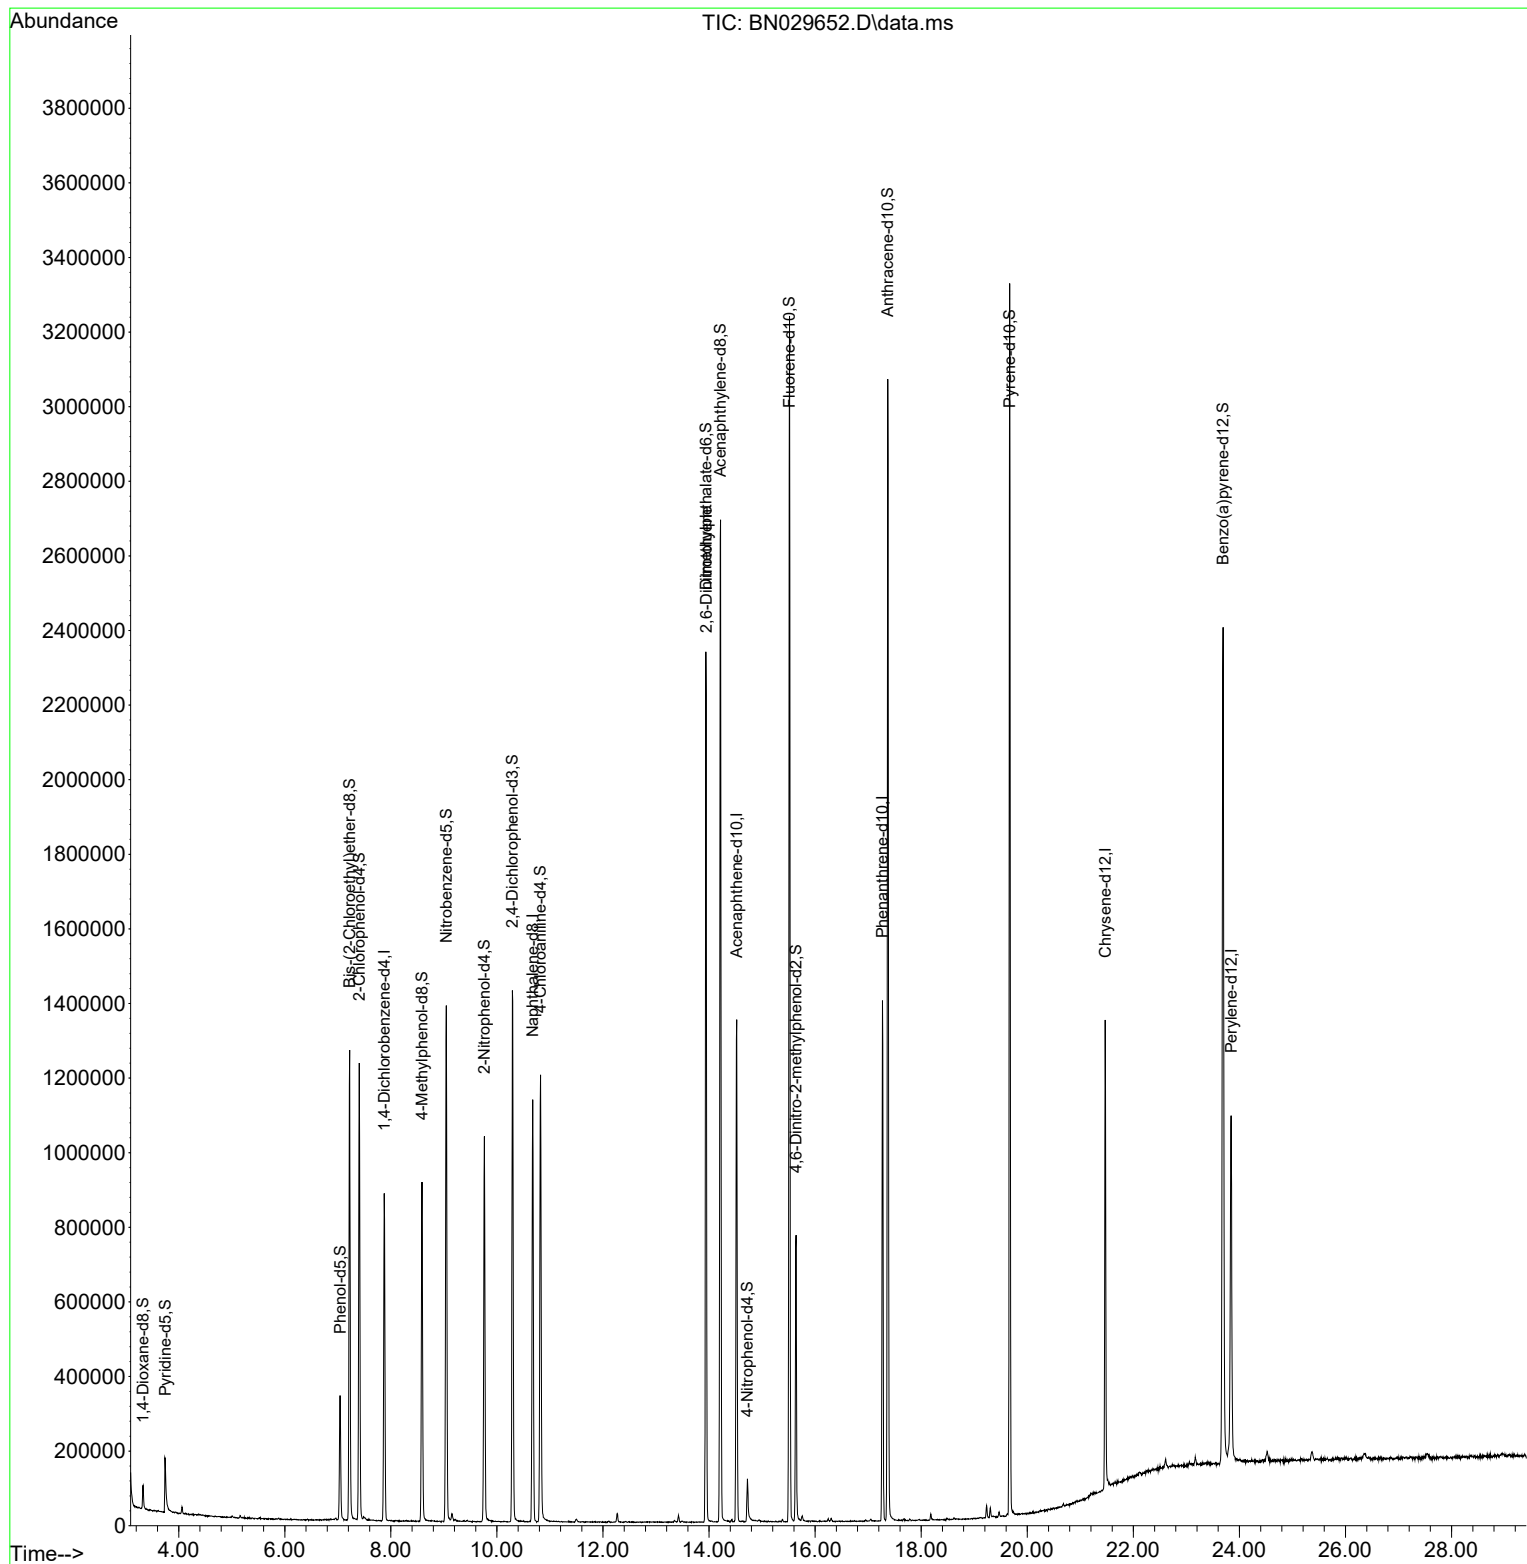

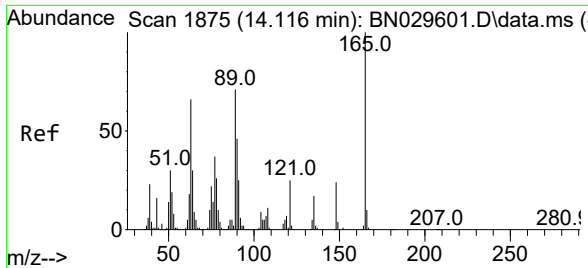

#48
 2,6-Dinitrotoluene
 Concen: 1.657 ng/ul
 RT: 13.945 min Scan# 11
 Delta R.T. -0.176 min
 Lab File: BN029652.D
 Acq: 10 Feb 2024 17:36

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ3

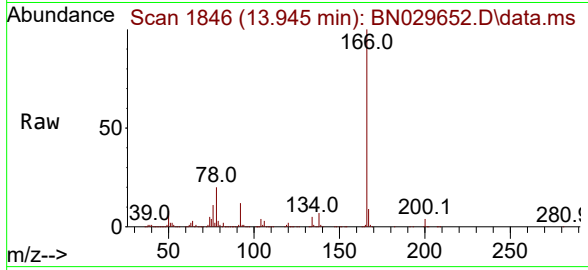

Tgt Ion:	165	Resp:	9653
Ion	Ratio	Lower	Upper
165	100		
89	2.5	55.8	83.8#
121	41.2	19.8	29.6#

