

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029602.D
 Acq On : 09 Feb 2024 10:20
 Operator : MA/JU
 Sample : PB158824BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK824

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	49	rVB	85969	109016	3.22%	0.232%
2	3.734	107	110	129	rBV	941856	1453082	42.86%	3.086%
3	4.064	162	166	170	rVB	22938	31721	0.94%	0.067%
4	7.046	666	673	684	rBV	1092211	1726495	50.93%	3.667%
5	7.222	697	703	715	rVB	918144	1418945	41.86%	3.013%
6	7.405	727	734	742	rBV	1081401	1728493	50.99%	3.671%
7	7.881	808	815	825	rVB	899604	1425606	42.05%	3.028%
8	8.587	928	935	948	rBV	1252652	2005957	59.17%	4.260%
9	9.046	1006	1013	1025	rBV	965855	1601956	47.26%	3.402%
10	9.763	1128	1135	1148	rVV	696218	1162108	34.28%	2.468%
11	10.299	1218	1226	1241	rBV	1139770	1885172	55.61%	4.004%
12	10.681	1282	1291	1302	rVB	1129226	1940116	57.23%	4.120%
13	10.822	1306	1315	1329	rBV	1138776	1998908	58.97%	4.245%
14	11.134	1367	1368	1374	rVB6	2999	3992	0.12%	0.008%
15	12.269	1557	1561	1568	rVV3	15707	28461	0.84%	0.060%
16	13.428	1752	1758	1762	rBV4	12015	18162	0.54%	0.039%
17	13.498	1765	1770	1773	rBV6	2994	5237	0.15%	0.011%
18	13.945	1839	1846	1854	rBV	1599314	2278903	67.23%	4.840%
19	14.216	1885	1892	1901	rBV	2006996	2901151	85.58%	6.161%
20	14.522	1937	1944	1953	rBV	1419413	2064375	60.90%	4.384%
21	14.722	1970	1978	1995	rBV	614064	969972	28.61%	2.060%
22	14.945	2013	2016	2019	rVB5	3806	5387	0.16%	0.011%
23	15.516	2105	2113	2127	rBV	2304430	3301124	97.38%	7.011%
24	15.640	2127	2134	2146	rVV	529196	730673	21.55%	1.552%
25	15.757	2150	2154	2159	rVB4	10286	14997	0.44%	0.032%
26	16.304	2242	2247	2253	rVB7	7260	12735	0.38%	0.027%
27	16.957	2352	2358	2361	rVB5	5130	7242	0.21%	0.015%
28	17.275	2405	2412	2419	rBV	1459909	2072741	61.14%	4.402%
29	17.375	2422	2429	2441	rBV	2249262	3230711	95.30%	6.861%
30	18.192	2563	2568	2572	rBV6	5640	10670	0.31%	0.023%
31	19.233	2741	2745	2750	rVV3	22671	31183	0.92%	0.066%
32	19.304	2754	2757	2762	rVB2	21504	28739	0.85%	0.061%
33	19.404	2772	2774	2776	rBV2	4281	4150	0.12%	0.009%
34	19.469	2783	2785	2788	rBV4	4478	4576	0.13%	0.010%
35	19.669	2813	2819	2827	rBV	2474878	3389926	100.00%	7.199%
36	21.469	3120	3125	3140	rBV	1390432	1968979	58.08%	4.182%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029602.D
Acq On : 09 Feb 2024 10:20
Operator : MA/JU
Sample : PB158824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	23.692	3496	3503	3517	rBV2	1724434	3361501	99.16%	7.139%
38	23.845	3522	3529	3541	rVB	1090734	2154005	63.54%	4.575%




Sum of corrected areas: 47087167

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029602.D
Acq On : 09 Feb 2024 10:20
Operator : MA/JU
Sample : PB158824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

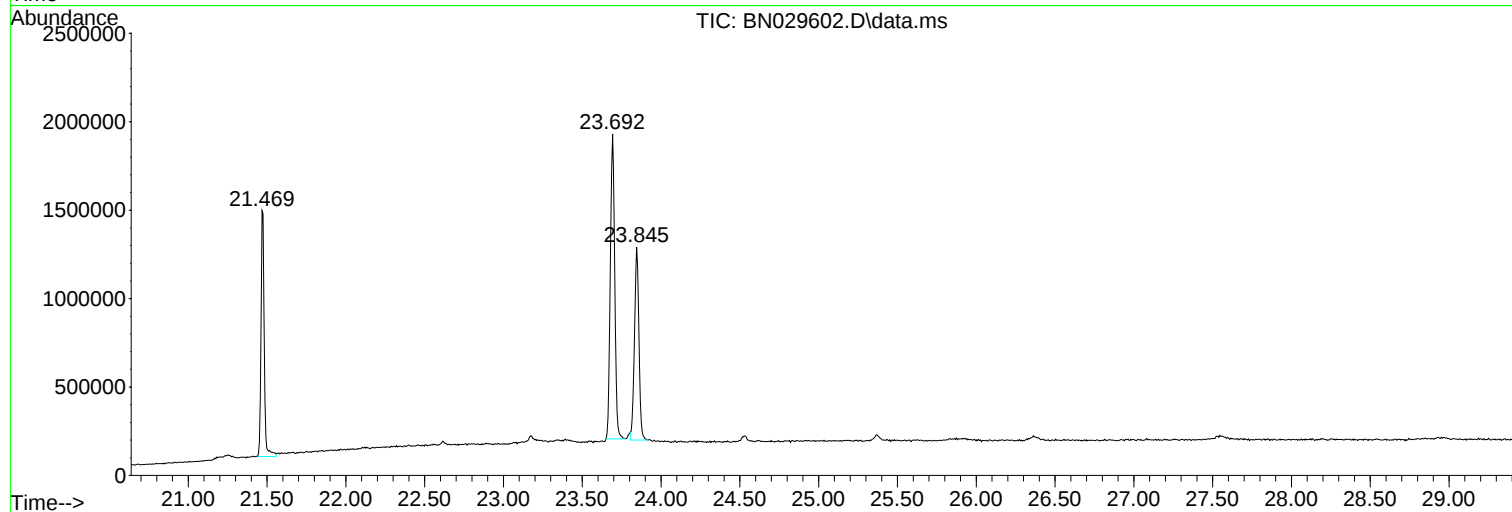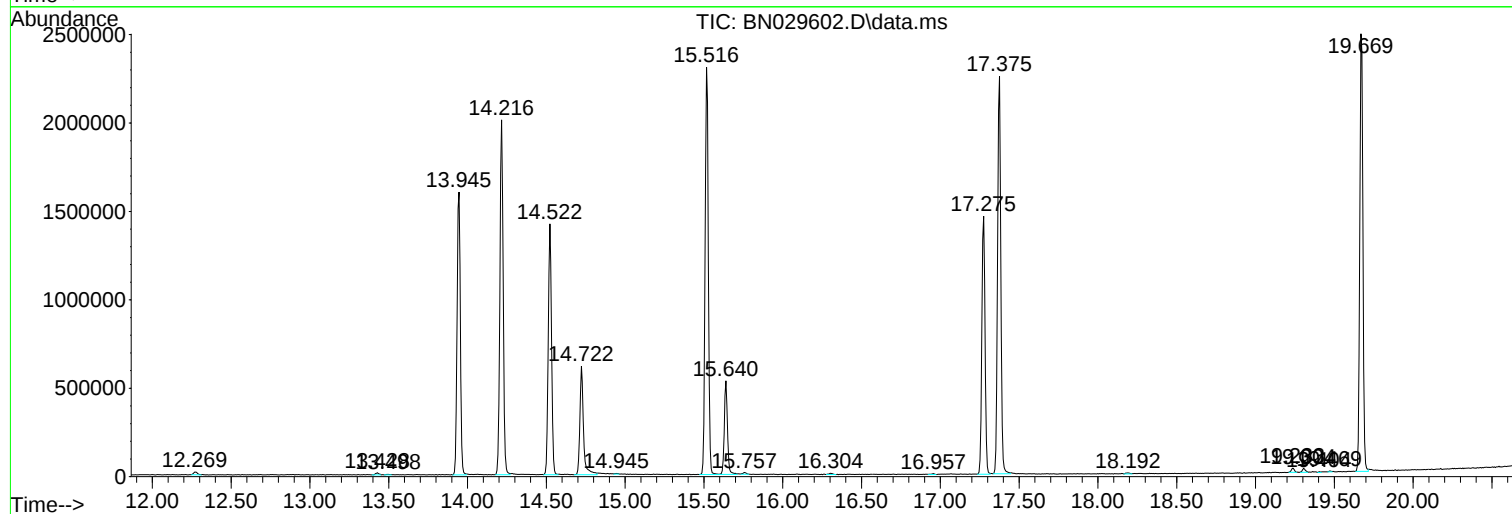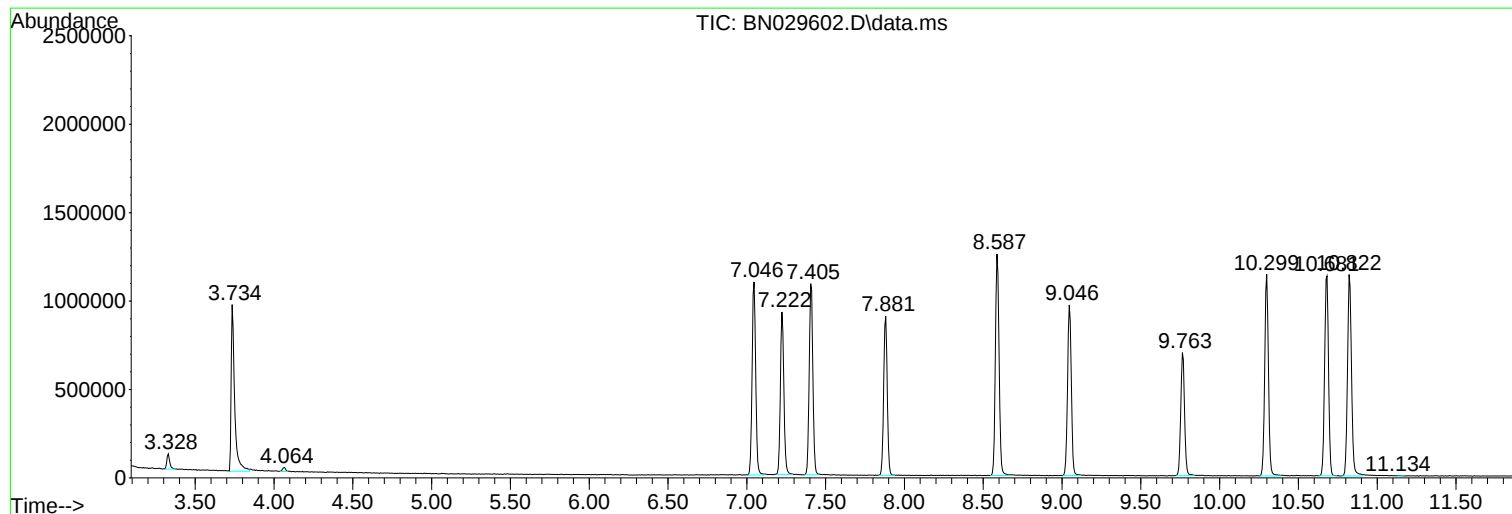

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029602.D
Acq On : 09 Feb 2024 10:20
Operator : MA/JU
Sample : PB158824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029602.D
Acq On : 09 Feb 2024 10:20
Operator : MA/JU
Sample : PB158824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------