

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029608.D
 Acq On : 09 Feb 2024 13:56
 Operator : MA/JU
 Sample : P1348-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	48	rVB	55405	74929	1.66%	0.169%
2	3.740	108	111	129	rBV	211494	363957	8.06%	0.819%
3	4.064	163	166	172	rVB	24975	33853	0.75%	0.076%
4	5.193	354	358	361	rBV5	4267	5727	0.13%	0.013%
5	5.387	387	391	395	rVB7	3658	5896	0.13%	0.013%
6	5.517	410	413	415	rBV4	4948	4857	0.11%	0.011%
7	5.811	461	463	469	rVB5	6515	9123	0.20%	0.021%
8	5.875	469	474	475	rBV4	4417	6439	0.14%	0.014%
9	5.987	490	493	496	rBV5	4681	5067	0.11%	0.011%
10	7.046	666	673	684	rVB	293816	454902	10.08%	1.024%
11	7.222	696	703	717	rBV	927579	1477671	32.74%	3.326%
12	7.405	728	734	745	rBV	851122	1372779	30.41%	3.090%
13	7.499	747	750	753	rVB5	4345	4747	0.11%	0.011%
14	7.881	807	815	824	rBV	796482	1260374	27.92%	2.837%
15	7.946	824	826	830	rVB5	4436	4667	0.10%	0.011%
16	8.587	927	935	945	rBV	718600	1141626	25.29%	2.570%
17	9.046	1005	1013	1027	rVV	1018084	1680614	37.23%	3.783%
18	9.152	1029	1031	1036	rVB5	4441	6337	0.14%	0.014%
19	9.434	1077	1079	1083	rBV3	6064	8748	0.19%	0.020%
20	9.769	1127	1136	1146	rBV	565150	967303	21.43%	2.177%
21	10.152	1199	1201	1206	rBV6	3236	5312	0.12%	0.012%
22	10.299	1218	1226	1240	rBV	1038069	1713724	37.97%	3.857%
23	10.681	1283	1291	1298	rBV	989335	1660267	36.78%	3.737%
24	10.822	1307	1315	1329	rBV	973970	1699211	37.65%	3.825%
25	10.969	1338	1340	1348	rVB9	2986	5702	0.13%	0.013%
26	12.104	1528	1533	1536	rBV7	2616	5072	0.11%	0.011%
27	12.275	1556	1562	1569	rVB3	16581	29726	0.66%	0.067%
28	13.428	1753	1758	1764	rVB2	16513	26276	0.58%	0.059%
29	13.498	1764	1770	1772	rBV7	3888	4948	0.11%	0.011%
30	13.946	1838	1846	1854	rBV	1875743	2546436	56.42%	5.732%
31	14.216	1882	1892	1909	rBV2	2171739	3133871	69.43%	7.054%
32	14.522	1937	1944	1951	rBV	1229933	1809525	40.09%	4.073%
33	14.610	1956	1959	1963	rVB5	9175	12493	0.28%	0.028%
34	14.722	1970	1978	1989	rBV2	91171	180933	4.01%	0.407%
35	14.963	2013	2019	2024	rVB8	3715	7123	0.16%	0.016%
36	15.204	2057	2060	2067	rBV6	5419	9198	0.20%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029608.D
 Acq On : 09 Feb 2024 13:56
 Operator : MA/JU
 Sample : P1348-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	15.334	2078	2082	2084	rBV2	6265	8109	0.18%	0.018%
38	15.516	2107	2113	2128	rVB	2511532	3691987	81.80%	8.310%
39	15.640	2128	2134	2146	rBV	262355	381542	8.45%	0.859%
40	15.757	2151	2154	2158	rVB4	11040	13022	0.29%	0.029%
41	15.892	2174	2177	2184	rBV8	5064	7619	0.17%	0.017%
42	16.304	2242	2247	2253	rBV6	7788	12034	0.27%	0.027%
43	16.428	2263	2268	2271	rBV6	3848	5548	0.12%	0.012%
44	17.275	2405	2412	2422	rBV	1312375	1837172	40.70%	4.135%
45	17.375	2422	2429	2444	rBV2	2871474	4044407	89.60%	9.103%
46	17.675	2472	2480	2485	rBV2	4748	13102	0.29%	0.029%
47	17.951	2521	2527	2532	rBV	50564	70740	1.57%	0.159%
48	18.181	2563	2566	2574	rBV8	10605	16747	0.37%	0.038%
49	18.263	2577	2580	2583	rVB2	6736	6746	0.15%	0.015%
50	18.622	2638	2641	2645	rBV6	7117	7762	0.17%	0.017%
51	19.233	2741	2745	2749	rBV2	32462	47195	1.05%	0.106%
52	19.304	2753	2757	2761	rBV	25912	37773	0.84%	0.085%
53	19.469	2782	2785	2789	rBV6	9413	12473	0.28%	0.028%
54	19.669	2813	2819	2829	rBV	3127326	4284982	94.93%	9.645%
55	21.469	3120	3125	3133	rBV	1259504	1734948	38.44%	3.905%
56	23.692	3495	3503	3515	rBV2	2250846	4513606	100.00%	10.159%
57	23.845	3522	3529	3540	rVB	945036	1940902	43.00%	4.369%




Sum of corrected areas: 44427849

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029608.D
Acq On : 09 Feb 2024 13:56
Operator : MA/JU
Sample : P1348-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

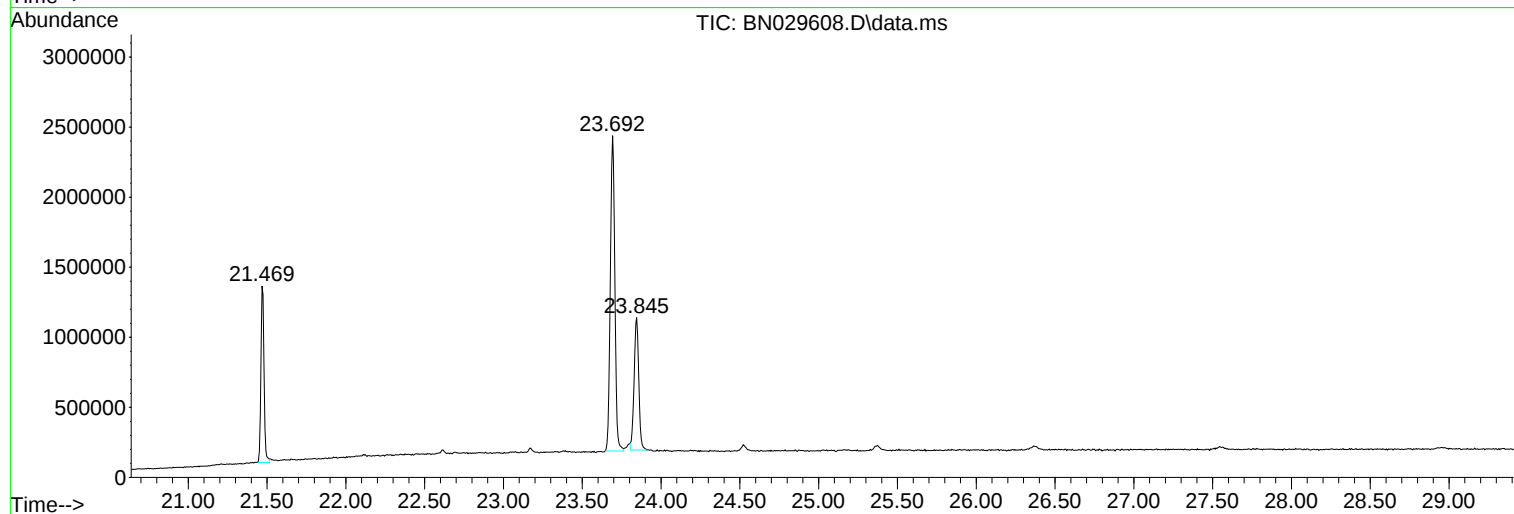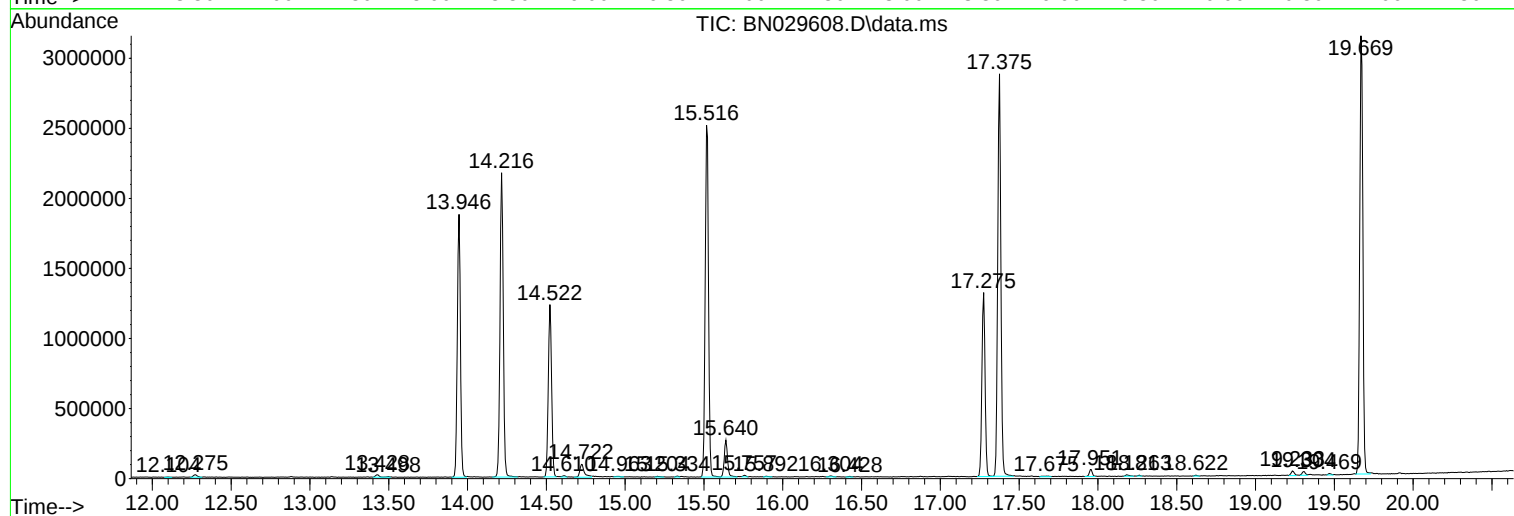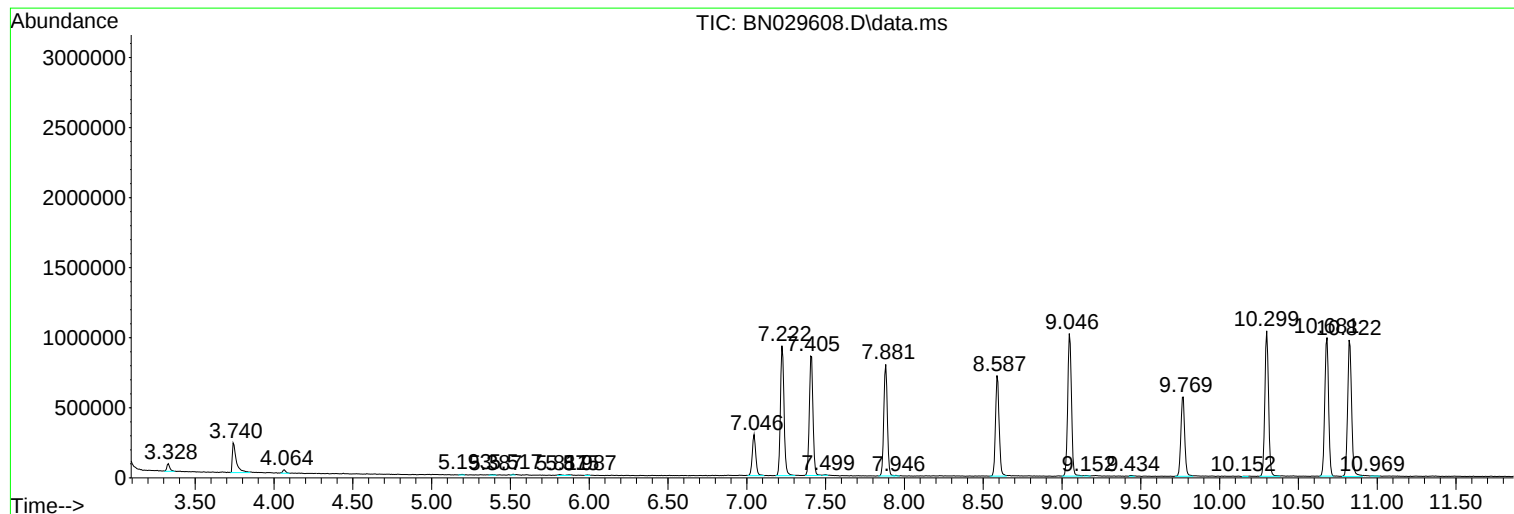

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029608.D
Acq On : 09 Feb 2024 13:56
Operator : MA/JU
Sample : P1348-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029608.D
Acq On : 09 Feb 2024 13:56
Operator : MA/JU
Sample : P1348-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------