

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029612.D
 Acq On : 09 Feb 2024 16:20
 Operator : MA/JU
 Sample : PB158824BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK824

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	46	rBV	81263	99747	2.95%	0.222%
2	3.734	107	110	134	rBV	900523	1371243	40.59%	3.046%
3	4.064	162	166	171	rVB	21717	30854	0.91%	0.069%
4	7.046	666	673	687	rBV	1040924	1630205	48.25%	3.621%
5	7.222	696	703	715	rBV	860306	1346214	39.85%	2.990%
6	7.410	727	735	746	rBV	1011980	1643347	48.64%	3.650%
7	7.881	806	815	823	rBV	857049	1358063	40.20%	3.017%
8	8.587	928	935	947	rBV	1160637	1894830	56.09%	4.209%
9	9.046	1005	1013	1028	rBV	906433	1511194	44.73%	3.357%
10	9.763	1128	1135	1145	rBV	654872	1091736	32.31%	2.425%
11	10.299	1217	1226	1240	rBV	1076975	1776861	52.59%	3.947%
12	10.681	1283	1291	1300	rVB	1048063	1796583	53.18%	3.991%
13	10.822	1308	1315	1329	rBV	1050017	1850191	54.76%	4.110%
14	12.275	1557	1562	1568	rBV2	14363	24045	0.71%	0.053%
15	13.428	1751	1758	1764	rVB3	13913	22697	0.67%	0.050%
16	13.945	1840	1846	1855	rBV	1555687	2143712	63.45%	4.762%
17	14.216	1884	1892	1904	rBV	1901307	2741978	81.16%	6.091%
18	14.522	1937	1944	1953	rBV	1325933	1938992	57.39%	4.307%
19	14.722	1972	1978	1991	rBV	585958	923016	27.32%	2.050%
20	14.881	2003	2005	2011	rVB7	2976	3980	0.12%	0.009%
21	15.328	2078	2081	2085	rBV5	1980	3678	0.11%	0.008%
22	15.516	2106	2113	2126	rBV	2141745	3139968	92.94%	6.975%
23	15.639	2127	2134	2145	rBV	518840	712557	21.09%	1.583%
24	15.757	2151	2154	2159	rVB6	10173	15238	0.45%	0.034%
25	16.310	2241	2248	2253	rBV7	6847	12337	0.37%	0.027%
26	16.775	2325	2327	2331	rVB4	3353	3774	0.11%	0.008%
27	16.816	2331	2334	2337	rBV4	2500	3866	0.11%	0.009%
28	16.951	2355	2357	2361	rVB5	3922	3674	0.11%	0.008%
29	17.069	2372	2377	2379	rBV5	3532	5333	0.16%	0.012%
30	17.275	2405	2412	2420	rBV	1413704	1982545	58.68%	4.404%
31	17.375	2422	2429	2442	rBV2	2142039	3103033	91.85%	6.893%
32	18.192	2563	2568	2571	rBV5	4609	8124	0.24%	0.018%
33	19.239	2741	2746	2750	rBV	24956	34103	1.01%	0.076%
34	19.304	2753	2757	2762	rVV	19446	24856	0.74%	0.055%
35	19.474	2782	2786	2792	rBV8	4287	8214	0.24%	0.018%
36	19.674	2813	2820	2830	rBV	2371678	3331392	98.61%	7.400%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029612.D
Acq On : 09 Feb 2024 16:20
Operator : MA/JU
Sample : PB158824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.798	2839	2841	2844	rBV3	4888	3431	0.10%	0.008%
38	21.474	3120	3126	3139	rBV	1430766	1922467	56.90%	4.270%
39	23.692	3496	3503	3514	rBV2	1719911	3378456	100.00%	7.505%
40	23.845	3523	3529	3541	rVB	1024540	2122103	62.81%	4.714%




Sum of corrected areas: 45018637

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029612.D
Acq On : 09 Feb 2024 16:20
Operator : MA/JU
Sample : PB158824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

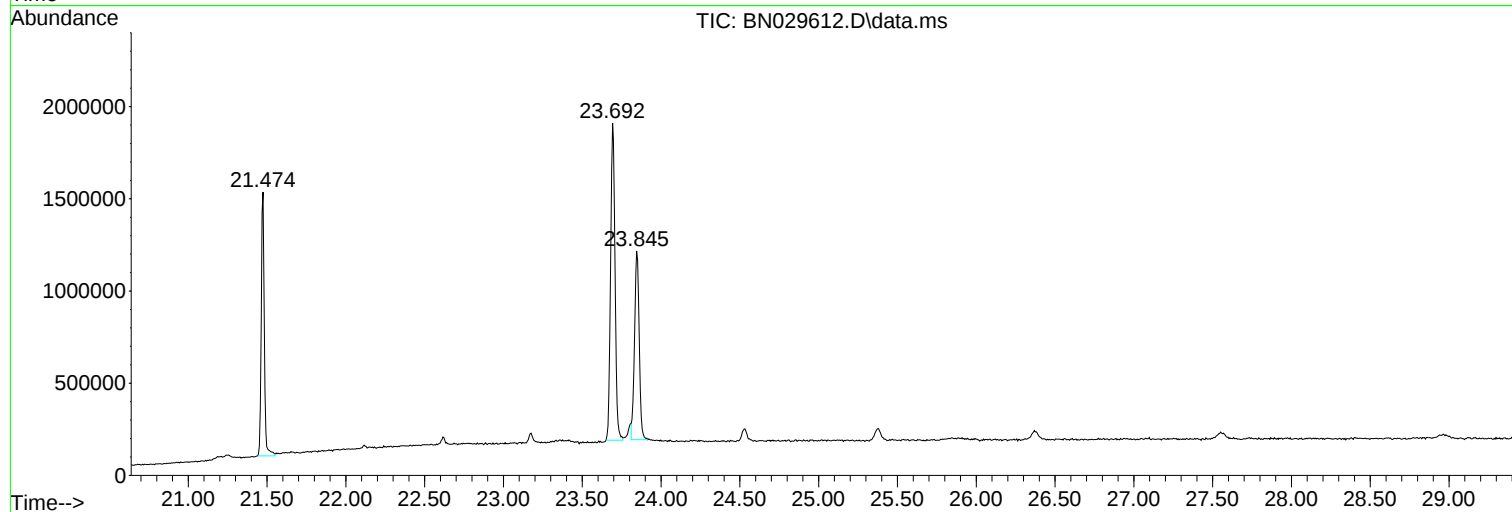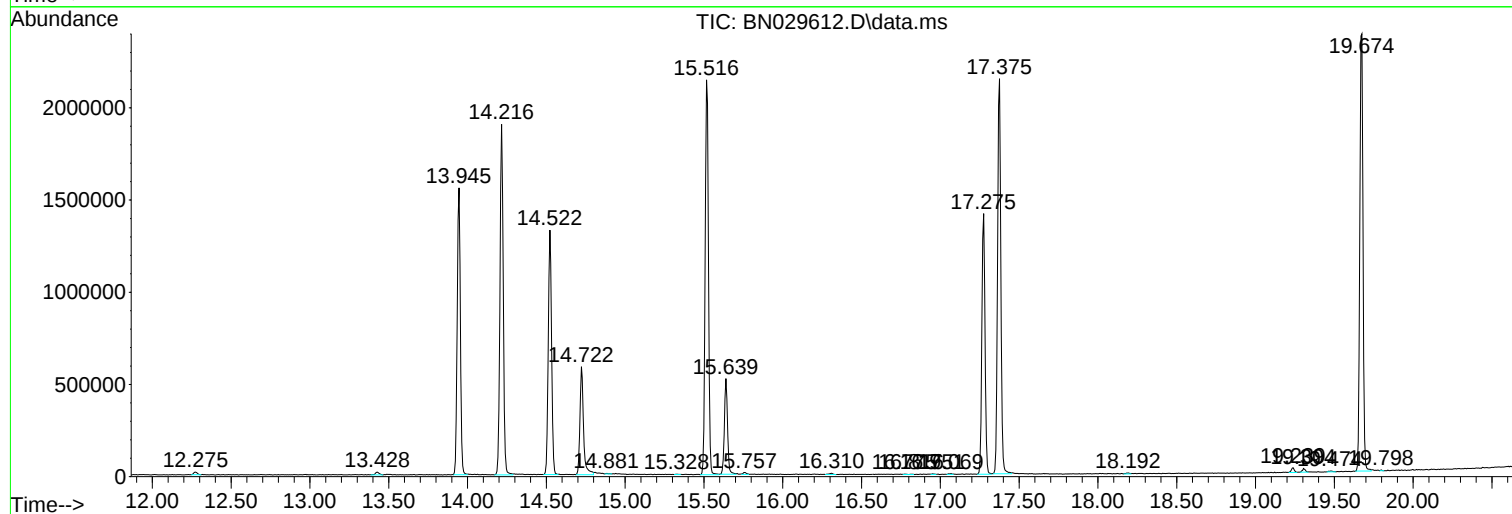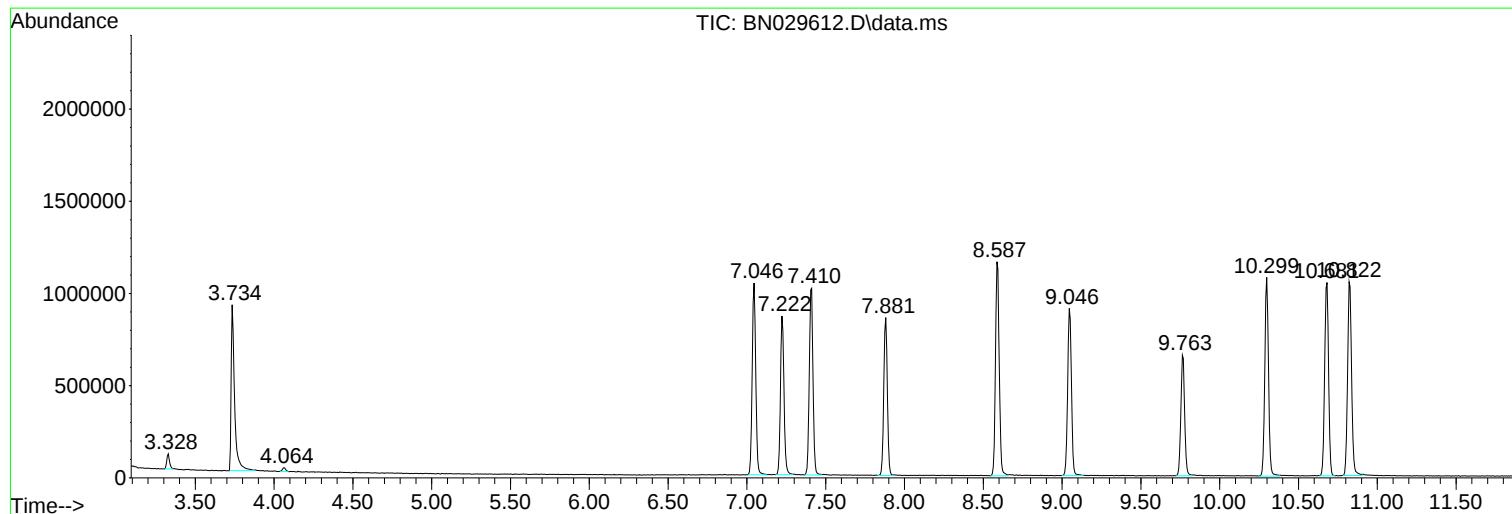

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029612.D
Acq On : 09 Feb 2024 16:20
Operator : MA/JU
Sample : PB158824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029612.D
Acq On : 09 Feb 2024 16:20
Operator : MA/JU
Sample : PB158824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc