

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029613.D
 Acq On : 09 Feb 2024 16:56
 Operator : MA/JU
 Sample : PB158919BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK919

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029613.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	48	rVB	79649	109744	3.43%	0.239%
2	3.734	106	110	128	rBV	920065	1391372	43.46%	3.028%
3	4.064	162	166	172	rVB	24040	35037	1.09%	0.076%
4	5.981	488	492	496	rVB7	2897	5121	0.16%	0.011%
5	6.905	645	649	653	rVB7	2089	3312	0.10%	0.007%
6	7.046	666	673	686	rBV	1060368	1651352	51.58%	3.594%
7	7.222	694	703	720	rBV	885998	1393581	43.53%	3.033%
8	7.411	727	735	749	rBV	1043425	1672289	52.23%	3.640%
9	7.881	808	815	823	rBV	939596	1511667	47.21%	3.290%
10	8.099	847	852	853	rBV3	3250	4532	0.14%	0.010%
11	8.587	928	935	949	rBV	1199122	1935552	60.45%	4.213%
12	9.046	1004	1013	1022	rBV	942121	1546906	48.31%	3.367%
13	9.763	1127	1135	1149	rBV	685946	1126367	35.18%	2.451%
14	10.299	1218	1226	1237	rBV	1103730	1798588	56.18%	3.915%
15	10.681	1282	1291	1299	rBV	1200173	2033202	63.50%	4.425%
16	10.822	1307	1315	1332	rBV	1090461	1907403	59.57%	4.151%
17	12.275	1555	1562	1566	rBV3	14585	26345	0.82%	0.057%
18	12.481	1594	1597	1600	rBV4	2628	4256	0.13%	0.009%
19	12.881	1661	1665	1668	rVV6	1818	3351	0.10%	0.007%
20	13.428	1753	1758	1764	rVV	21288	34286	1.07%	0.075%
21	13.945	1839	1846	1855	rBV	1566802	2184809	68.24%	4.755%
22	14.216	1884	1892	1905	rBV	1895978	2784101	86.96%	6.059%
23	14.522	1937	1944	1952	rBV	1489339	2155077	67.31%	4.690%
24	14.722	1971	1978	1998	rBV	570619	919336	28.71%	2.001%
25	14.887	2004	2006	2009	rVB4	3824	3534	0.11%	0.008%
26	14.945	2013	2016	2022	rVB8	3555	5744	0.18%	0.013%
27	15.516	2107	2113	2121	rBV	2176448	3142766	98.16%	6.840%
28	15.640	2128	2134	2144	rBV	507069	690324	21.56%	1.502%
29	15.757	2150	2154	2159	rVB2	9868	16223	0.51%	0.035%
30	16.304	2242	2247	2252	rVB6	7683	11502	0.36%	0.025%
31	17.275	2405	2412	2422	rBV	1522178	2148934	67.12%	4.677%
32	17.375	2422	2429	2448	rVV	2080507	3053883	95.38%	6.647%
33	17.828	2504	2506	2510	rBV5	3635	4558	0.14%	0.010%
34	18.186	2564	2567	2572	rBV7	4007	6965	0.22%	0.015%
35	18.786	2664	2669	2672	rVB7	2772	4658	0.15%	0.010%
36	19.233	2742	2745	2750	rVB4	21664	29587	0.92%	0.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029613.D
Acq On : 09 Feb 2024 16:56
Operator : MA/JU
Sample : PB158919BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK919

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.304	2754	2757	2763	rBV2	18996	24242	0.76%	0.053%
38	19.433	2777	2779	2781	rBV2	4914	3430	0.11%	0.007%
39	19.469	2783	2785	2791	rVB6	4754	8199	0.26%	0.018%
40	19.669	2813	2819	2829	rBV	2313091	3201721	100.00%	6.968%
41	21.474	3120	3126	3139	rBV	1431511	1986769	62.05%	4.324%
42	23.692	3496	3503	3517	rBV2	1629631	3160007	98.70%	6.878%
43	23.845	3522	3529	3542	rVB	1093761	2206152	68.91%	4.802%




Sum of corrected areas: 45946784

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029613.D
Acq On : 09 Feb 2024 16:56
Operator : MA/JU
Sample : PB158919BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK919

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

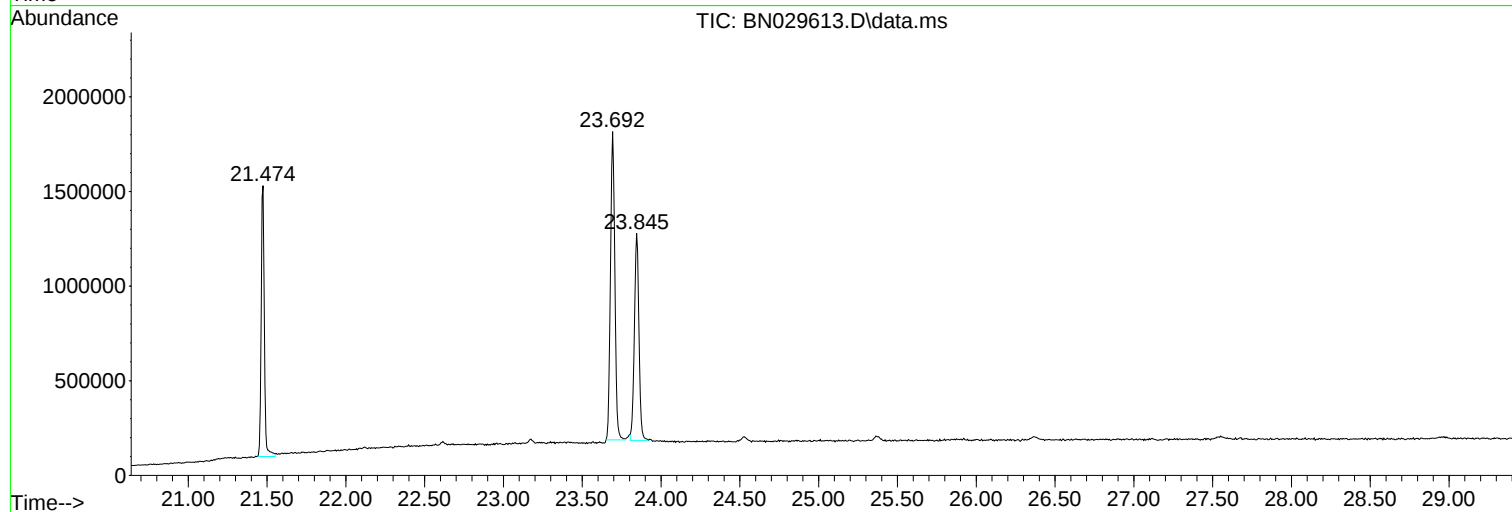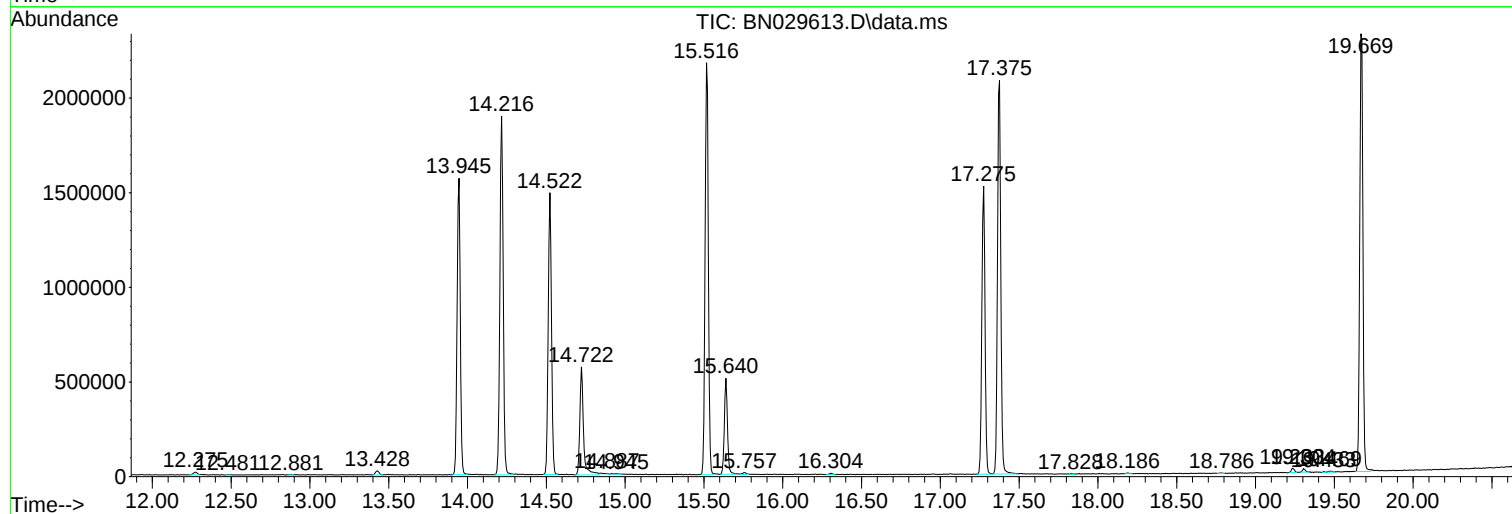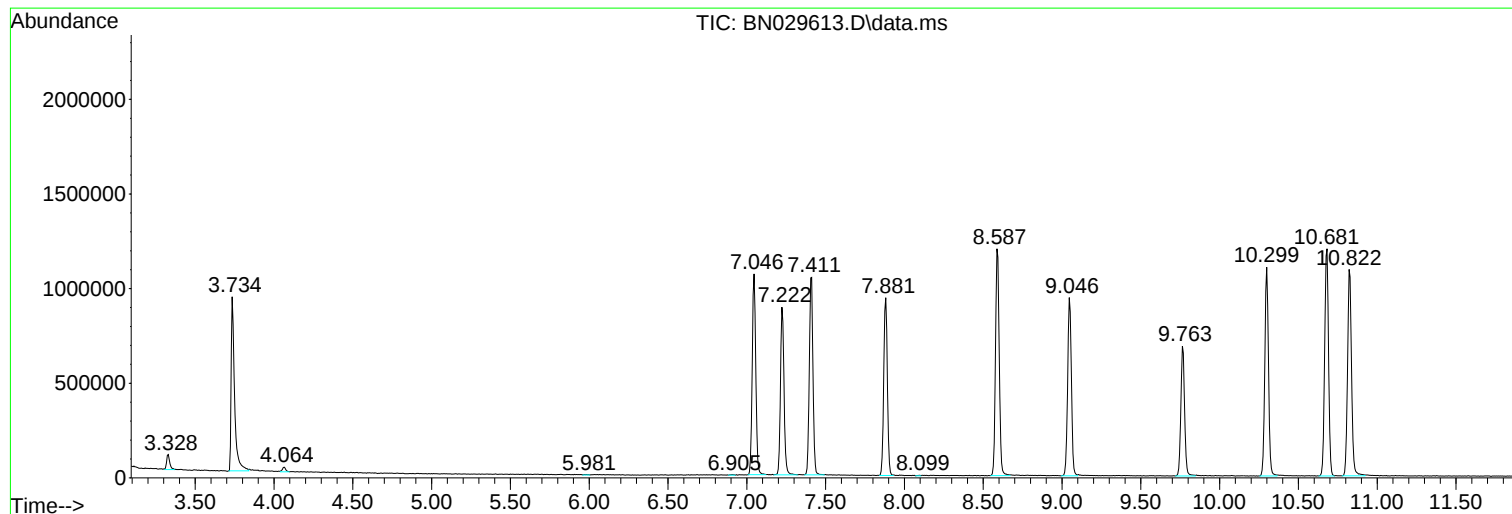

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029613.D
Acq On : 09 Feb 2024 16:56
Operator : MA/JU
Sample : PB158919BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK919

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029613.D
Acq On : 09 Feb 2024 16:56
Operator : MA/JU
Sample : PB158919BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK919

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc