

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029614.D
 Acq On : 09 Feb 2024 17:32
 Operator : MA/JU
 Sample : P1398-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	47	rVB	49211	59543	1.52%	0.141%
2	3.740	108	111	129	rBV	250854	426276	10.91%	1.011%
3	4.064	162	166	172	rVB	36327	50392	1.29%	0.119%
4	4.587	252	255	259	rVB5	10638	14296	0.37%	0.034%
5	7.046	666	673	680	rBV	190611	300404	7.69%	0.712%
6	7.222	697	703	719	rBV	875593	1381765	35.37%	3.277%
7	7.405	728	734	743	rBV	771631	1229168	31.46%	2.915%
8	7.487	746	748	753	rVB6	4474	7063	0.18%	0.017%
9	7.881	806	815	823	rBV	843929	1341647	34.34%	3.181%
10	7.946	823	826	829	rVB5	5943	8294	0.21%	0.020%
11	8.587	926	935	950	rBV	535119	869997	22.27%	2.063%
12	9.046	1006	1013	1025	rBV	942117	1559522	39.92%	3.698%
13	9.157	1028	1032	1035	rVB5	4100	5577	0.14%	0.013%
14	9.440	1077	1080	1083	rBV2	5174	5473	0.14%	0.013%
15	9.763	1128	1135	1146	rBV	628535	1057033	27.06%	2.507%
16	10.298	1218	1226	1240	rBV	978095	1606888	41.13%	3.810%
17	10.681	1282	1291	1300	rBV	1035420	1774871	45.43%	4.209%
18	10.822	1307	1315	1332	rBV	898202	1575935	40.34%	3.737%
19	12.275	1557	1562	1567	rVB	16369	26678	0.68%	0.063%
20	13.151	1707	1711	1716	rVB	22537	34972	0.90%	0.083%
21	13.357	1741	1746	1749	rBV6	3389	5823	0.15%	0.014%
22	13.428	1751	1758	1763	rVB4	13512	21737	0.56%	0.052%
23	13.487	1763	1768	1774	rBV7	2941	5280	0.14%	0.013%
24	13.945	1839	1846	1856	rBV	1706941	2332135	59.70%	5.530%
25	14.216	1885	1892	1906	rBV2	1898139	2774625	71.02%	6.580%
26	14.522	1937	1944	1952	rBV	1288761	1883237	48.21%	4.466%
27	14.722	1972	1978	1984	rBV2	65570	119295	3.05%	0.283%
28	14.951	2013	2017	2019	rBV5	3925	5173	0.13%	0.012%
29	15.281	2068	2073	2075	rBV6	2627	4471	0.11%	0.011%
30	15.516	2107	2113	2120	rBV	2321588	3395414	86.92%	8.052%
31	15.639	2128	2134	2144	rBV	602470	834153	21.35%	1.978%
32	15.763	2150	2155	2159	rVB6	10601	17399	0.45%	0.041%
33	16.310	2241	2248	2251	rVB6	6399	10292	0.26%	0.024%
34	16.416	2262	2266	2270	rBV6	1924	4418	0.11%	0.010%
35	17.063	2369	2376	2378	rBV6	3285	6188	0.16%	0.015%
36	17.275	2406	2412	2422	rBV	1375059	1921535	49.19%	4.557%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029614.D
 Acq On : 09 Feb 2024 17:32
 Operator : MA/JU
 Sample : P1398-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.375	2422	2429	2440	rBV	2465653	3548684	90.84%	8.415%
38	17.628	2468	2472	2475	rBV4	2956	5068	0.13%	0.012%
39	17.669	2477	2479	2484	rVB5	3375	4618	0.12%	0.011%
40	17.951	2522	2527	2533	rBV9	4659	11778	0.30%	0.028%
41	18.180	2562	2566	2576	rBV3	42867	61835	1.58%	0.147%
42	19.233	2741	2745	2751	rBV3	26434	38132	0.98%	0.090%
43	19.304	2753	2757	2762	rBV2	22777	33556	0.86%	0.080%
44	19.469	2781	2785	2789	rBV4	26239	33977	0.87%	0.081%
45	19.627	2809	2812	2813	rBV3	6880	5850	0.15%	0.014%
46	19.674	2813	2820	2827	rVV	2751064	3853043	98.63%	9.137%
47	21.204	3077	3080	3086	rBV7	20956	34250	0.88%	0.081%
48	21.410	3111	3115	3120	rBV	83424	103875	2.66%	0.246%
49	21.474	3120	3126	3139	rVV	1389215	1861485	47.65%	4.414%
50	23.698	3496	3504	3514	rBV	1934140	3906555	100.00%	9.264%
51	23.845	3523	3529	3540	rVB2	947979	1990660	50.96%	4.721%




Sum of corrected areas: 42170335

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029614.D
Acq On : 09 Feb 2024 17:32
Operator : MA/JU
Sample : P1398-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

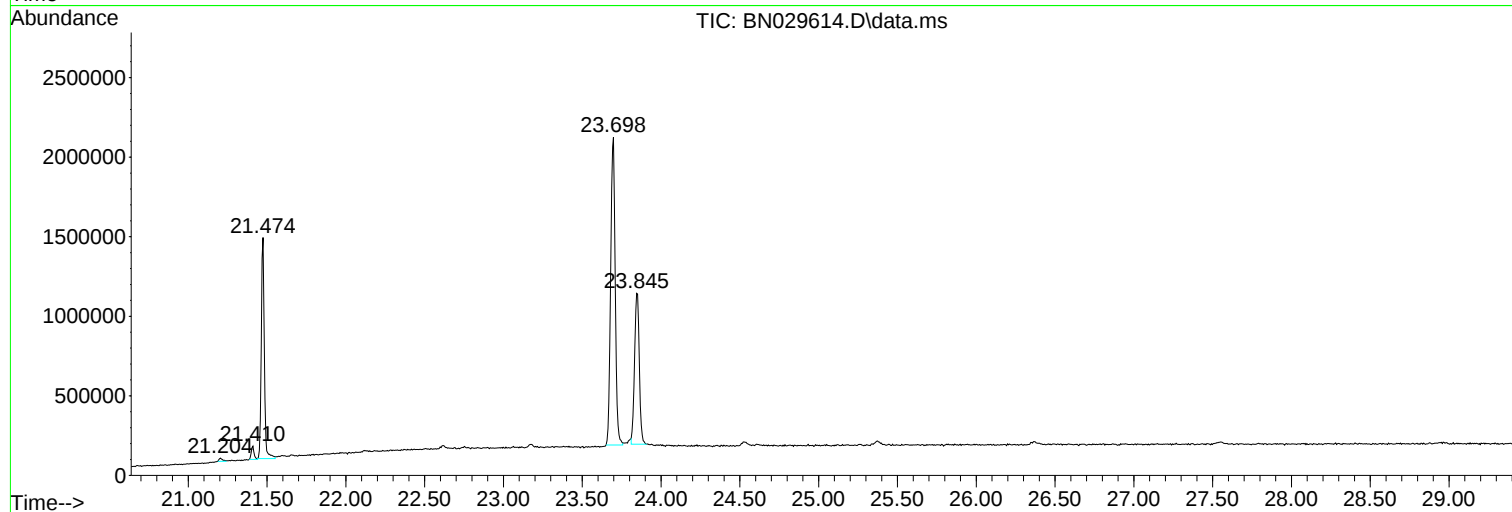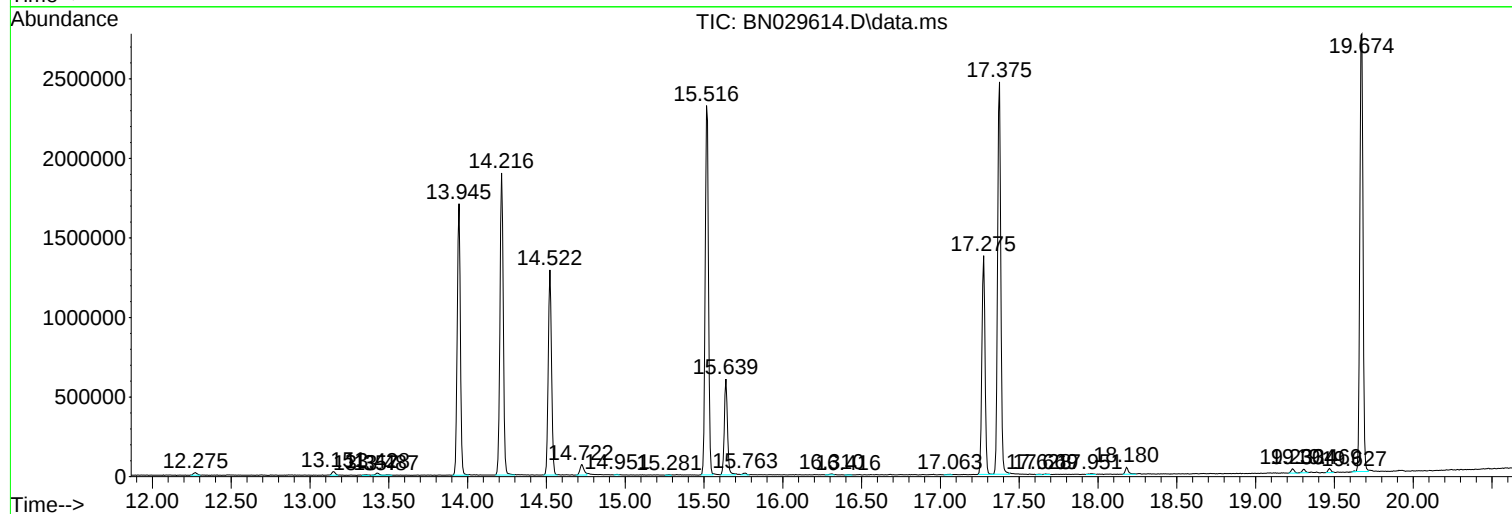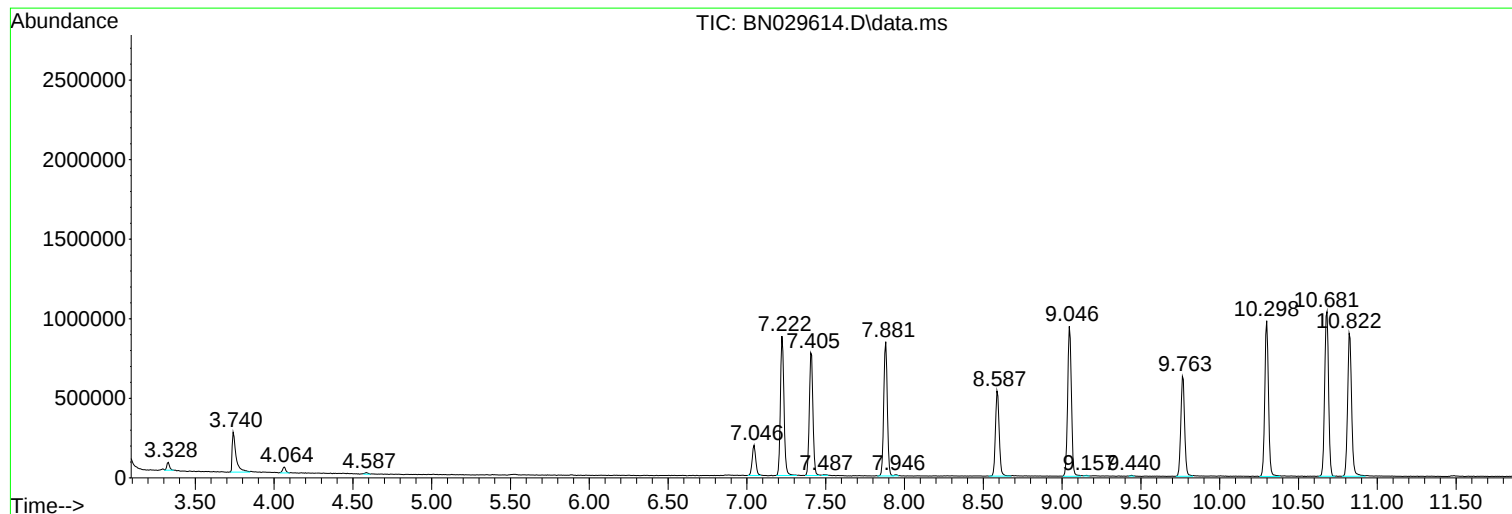

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029614.D
Acq On : 09 Feb 2024 17:32
Operator : MA/JU
Sample : P1398-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029614.D
Acq On : 09 Feb 2024 17:32
Operator : MA/JU
Sample : P1398-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc