

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029616.D
 Acq On : 09 Feb 2024 18:44
 Operator : MA/JU
 Sample : P1398-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029616.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	45	rBV	56277	74288	1.64%	0.157%
2	3.740	108	111	127	rBV	213426	360157	7.94%	0.761%
3	4.064	162	166	172	rVB	25543	34156	0.75%	0.072%
4	5.887	472	476	479	rVB6	3477	5106	0.11%	0.011%
5	5.934	479	484	490	rBV4	12847	20618	0.45%	0.044%
6	6.787	627	629	636	rVB8	2816	6498	0.14%	0.014%
7	7.046	666	673	686	rVB	294022	476282	10.50%	1.006%
8	7.222	694	703	717	rBV	1022175	1606557	35.42%	3.393%
9	7.405	727	734	745	rBV	989445	1556796	34.32%	3.287%
10	7.634	768	773	776	rVB6	3656	6405	0.14%	0.014%
11	7.669	776	779	784	rBV6	2873	5650	0.12%	0.012%
12	7.881	807	815	822	rBV	834483	1325231	29.22%	2.798%
13	8.587	928	935	946	rBV	760336	1199563	26.44%	2.533%
14	9.046	1003	1013	1026	rBV	1113729	1827424	40.29%	3.859%
15	9.152	1026	1031	1038	rVV4	13049	28512	0.63%	0.060%
16	9.434	1075	1079	1083	rVB6	3939	7526	0.17%	0.016%
17	9.763	1126	1135	1152	rBV	778888	1298416	28.62%	2.742%
18	10.299	1218	1226	1242	rBV	1135740	1924913	42.44%	4.065%
19	10.675	1280	1290	1301	rBV	1024363	1772212	39.07%	3.742%
20	10.822	1306	1315	1327	rBV	1054503	1832208	40.39%	3.869%
21	11.481	1422	1427	1429	rBV5	4730	6588	0.15%	0.014%
22	12.269	1556	1561	1568	rBV	20096	33612	0.74%	0.071%
23	13.351	1740	1745	1752	rVB8	5384	9159	0.20%	0.019%
24	13.428	1752	1758	1764	rVB2	18521	31327	0.69%	0.066%
25	13.493	1764	1769	1774	rBV5	4252	7510	0.17%	0.016%
26	13.945	1839	1846	1855	rBV	1947245	2663492	58.72%	5.624%
27	14.051	1862	1864	1871	rVB5	4071	7388	0.16%	0.016%
28	14.216	1882	1892	1905	rBV	2246995	3297612	72.70%	6.963%
29	14.428	1923	1928	1932	rBV5	12613	18494	0.41%	0.039%
30	14.522	1937	1944	1956	rBV	1292803	1878173	41.40%	3.966%
31	14.722	1971	1978	1987	rBV	118006	208713	4.60%	0.441%
32	14.875	2003	2004	2010	rVB6	3678	6428	0.14%	0.014%
33	15.122	2041	2046	2048	rVB4	3929	4979	0.11%	0.011%
34	15.328	2076	2081	2083	rBV4	5143	6073	0.13%	0.013%
35	15.381	2083	2090	2095	rVB5	18529	31118	0.69%	0.066%
36	15.516	2106	2113	2120	rBV	2759823	3838084	84.61%	8.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029616.D
Acq On : 09 Feb 2024 18:44
Operator : MA/JU
Sample : P1398-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	15.639	2127	2134	2148	rBV	727630	1001425	22.08%	2.115%
38	15.757	2150	2154	2157	rBV4	11327	15022	0.33%	0.032%
39	15.892	2174	2177	2180	rVB3	5949	5400	0.12%	0.011%
40	16.004	2193	2196	2201	rVB7	5272	5833	0.13%	0.012%
41	16.087	2206	2210	2214	rVB6	3398	5551	0.12%	0.012%
42	16.245	2233	2237	2244	rVV2	27289	47322	1.04%	0.100%
43	16.304	2244	2247	2252	rVB5	8726	13162	0.29%	0.028%
44	16.416	2264	2266	2270	rBV5	3999	4650	0.10%	0.010%
45	16.751	2321	2323	2328	rVB5	3748	5618	0.12%	0.012%
46	16.951	2355	2357	2361	rVB5	4440	5044	0.11%	0.011%
47	17.045	2369	2373	2379	rBV2	27336	38043	0.84%	0.080%
48	17.092	2379	2381	2385	rVB4	5866	7150	0.16%	0.015%
49	17.275	2405	2412	2421	rBV	1285010	1859838	41.00%	3.927%
50	17.375	2422	2429	2444	rVV	2821196	4155969	91.62%	8.776%
51	17.522	2451	2454	2458	rVB4	5508	6979	0.15%	0.015%
52	17.581	2460	2464	2468	rVB5	5602	11075	0.24%	0.023%
53	17.657	2473	2477	2478	rBV3	3814	5358	0.12%	0.011%
54	17.786	2495	2499	2504	rBV2	21964	29108	0.64%	0.061%
55	17.957	2525	2528	2534	rVB8	7400	11885	0.26%	0.025%
56	18.181	2562	2566	2572	rBV2	26519	40885	0.90%	0.086%
57	18.486	2614	2618	2623	rBV2	13063	16382	0.36%	0.035%
58	19.116	2723	2725	2729	rVB3	7802	8574	0.19%	0.018%
59	19.233	2741	2745	2750	rBV3	32562	43910	0.97%	0.093%
60	19.304	2753	2757	2762	rVV3	27043	33033	0.73%	0.070%
61	19.469	2781	2785	2793	rBV4	21707	32762	0.72%	0.069%
62	19.622	2809	2811	2813	rBV3	5981	5392	0.12%	0.011%
63	19.669	2813	2819	2829	rVV	3147242	4384900	96.67%	9.259%
64	21.469	3120	3125	3137	rBV	1218973	1691392	37.29%	3.572%
65	23.692	3495	3503	3514	rBV	2233560	4536126	100.00%	9.579%
66	23.845	3522	3529	3543	rVB	949410	1910684	42.12%	4.035%




Sum of corrected areas: 47355740

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029616.D
Acq On : 09 Feb 2024 18:44
Operator : MA/JU
Sample : P1398-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

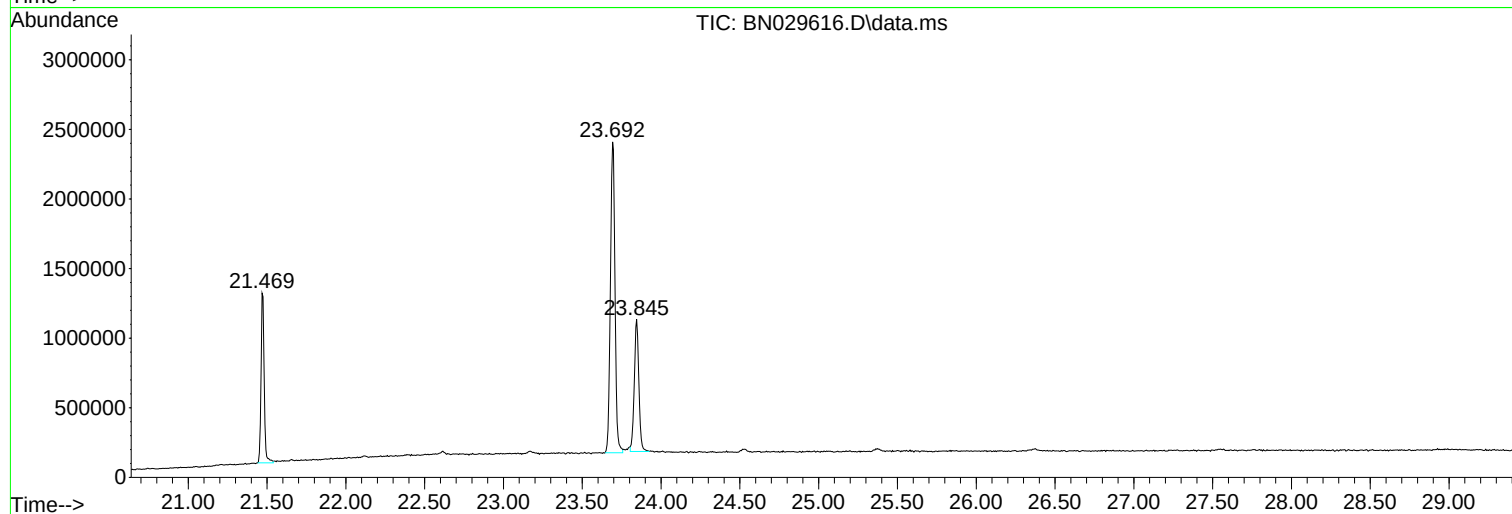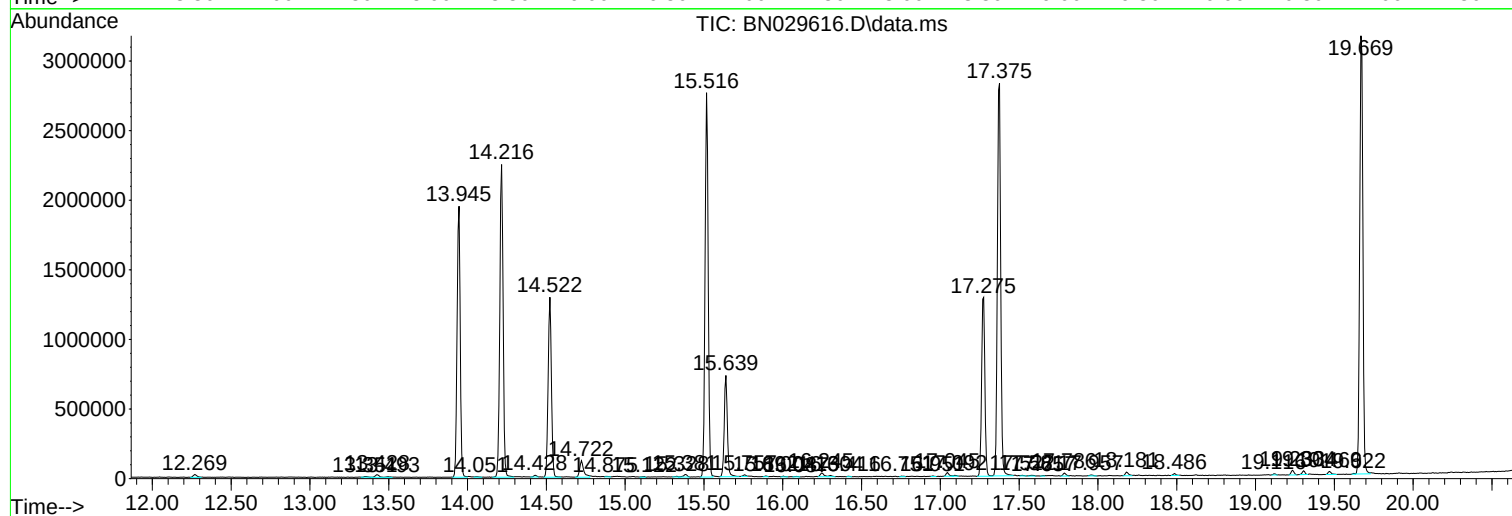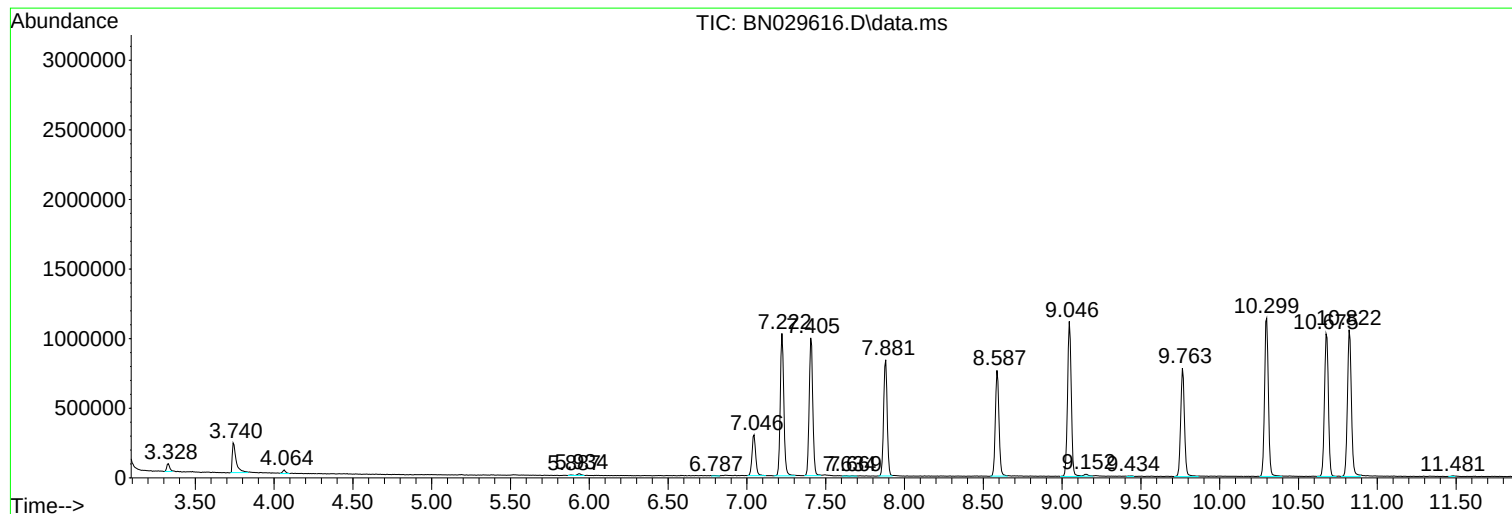

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029616.D
Acq On : 09 Feb 2024 18:44
Operator : MA/JU
Sample : P1398-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029616.D
Acq On : 09 Feb 2024 18:44
Operator : MA/JU
Sample : P1398-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc