

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029617.D
 Acq On : 09 Feb 2024 19:20
 Operator : MA/JU
 Sample : P1398-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	50	rVB	58617	77499	1.72%	0.163%
2	3.740	108	111	122	rBV	191736	327635	7.29%	0.688%
3	4.063	162	166	171	rVB	23971	30891	0.69%	0.065%
4	4.587	251	255	260	rVB5	8785	12760	0.28%	0.027%
5	6.869	636	643	648	rBV7	10899	22341	0.50%	0.047%
6	7.046	666	673	686	rVB	267579	434884	9.68%	0.913%
7	7.222	696	703	719	rBV	1026548	1622634	36.11%	3.408%
8	7.404	727	734	744	rBV	971427	1537266	34.21%	3.229%
9	7.881	808	815	824	rVV	869705	1380077	30.72%	2.899%
10	8.587	928	935	946	rBV	733329	1160650	25.83%	2.438%
11	9.046	1005	1013	1023	rBV	1138541	1845569	41.08%	3.876%
12	9.210	1037	1041	1045	rVB6	3498	6615	0.15%	0.014%
13	9.763	1127	1135	1146	rBV	780991	1292256	28.76%	2.714%
14	10.298	1219	1226	1239	rBV	1175985	1960349	43.63%	4.117%
15	10.398	1241	1243	1248	rVB6	3044	4715	0.10%	0.010%
16	10.675	1283	1290	1299	rVB	1087739	1833744	40.81%	3.851%
17	10.822	1308	1315	1326	rBV	984519	1719315	38.27%	3.611%
18	12.269	1556	1561	1567	rBV2	19323	31375	0.70%	0.066%
19	12.528	1601	1605	1610	rVB8	6307	9465	0.21%	0.020%
20	13.304	1731	1737	1740	rBV7	8331	15413	0.34%	0.032%
21	13.422	1751	1757	1763	rBV2	17525	29092	0.65%	0.061%
22	13.492	1766	1769	1776	rBV7	4636	10321	0.23%	0.022%
23	13.745	1804	1812	1818	rBV3	24836	39821	0.89%	0.084%
24	13.945	1837	1846	1859	rBV	1879981	2651695	59.02%	5.569%
25	14.051	1861	1864	1870	rVB8	2675	4786	0.11%	0.010%
26	14.216	1881	1892	1905	rBV	2281066	3333753	74.20%	7.002%
27	14.434	1925	1929	1934	rVB8	3181	5165	0.11%	0.011%
28	14.522	1937	1944	1956	rVV	1330367	1939554	43.17%	4.074%
29	14.722	1972	1978	1989	rBV	102138	185382	4.13%	0.389%
30	14.792	1989	1990	1996	rVB6	4091	5423	0.12%	0.011%
31	14.945	2011	2016	2023	rVB10	4507	10234	0.23%	0.021%
32	15.381	2088	2090	2095	rVB6	5092	7008	0.16%	0.015%
33	15.516	2104	2113	2127	rBV	2703916	3833260	85.32%	8.051%
34	15.639	2127	2134	2144	rBV	717650	967887	21.54%	2.033%
35	15.757	2150	2154	2158	rVB3	9360	11678	0.26%	0.025%
36	16.245	2230	2237	2243	rBV8	8448	17141	0.38%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029617.D
 Acq On : 09 Feb 2024 19:20
 Operator : MA/JU
 Sample : P1398-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	16.298	2243	2246	2252	rVB5	7368	11328	0.25%	0.024%
38	17.045	2369	2373	2378	rBV6	9071	13824	0.31%	0.029%
39	17.086	2378	2380	2392	rVB10	4381	10412	0.23%	0.022%
40	17.275	2405	2412	2421	rBV	1351797	1940774	43.20%	4.076%
41	17.375	2421	2429	2444	rBV2	2844422	4082398	90.86%	8.574%
42	17.580	2460	2464	2468	rBV6	3384	5047	0.11%	0.011%
43	17.669	2477	2479	2488	rVB9	6674	12065	0.27%	0.025%
44	17.786	2495	2499	2503	rBV7	7945	11487	0.26%	0.024%
45	17.963	2524	2529	2535	rBV	115078	151531	3.37%	0.318%
46	18.180	2563	2566	2573	rBV4	23759	33360	0.74%	0.070%
47	18.263	2577	2580	2583	rVB3	4908	6262	0.14%	0.013%
48	18.486	2614	2618	2621	rBV4	8589	11375	0.25%	0.024%
49	18.622	2637	2641	2645	rBV5	13147	17081	0.38%	0.036%
50	19.110	2721	2724	2726	rBV3	17847	20908	0.47%	0.044%
51	19.145	2726	2730	2733	rVB3	58256	70071	1.56%	0.147%
52	19.233	2741	2745	2749	rBV2	32230	44892	1.00%	0.094%
53	19.280	2749	2753	2755	rVV	23506	31631	0.70%	0.066%
54	19.304	2755	2757	2762	rVB	24198	29068	0.65%	0.061%
55	19.469	2781	2785	2791	rBV6	23338	30415	0.68%	0.064%
56	19.621	2809	2811	2813	rBV3	5182	5273	0.12%	0.011%
57	19.669	2813	2819	2828	rVV	3071536	4322988	96.22%	9.080%
58	21.468	3120	3125	3139	rBV	1344299	1847951	41.13%	3.881%
59	23.692	3495	3503	3515	rBV2	2247453	4493021	100.00%	9.437%
60	23.845	3522	3529	3544	rVB	977522	2031682	45.22%	4.267%




Sum of corrected areas: 47612497

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029617.D
Acq On : 09 Feb 2024 19:20
Operator : MA/JU
Sample : P1398-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

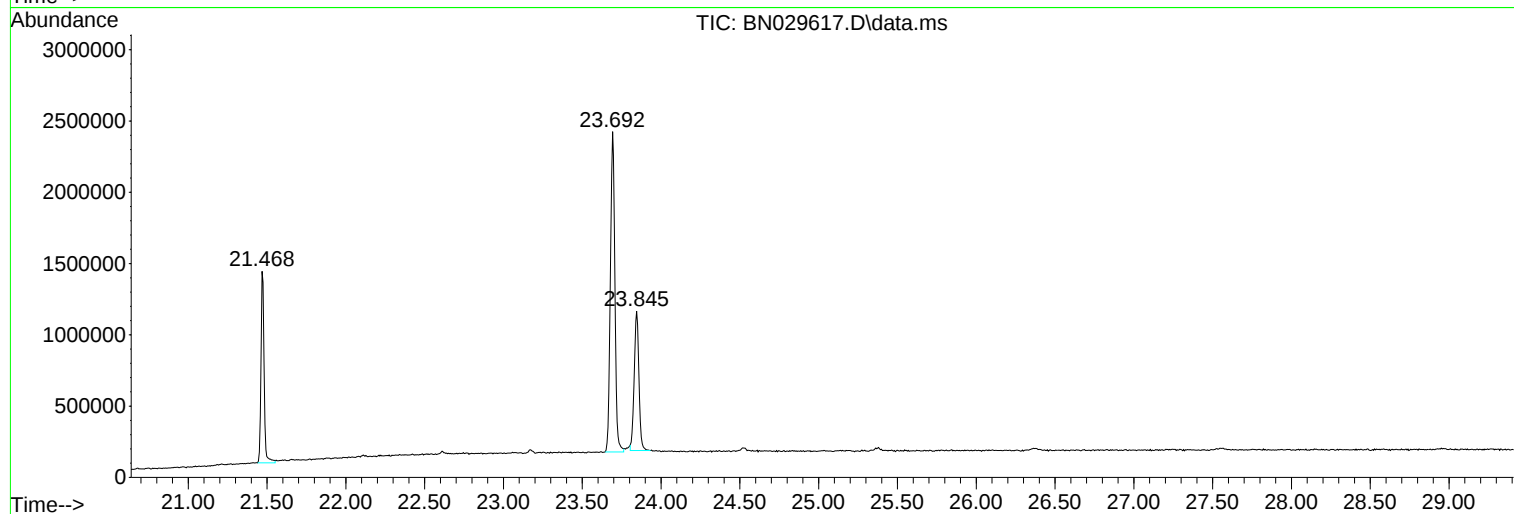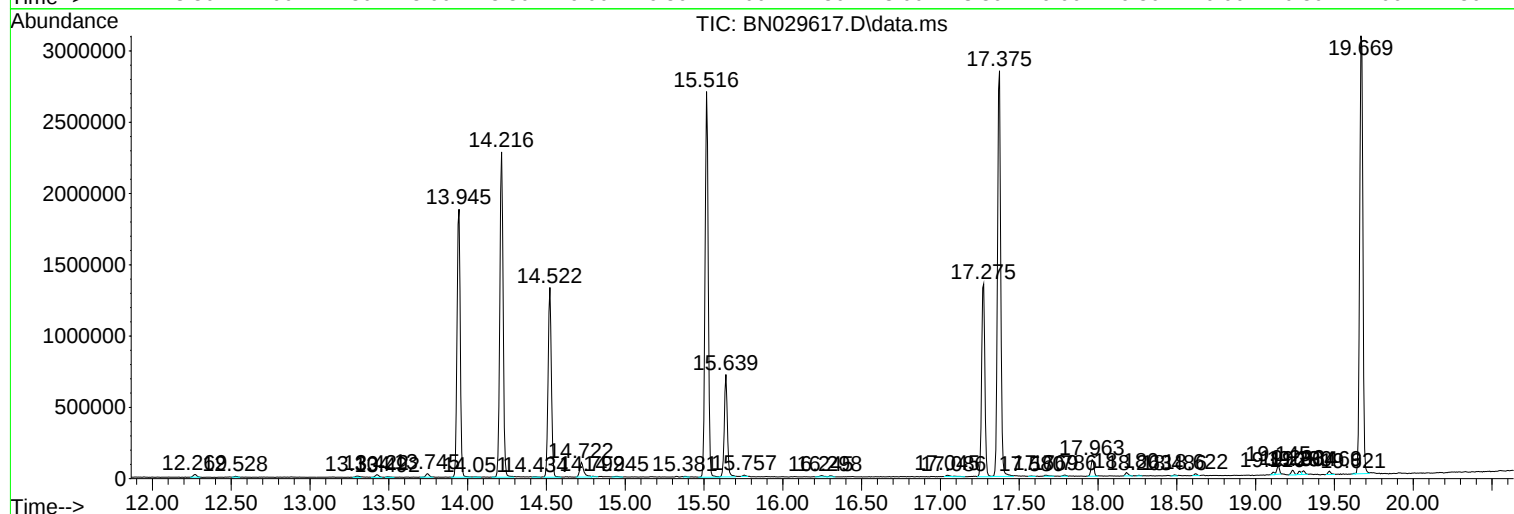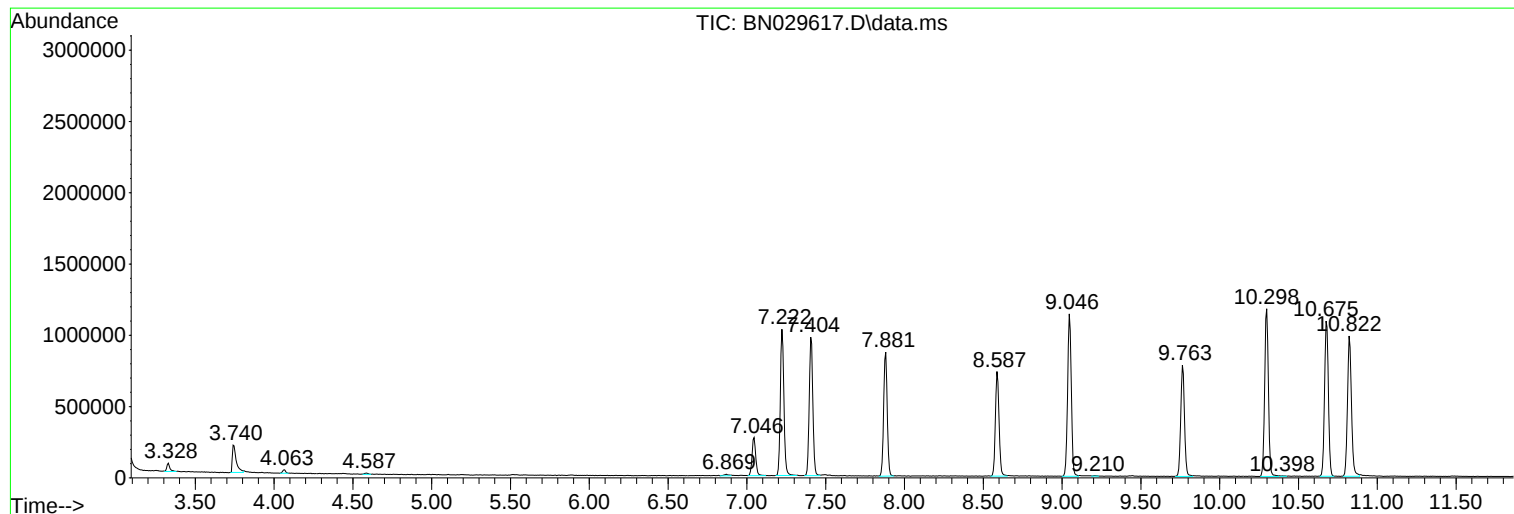

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029617.D
Acq On : 09 Feb 2024 19:20
Operator : MA/JU
Sample : P1398-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029617.D
Acq On : 09 Feb 2024 19:20
Operator : MA/JU
Sample : P1398-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc