

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029619.D
 Acq On : 09 Feb 2024 20:32
 Operator : MA/JU
 Sample : P1398-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	49	rVB	54098	71942	1.75%	0.160%
2	3.740	108	111	130	rBV	293086	479372	11.64%	1.064%
3	4.064	162	166	173	rVB	37451	52841	1.28%	0.117%
4	5.387	387	391	393	rBV5	3665	4426	0.11%	0.010%
5	5.522	408	414	415	rBV5	6090	8947	0.22%	0.020%
6	5.881	471	475	479	rBV6	4549	7410	0.18%	0.016%
7	6.952	656	657	662	rBV5	3263	4618	0.11%	0.010%
8	7.046	667	673	685	rVB	234324	377924	9.17%	0.839%
9	7.222	696	703	718	rBV	1030400	1620557	39.34%	3.598%
10	7.405	727	734	746	rBV	923149	1470310	35.69%	3.264%
11	7.493	746	749	752	rVB5	4375	5840	0.14%	0.013%
12	7.881	808	815	823	rBV	803045	1260265	30.59%	2.798%
13	8.587	927	935	948	rBV	677667	1072565	26.04%	2.381%
14	9.046	1006	1013	1027	rBV	1118903	1843448	44.75%	4.093%
15	9.440	1075	1080	1084	rVB7	4801	7877	0.19%	0.017%
16	9.763	1127	1135	1146	rBV	769071	1271900	30.88%	2.824%
17	10.299	1218	1226	1238	rBV	1154246	1879113	45.62%	4.172%
18	10.675	1282	1290	1300	rVB	995145	1677121	40.71%	3.724%
19	10.822	1307	1315	1330	rBV	1141383	1951425	47.37%	4.333%
20	11.446	1416	1421	1428	rBV7	6064	12163	0.30%	0.027%
21	12.269	1554	1561	1570	rBV	18438	34868	0.85%	0.077%
22	13.145	1705	1710	1717	rBV	30946	48556	1.18%	0.108%
23	13.422	1753	1757	1764	rBV2	16003	25165	0.61%	0.056%
24	13.945	1839	1846	1855	rBV	1843663	2619216	63.58%	5.815%
25	14.045	1861	1863	1869	rVB5	3877	4351	0.11%	0.010%
26	14.216	1883	1892	1905	rBV2	2202101	3305509	80.24%	7.339%
27	14.522	1937	1944	1953	rBV	1183979	1762501	42.79%	3.913%
28	14.722	1971	1978	1993	rBV2	72622	149366	3.63%	0.332%
29	14.939	2011	2015	2016	rBV3	4292	5020	0.12%	0.011%
30	15.322	2076	2080	2084	rBV6	3524	4722	0.11%	0.010%
31	15.516	2104	2113	2123	rBV	2636139	3770591	91.54%	8.372%
32	15.639	2127	2134	2148	rVV	626105	860345	20.89%	1.910%
33	15.757	2150	2154	2159	rVB4	11718	16586	0.40%	0.037%
34	16.304	2243	2247	2252	rBV5	7921	10794	0.26%	0.024%
35	17.045	2370	2373	2380	rBV7	3654	7839	0.19%	0.017%
36	17.275	2405	2412	2422	rBV	1193986	1743790	42.33%	3.872%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029619.D
Acq On : 09 Feb 2024 20:32
Operator : MA/JU
Sample : P1398-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	17.375	2422	2429	2443	rBV2	2552034	3803729	92.34%	8.445%
38	18.180	2562	2566	2572	rBV3	31242	45404	1.10%	0.101%
39	19.051	2710	2714	2716	rBV5	3679	4808	0.12%	0.011%
40	19.233	2741	2745	2750	rVB2	29600	40724	0.99%	0.090%
41	19.304	2750	2757	2761	rBV	25112	39643	0.96%	0.088%
42	19.469	2781	2785	2789	rBV3	19905	24647	0.60%	0.055%
43	19.669	2813	2819	2836	rVV	2924917	4020651	97.61%	8.927%
44	19.916	2859	2861	2864	rBV4	5492	5404	0.13%	0.012%
45	21.198	3077	3079	3083	rVB4	18186	19930	0.48%	0.044%
46	21.469	3120	3125	3133	rBV2	1196052	1650654	40.07%	3.665%
47	23.692	3495	3503	3516	rBV2	2070119	4119281	100.00%	9.146%
48	23.845	3522	3529	3539	rVB	896288	1816616	44.10%	4.033%




Sum of corrected areas: 45040774

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029619.D
Acq On : 09 Feb 2024 20:32
Operator : MA/JU
Sample : P1398-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

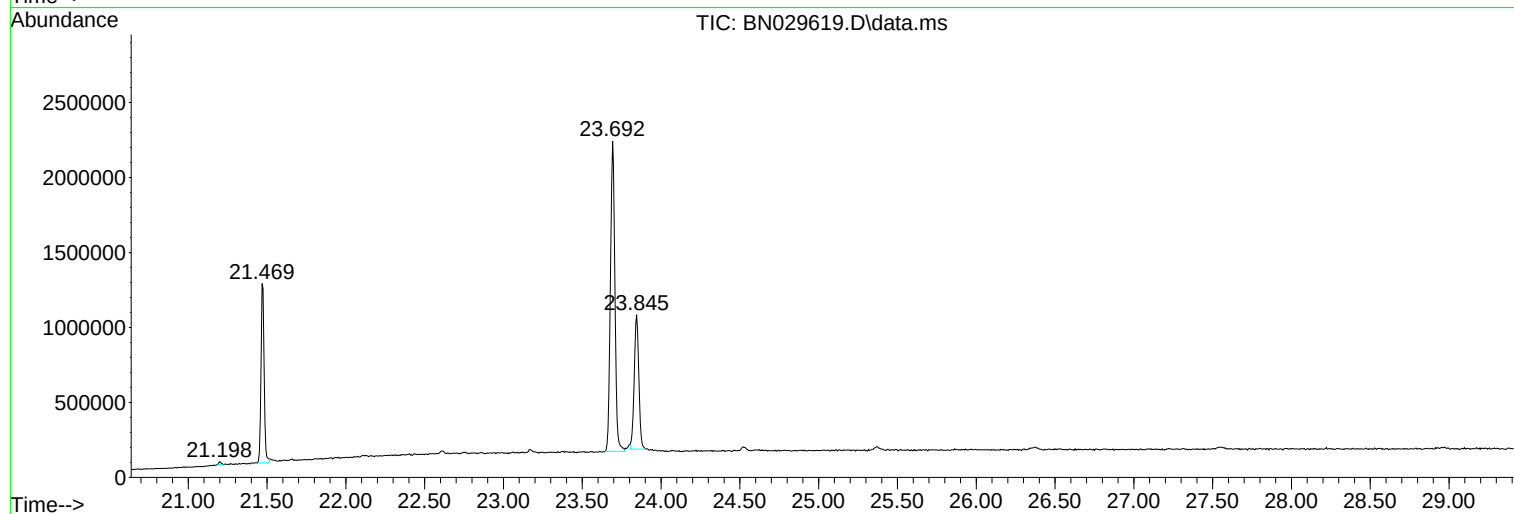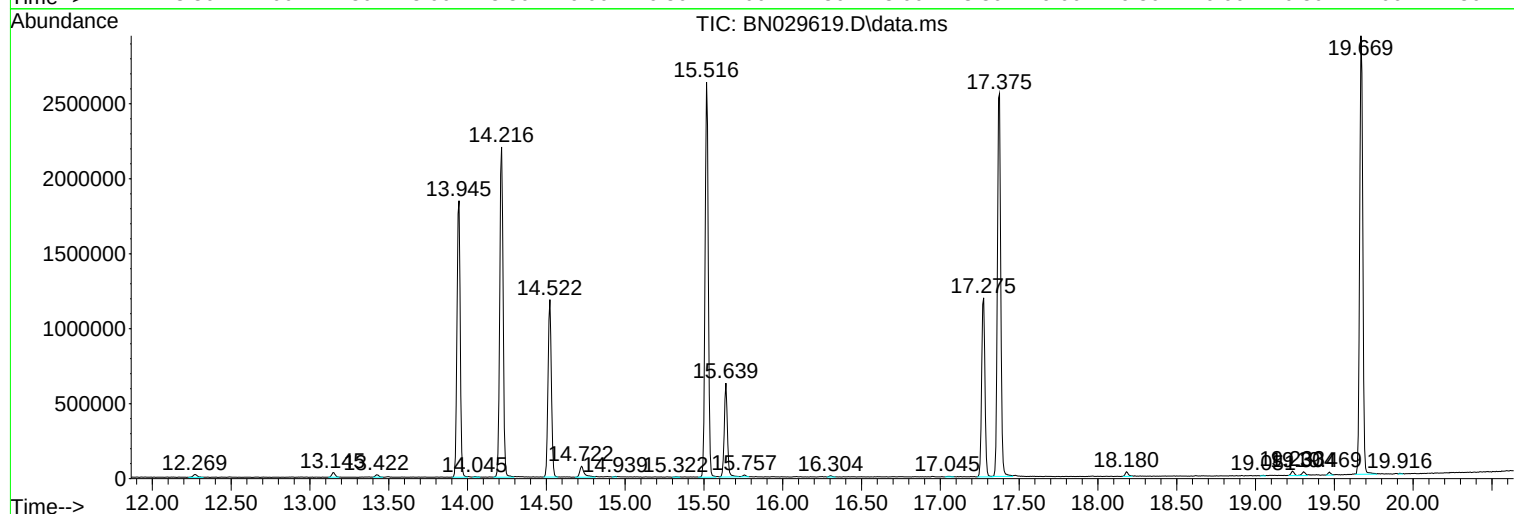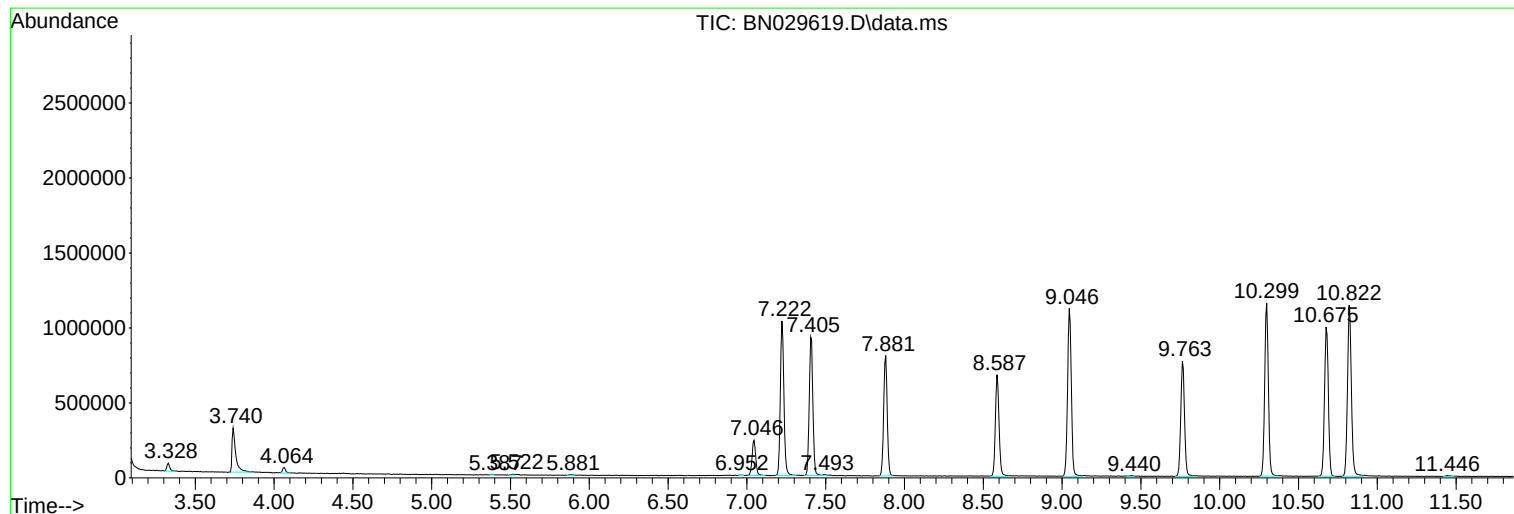

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029619.D
Acq On : 09 Feb 2024 20:32
Operator : MA/JU
Sample : P1398-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029619.D
Acq On : 09 Feb 2024 20:32
Operator : MA/JU
Sample : P1398-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------