

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029620.D
 Acq On : 09 Feb 2024 21:08
 Operator : MA/JU
 Sample : P1398-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	52	rVB	62114	87324	2.09%	0.185%
2	3.740	108	111	129	rBV	271749	454855	10.89%	0.965%
3	4.063	162	166	172	rVB	47771	66737	1.60%	0.142%
4	5.516	408	413	415	rBV6	6484	9694	0.23%	0.021%
5	5.893	472	477	482	rVB5	4530	8596	0.21%	0.018%
6	7.046	667	673	683	rVV	239311	385000	9.21%	0.817%
7	7.222	696	703	717	rBV	1081553	1685018	40.32%	3.575%
8	7.404	728	734	745	rBV	943876	1510896	36.16%	3.205%
9	7.504	746	751	752	rVV4	3919	4951	0.12%	0.011%
10	7.881	808	815	823	rBV	836759	1339106	32.05%	2.841%
11	7.946	823	826	831	rVB6	3111	5166	0.12%	0.011%
12	8.587	927	935	946	rBV	696277	1089966	26.08%	2.312%
13	9.045	1006	1013	1024	rBV	1161984	1911012	45.73%	4.054%
14	9.440	1075	1080	1084	rVB3	6045	9739	0.23%	0.021%
15	9.634	1109	1113	1119	rVB7	4735	8668	0.21%	0.018%
16	9.763	1127	1135	1144	rBV	798225	1318763	31.56%	2.798%
17	10.298	1218	1226	1239	rBV	1186511	1964995	47.03%	4.168%
18	10.681	1283	1291	1299	rVV	1027829	1768104	42.31%	3.751%
19	10.822	1306	1315	1330	rBV	1082449	1902603	45.53%	4.036%
20	11.234	1381	1385	1391	rBV8	3431	7782	0.19%	0.017%
21	11.439	1414	1420	1424	rBV4	13001	24448	0.59%	0.052%
22	12.192	1544	1548	1553	rBV5	2563	4390	0.11%	0.009%
23	12.269	1553	1561	1567	rBV2	22560	38143	0.91%	0.081%
24	12.881	1658	1665	1672	rVV5	10666	20348	0.49%	0.043%
25	13.145	1703	1710	1717	rBV3	47934	85525	2.05%	0.181%
26	13.428	1753	1758	1762	rVB5	11634	18140	0.43%	0.038%
27	13.504	1768	1771	1777	rVB7	3035	4349	0.10%	0.009%
28	13.857	1825	1831	1835	rBV7	3707	6253	0.15%	0.013%
29	13.945	1839	1846	1853	rBV	1955452	2715406	64.98%	5.760%
30	14.051	1860	1864	1868	rBV5	2420	4333	0.10%	0.009%
31	14.092	1868	1871	1875	rVB5	3775	5158	0.12%	0.011%
32	14.216	1879	1892	1900	rBV2	2326736	3430042	82.09%	7.276%
33	14.292	1901	1905	1914	rVB	25825	44766	1.07%	0.095%
34	14.522	1937	1944	1950	rBV	1293355	1885802	45.13%	4.000%
35	14.722	1966	1978	1991	rBV2	98112	203057	4.86%	0.431%
36	14.945	2011	2016	2020	rVB7	8097	12799	0.31%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029620.D
 Acq On : 09 Feb 2024 21:08
 Operator : MA/JU
 Sample : P1398-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	15.333	2076	2082	2083	rBV3	6272	9658	0.23%	0.020%
38	15.357	2083	2086	2094	rVB	19099	27929	0.67%	0.059%
39	15.516	2105	2113	2121	rBV	2707304	3992126	95.54%	8.469%
40	15.639	2126	2134	2143	rBV	696202	947330	22.67%	2.010%
41	15.757	2149	2154	2159	rVB4	12870	19311	0.46%	0.041%
42	15.892	2174	2177	2185	rVB10	4059	9994	0.24%	0.021%
43	16.075	2205	2208	2214	rVV7	3524	5197	0.12%	0.011%
44	16.298	2241	2246	2251	rBV7	6565	10491	0.25%	0.022%
45	16.751	2320	2323	2327	rBV5	3909	5371	0.13%	0.011%
46	16.951	2353	2357	2360	rBV5	3302	4317	0.10%	0.009%
47	17.045	2368	2373	2377	rBV5	7230	10687	0.26%	0.023%
48	17.092	2377	2381	2387	rVB7	2577	5217	0.12%	0.011%
49	17.274	2406	2412	2419	rBV	1318362	1840068	44.04%	3.903%
50	17.374	2422	2429	2440	rBV2	2702908	3923910	93.90%	8.324%
51	17.574	2459	2463	2471	rVB	16041	24474	0.59%	0.052%
52	17.963	2525	2529	2534	rVB4	8178	10872	0.26%	0.023%
53	18.069	2543	2547	2554	rVB10	5528	10470	0.25%	0.022%
54	18.180	2562	2566	2572	rBV2	65237	90839	2.17%	0.193%
55	18.457	2609	2613	2615	rBV5	5980	6988	0.17%	0.015%
56	19.233	2741	2745	2750	rVB2	31617	43432	1.04%	0.092%
57	19.304	2752	2757	2762	rBV2	26805	42686	1.02%	0.091%
58	19.380	2768	2770	2773	rVB4	5071	4951	0.12%	0.011%
59	19.468	2781	2785	2790	rBV2	36502	43810	1.05%	0.093%
60	19.627	2809	2812	2813	rBV3	8109	8141	0.19%	0.017%
61	19.668	2813	2819	2828	rVV	2958339	4106714	98.28%	8.712%
62	21.204	3076	3080	3085	rBV6	32794	49239	1.18%	0.104%
63	21.468	3120	3125	3137	rBV	1250074	1738467	41.60%	3.688%
64	23.692	3496	3503	3517	rBV2	2009038	4178611	100.00%	8.864%
65	23.845	3522	3529	3542	rVB	924066	1926385	46.10%	4.087%




Sum of corrected areas: 47139619

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029620.D
Acq On : 09 Feb 2024 21:08
Operator : MA/JU
Sample : P1398-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

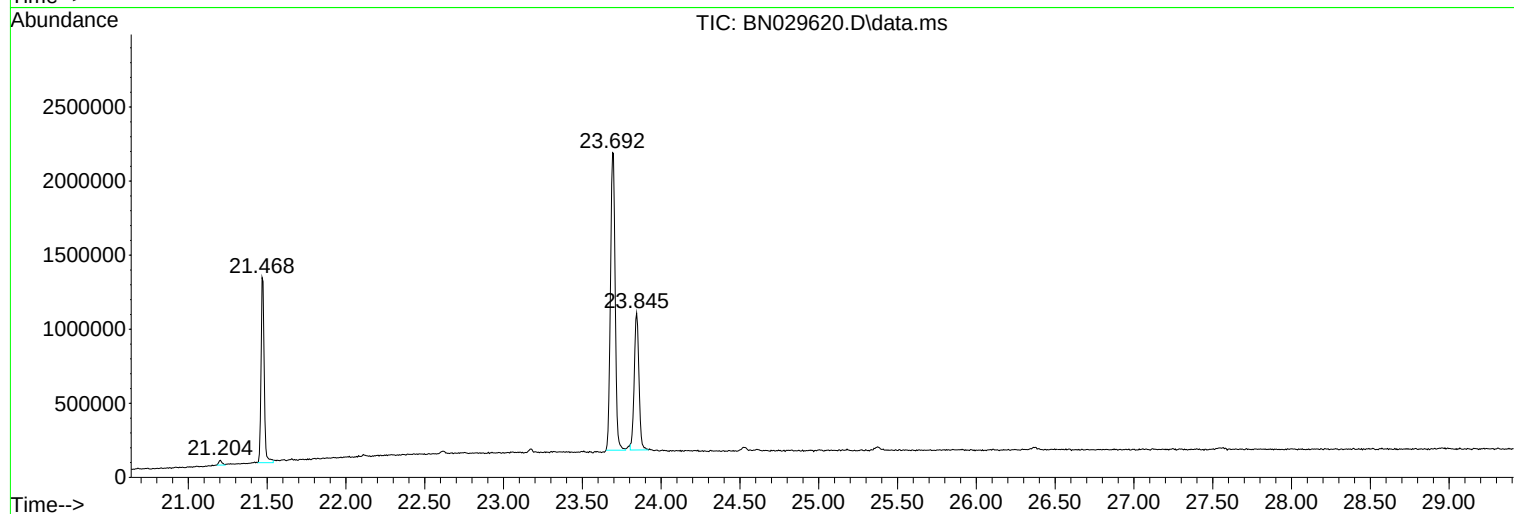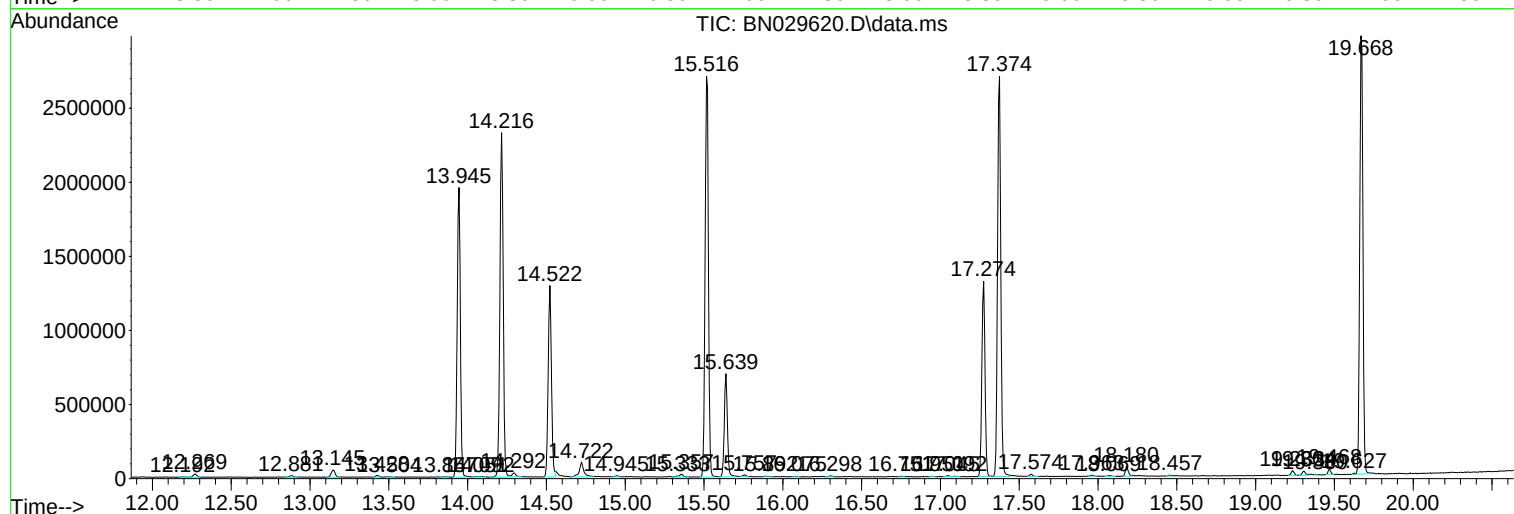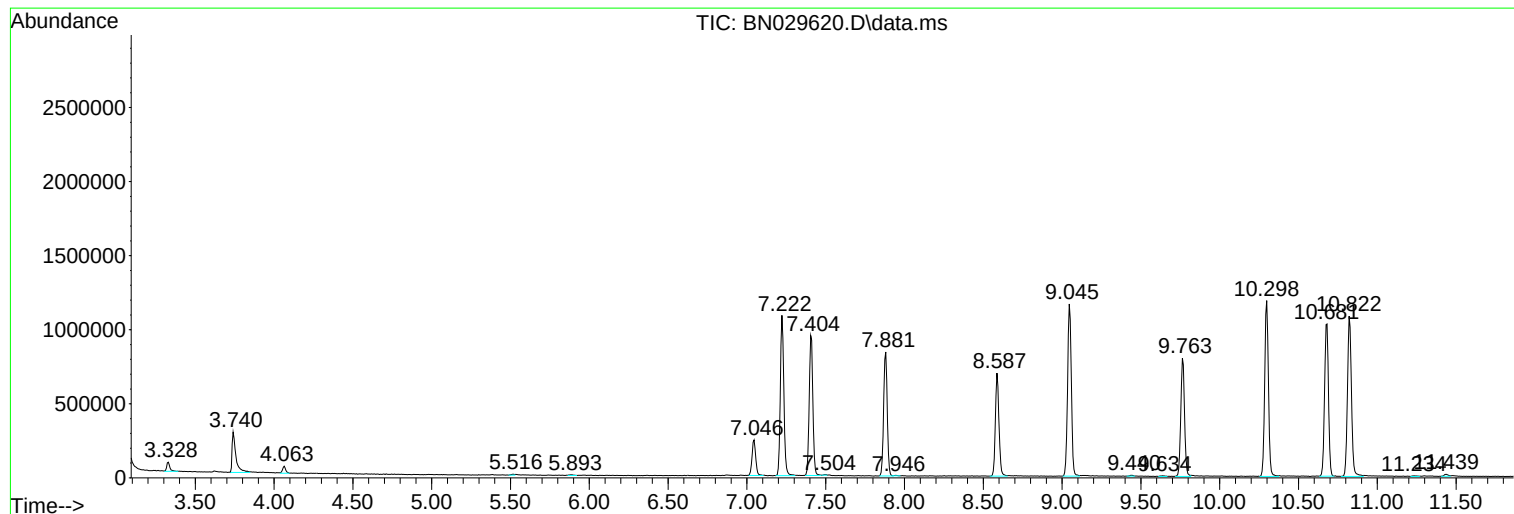

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029620.D
Acq On : 09 Feb 2024 21:08
Operator : MA/JU
Sample : P1398-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029620.D
Acq On : 09 Feb 2024 21:08
Operator : MA/JU
Sample : P1398-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------