

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029621.D
 Acq On : 09 Feb 2024 21:45
 Operator : MA/JU
 Sample : P1398-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029621.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	49	rVB	56428	78217	1.92%	0.169%
2	3.740	107	111	129	rBV	314979	532335	13.06%	1.151%
3	4.063	161	166	175	rVB	244381	331318	8.13%	0.717%
4	5.516	409	413	415	rBV4	6754	8426	0.21%	0.018%
5	5.887	472	476	481	rVB6	3828	6021	0.15%	0.013%
6	7.045	666	673	683	rBV	225351	357389	8.76%	0.773%
7	7.222	696	703	719	rBV	980704	1575330	38.63%	3.407%
8	7.410	727	735	747	rBV	886847	1431497	35.11%	3.096%
9	7.498	747	750	753	rBV4	4414	5338	0.13%	0.012%
10	7.881	808	815	823	rBV	836065	1322169	32.43%	2.860%
11	8.586	928	935	948	rBV	631537	1023802	25.11%	2.214%
12	9.045	1005	1013	1025	rBV	1101104	1834391	44.99%	3.967%
13	9.210	1037	1041	1045	rVB7	2434	4200	0.10%	0.009%
14	9.445	1074	1081	1084	rBV5	6099	11162	0.27%	0.024%
15	9.763	1127	1135	1146	rBV	742210	1266960	31.07%	2.740%
16	10.298	1217	1226	1236	rBV	1126264	1853430	45.45%	4.009%
17	10.681	1283	1291	1302	rVB	1063395	1818735	44.60%	3.933%
18	10.822	1305	1315	1329	rBV	1098514	1951746	47.87%	4.221%
19	11.445	1415	1421	1428	rBV4	9047	18023	0.44%	0.039%
20	12.269	1557	1561	1568	rVB2	20335	31927	0.78%	0.069%
21	12.480	1595	1597	1604	rVB5	3127	4411	0.11%	0.010%
22	13.151	1705	1711	1718	rVB	48808	71631	1.76%	0.155%
23	13.427	1752	1758	1764	rVB3	14132	21087	0.52%	0.046%
24	13.492	1764	1769	1775	rBV7	3395	6684	0.16%	0.014%
25	13.945	1838	1846	1856	rBV	1959328	2672916	65.55%	5.781%
26	14.216	1882	1892	1911	rBV2	2237131	3343379	81.99%	7.231%
27	14.521	1938	1944	1955	rBV	1322385	1941698	47.62%	4.199%
28	14.721	1972	1978	1990	rBV	74372	150219	3.68%	0.325%
29	14.951	2015	2017	2021	rVB4	3432	4222	0.10%	0.009%
30	15.321	2077	2080	2084	rBV6	3962	7038	0.17%	0.015%
31	15.516	2105	2113	2125	rBV	2603107	3915650	96.03%	8.469%
32	15.639	2128	2134	2146	rBV	679028	946272	23.21%	2.047%
33	15.757	2151	2154	2163	rVB4	11943	20907	0.51%	0.045%
34	16.080	2205	2209	2214	rVB8	4228	6495	0.16%	0.014%
35	16.251	2234	2238	2243	rBV7	3459	5550	0.14%	0.012%
36	16.304	2244	2247	2252	rVB5	6469	10253	0.25%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029621.D
 Acq On : 09 Feb 2024 21:45
 Operator : MA/JU
 Sample : P1398-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	16.421	2263	2267	2272	rVB8	3280	5924	0.15%	0.013%
38	16.963	2354	2359	2360	rBV5	3214	4429	0.11%	0.010%
39	17.057	2371	2375	2380	rBV6	4121	7377	0.18%	0.016%
40	17.274	2405	2412	2422	rBV	1412007	1906971	46.77%	4.124%
41	17.374	2422	2429	2441	rVV2	2790567	4026211	98.74%	8.708%
42	17.474	2444	2446	2450	rVB5	6578	9392	0.23%	0.020%
43	17.574	2458	2463	2467	rBV5	3657	7263	0.18%	0.016%
44	17.968	2524	2530	2534	rBV4	11329	15108	0.37%	0.033%
45	18.186	2562	2567	2573	rBV3	36402	57323	1.41%	0.124%
46	19.239	2740	2746	2751	rBV2	29442	43859	1.08%	0.095%
47	19.309	2753	2758	2762	rBV	26041	38697	0.95%	0.084%
48	19.468	2781	2785	2792	rBV7	21432	31040	0.76%	0.067%
49	19.627	2809	2812	2813	rBV2	6533	5316	0.13%	0.011%
50	19.674	2814	2820	2827	rVV	2985070	4077567	100.00%	8.819%
51	21.203	3077	3080	3084	rBV4	24432	31692	0.78%	0.069%
52	21.474	3120	3126	3143	rBV	1241871	1689998	41.45%	3.655%
53	23.697	3496	3504	3517	rBV2	1941004	3925985	96.28%	8.491%
54	23.845	3523	3529	3541	rVB	892623	1762242	43.22%	3.811%




Sum of corrected areas: 46237222

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029621.D
Acq On : 09 Feb 2024 21:45
Operator : MA/JU
Sample : P1398-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

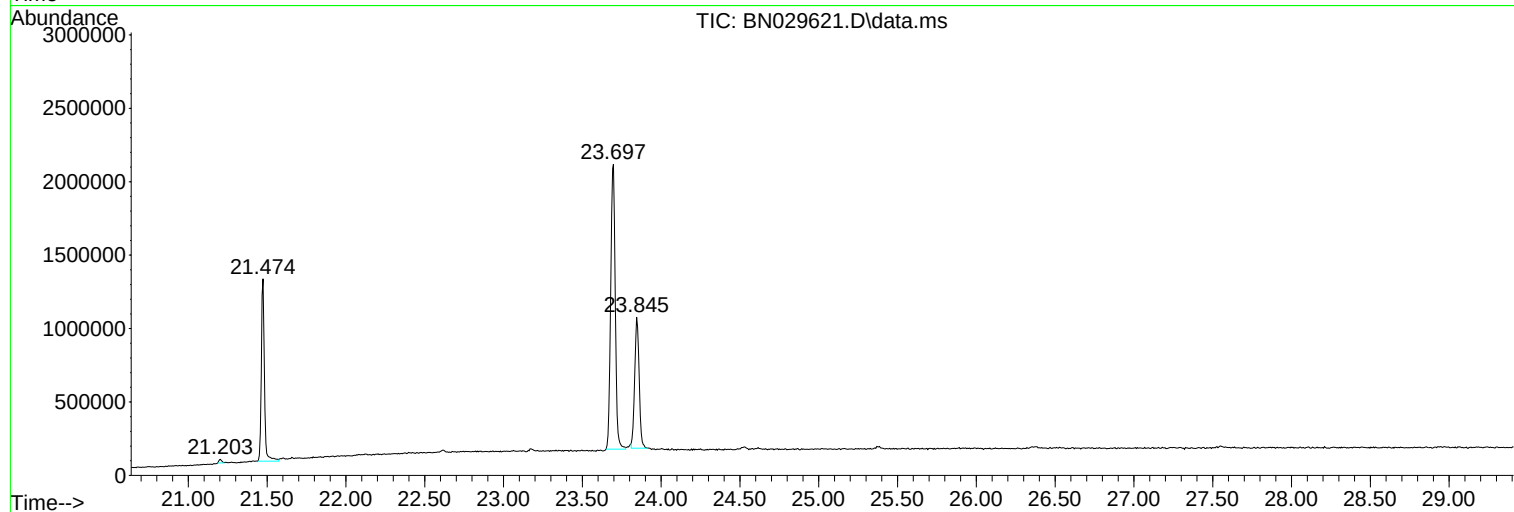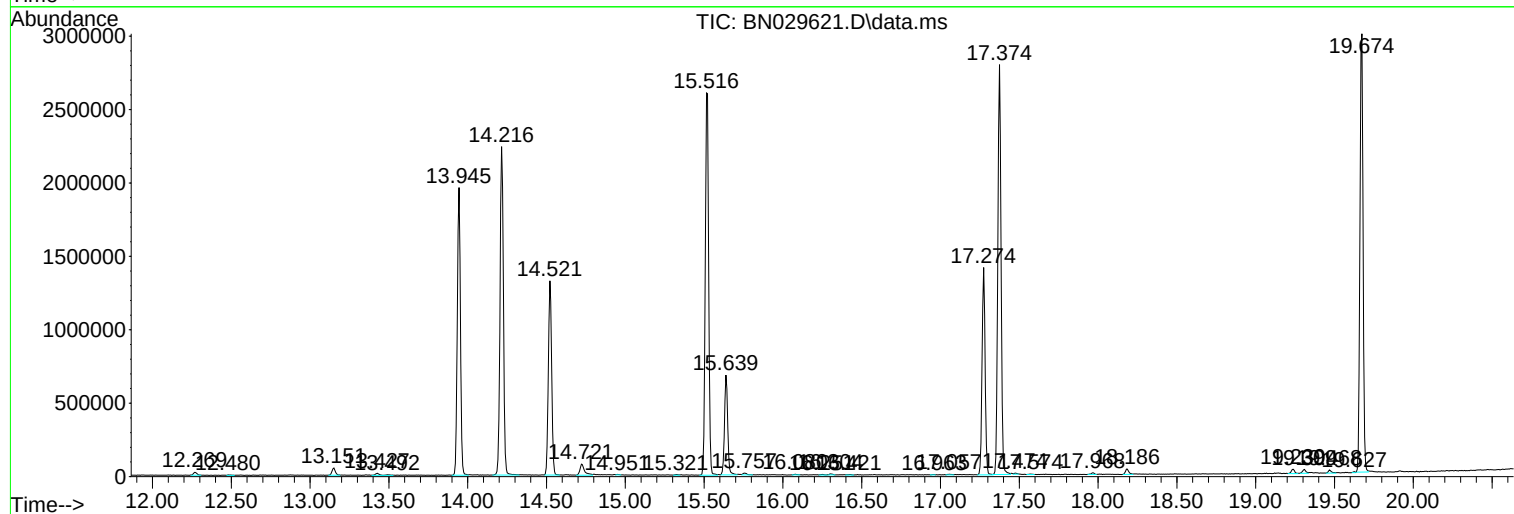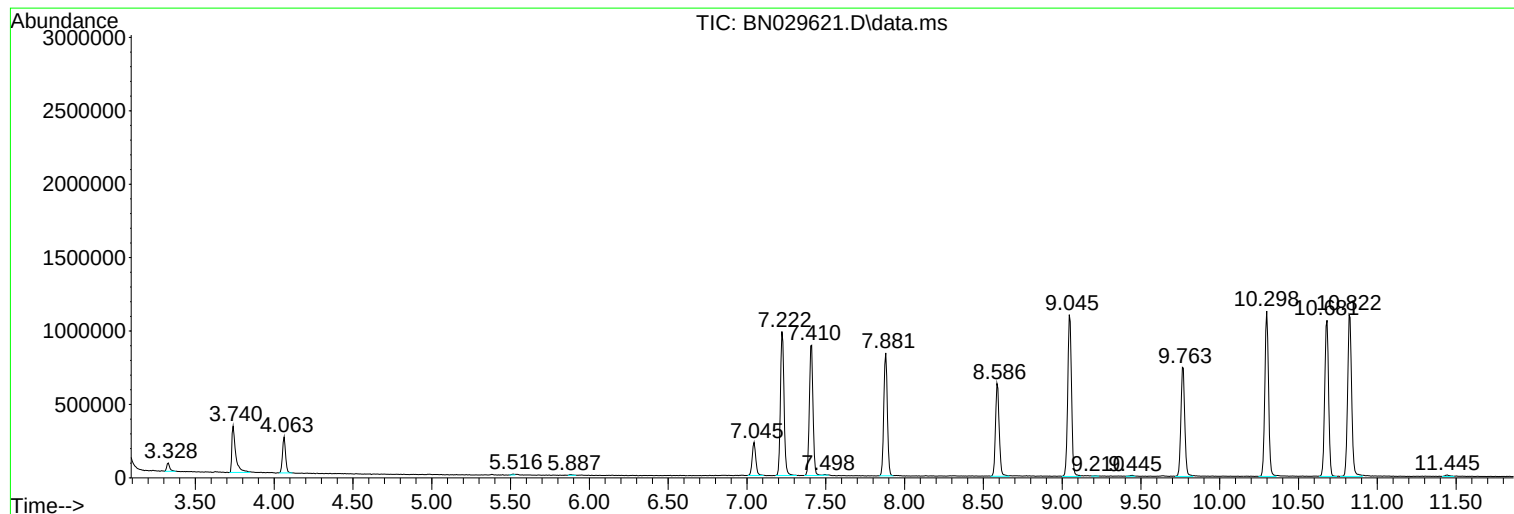

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029621.D
Acq On : 09 Feb 2024 21:45
Operator : MA/JU
Sample : P1398-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029621.D
Acq On : 09 Feb 2024 21:45
Operator : MA/JU
Sample : P1398-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc