

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029622.D
 Acq On : 09 Feb 2024 22:21
 Operator : MA/JU
 Sample : P1398-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	53	rVB	61294	90691	2.19%	0.199%
2	3.740	107	111	126	rBV	346053	559695	13.51%	1.226%
3	4.063	162	166	173	rVB	31922	43408	1.05%	0.095%
4	5.381	389	390	397	rVB6	4811	6599	0.16%	0.014%
5	5.516	410	413	420	rVB6	6571	13849	0.33%	0.030%
6	5.887	474	476	481	rVB4	5731	7062	0.17%	0.015%
7	5.946	481	486	490	rVB7	6168	11617	0.28%	0.025%
8	6.957	656	658	663	rVB5	2846	4646	0.11%	0.010%
9	7.046	667	673	683	rBV	230730	366369	8.84%	0.803%
10	7.222	697	703	719	rBV	1030907	1668044	40.27%	3.655%
11	7.410	728	735	745	rBV	947355	1500400	36.22%	3.288%
12	7.493	747	749	752	rBV4	4872	4537	0.11%	0.010%
13	7.881	806	815	825	rBV	803847	1285758	31.04%	2.817%
14	8.587	929	935	944	rBV	627250	1025353	24.75%	2.247%
15	9.046	1006	1013	1024	rBV	1131273	1887295	45.56%	4.136%
16	9.151	1029	1031	1035	rVB5	4698	6296	0.15%	0.014%
17	9.769	1127	1136	1148	rBV	782323	1313198	31.70%	2.878%
18	10.298	1218	1226	1238	rBV	1158291	1938892	46.81%	4.249%
19	10.681	1283	1291	1301	rVB	1001692	1678181	40.51%	3.677%
20	10.828	1306	1316	1329	rBV	1136179	2042716	49.32%	4.476%
21	12.269	1556	1561	1570	rBV2	18502	33670	0.81%	0.074%
22	12.881	1662	1665	1669	rVB5	3120	5654	0.14%	0.012%
23	13.151	1706	1711	1717	rBV2	34105	51064	1.23%	0.112%
24	13.428	1753	1758	1764	rBV3	16128	26704	0.64%	0.059%
25	13.504	1764	1771	1774	rVB8	3006	5423	0.13%	0.012%
26	13.945	1838	1846	1857	rBV	1921152	2612016	63.06%	5.724%
27	14.216	1885	1892	1901	rBV	2311256	3302761	79.74%	7.237%
28	14.522	1937	1944	1954	rBV	1210914	1760947	42.51%	3.859%
29	14.722	1973	1978	1993	rBV	68443	141852	3.42%	0.311%
30	14.957	2012	2018	2020	rVB7	3928	7427	0.18%	0.016%
31	15.516	2107	2113	2121	rBV	2559330	3786038	91.40%	8.296%
32	15.639	2128	2134	2143	rBV	627673	874703	21.12%	1.917%
33	15.763	2149	2155	2160	rVB6	10756	17772	0.43%	0.039%
34	16.239	2235	2236	2243	rVV6	3754	5583	0.13%	0.012%
35	16.304	2243	2247	2253	rVB6	7141	10843	0.26%	0.024%
36	16.798	2326	2331	2333	rBV5	2496	4228	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029622.D
 Acq On : 09 Feb 2024 22:21
 Operator : MA/JU
 Sample : P1398-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.051	2369	2374	2378	rBV7	4245	6658	0.16%	0.015%
38	17.275	2405	2412	2420	rBV	1284166	1792368	43.27%	3.928%
39	17.375	2422	2429	2444	rBV	2672310	3750630	90.55%	8.219%
40	17.969	2527	2530	2536	rVB6	3303	5239	0.13%	0.011%
41	18.180	2563	2566	2575	rVB5	13784	18060	0.44%	0.040%
42	19.233	2741	2745	2751	rVB2	29256	40407	0.98%	0.089%
43	19.304	2754	2757	2762	rVV2	23589	34928	0.84%	0.077%
44	19.351	2762	2765	2768	rVV5	4189	4617	0.11%	0.010%
45	19.433	2776	2779	2781	rBV4	3057	4198	0.10%	0.009%
46	19.474	2781	2786	2788	rVV5	10610	15476	0.37%	0.034%
47	19.627	2809	2812	2813	rBV2	7484	7606	0.18%	0.017%
48	19.674	2813	2820	2829	rVV	2864970	4061934	98.06%	8.901%
49	21.474	3120	3126	3139	rBV	1230972	1717072	41.45%	3.763%
50	23.692	3496	3503	3517	rBV2	2116869	4142149	100.00%	9.077%
51	23.845	3522	3529	3540	rVB	968748	1932703	46.66%	4.235%




Sum of corrected areas: 45635336

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029622.D
Acq On : 09 Feb 2024 22:21
Operator : MA/JU
Sample : P1398-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

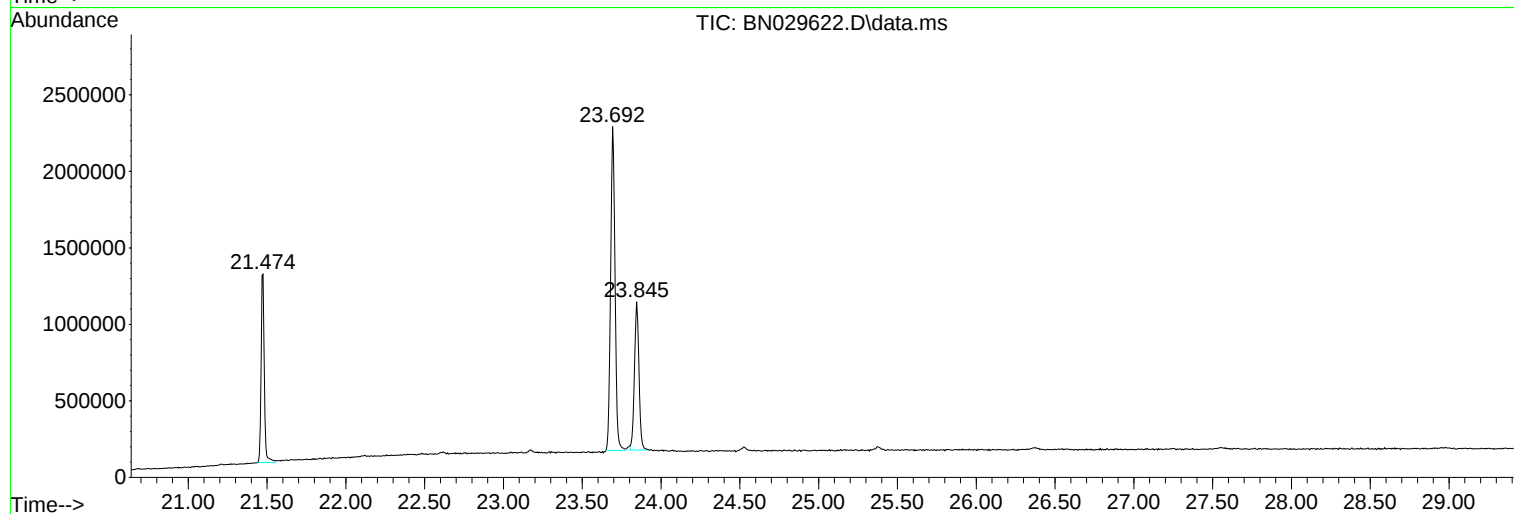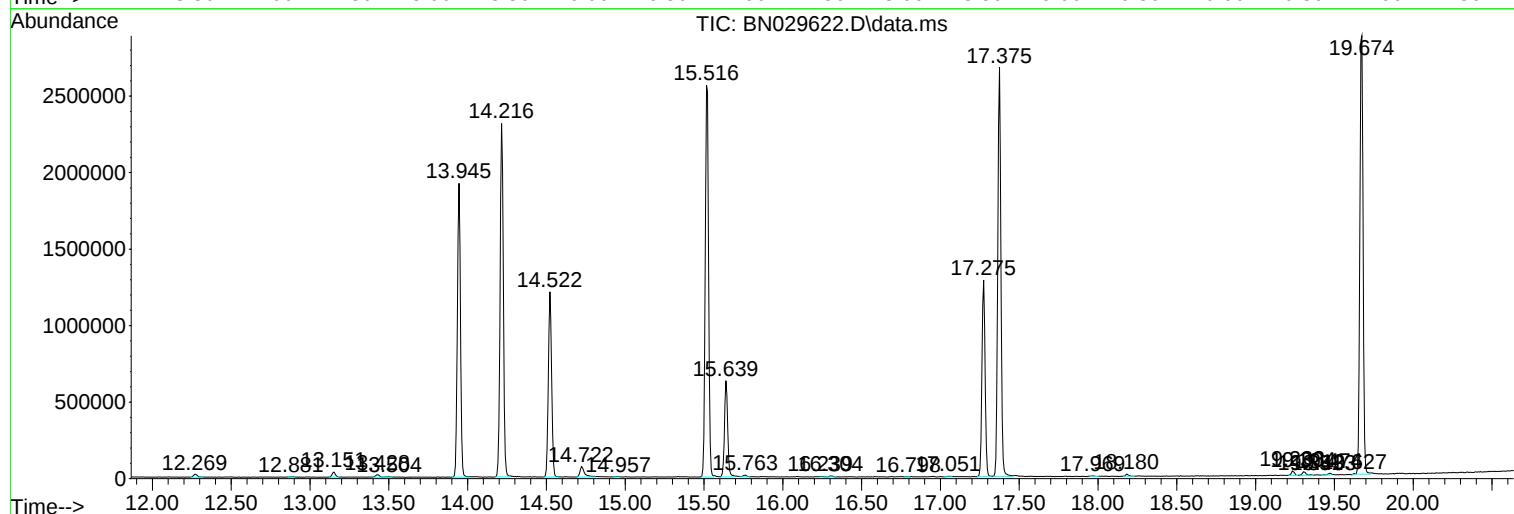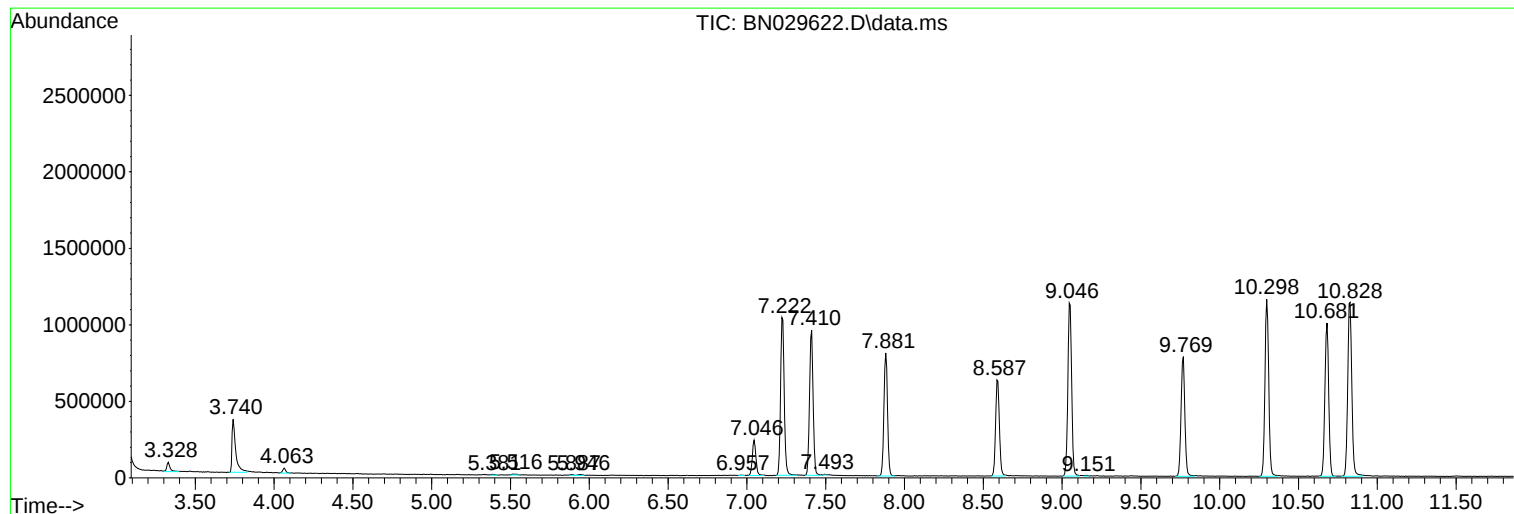

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029622.D
Acq On : 09 Feb 2024 22:21
Operator : MA/JU
Sample : P1398-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029622.D
Acq On : 09 Feb 2024 22:21
Operator : MA/JU
Sample : P1398-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc