

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029623.D
 Acq On : 09 Feb 2024 22:57
 Operator : MA/JU
 Sample : P1398-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	46	rVB	60610	73995	1.68%	0.159%
2	3.740	108	111	130	rBV	342287	567877	12.87%	1.216%
3	4.064	162	166	171	rVB	32569	41632	0.94%	0.089%
4	5.522	410	414	421	rVB7	5747	13170	0.30%	0.028%
5	5.934	481	484	487	rVV3	5114	6059	0.14%	0.013%
6	7.046	666	673	684	rBV	259007	407916	9.25%	0.874%
7	7.222	697	703	717	rBV	1080463	1740327	39.45%	3.728%
8	7.411	728	735	746	rBV	1004773	1591341	36.07%	3.409%
9	7.881	807	815	825	rBV	774578	1232171	27.93%	2.639%
10	8.587	928	935	946	rBV	691644	1129212	25.60%	2.419%
11	9.046	1006	1013	1029	rBV	1181139	1968833	44.63%	4.217%
12	9.440	1075	1080	1089	rVB5	8230	15284	0.35%	0.033%
13	9.769	1127	1136	1146	rBV	801848	1356185	30.74%	2.905%
14	10.299	1218	1226	1239	rBV	1236719	2008319	45.53%	4.302%
15	10.681	1283	1291	1299	rVB	959257	1613360	36.57%	3.456%
16	10.828	1308	1316	1329	rBV	1203490	2118377	48.02%	4.538%
17	12.275	1554	1562	1568	rBV2	19790	37882	0.86%	0.081%
18	13.152	1704	1711	1718	rBV	39471	62068	1.41%	0.133%
19	13.428	1753	1758	1764	rBV5	13971	20819	0.47%	0.045%
20	13.946	1840	1846	1858	rBV	1998722	2716799	61.59%	5.820%
21	14.216	1885	1892	1901	rBV	2344627	3398367	77.04%	7.280%
22	14.522	1938	1944	1956	rVV	1152557	1692910	38.38%	3.626%
23	14.722	1972	1978	1990	rBV	81403	159648	3.62%	0.342%
24	15.116	2042	2045	2050	rBV5	2718	4543	0.10%	0.010%
25	15.522	2106	2114	2121	rBV	2648593	3944304	89.41%	8.449%
26	15.640	2128	2134	2144	rBV	657746	910762	20.65%	1.951%
27	15.757	2150	2154	2161	rVB4	13772	23306	0.53%	0.050%
28	16.304	2242	2247	2253	rVB6	8571	13658	0.31%	0.029%
29	16.957	2354	2358	2361	rVB6	3593	5602	0.13%	0.012%
30	17.057	2371	2375	2380	rBV7	3861	8785	0.20%	0.019%
31	17.275	2405	2412	2420	rBV	1210078	1697015	38.47%	3.635%
32	17.375	2422	2429	2443	rVV2	2778274	3981936	90.27%	8.530%
33	17.475	2443	2446	2452	rVB7	7650	14505	0.33%	0.031%
34	17.963	2526	2529	2531	rBV4	4124	4891	0.11%	0.010%
35	18.181	2563	2566	2573	rBV6	6914	10667	0.24%	0.023%
36	19.234	2741	2745	2752	rBV3	27948	37625	0.85%	0.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029623.D
Acq On : 09 Feb 2024 22:57
Operator : MA/JU
Sample : P1398-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.304	2754	2757	2762	rVB	23520	31848	0.72%	0.068%
38	19.475	2781	2786	2789	rBV6	8170	13431	0.30%	0.029%
39	19.675	2813	2820	2828	rBV	3072177	4217691	95.61%	9.035%
40	21.469	3120	3125	3139	rBV	1167977	1607131	36.43%	3.443%
41	23.692	3495	3503	3516	rBV2	2197151	4411288	100.00%	9.449%
42	23.845	3522	3529	3538	rVB2	870366	1771454	40.16%	3.795%




Sum of corrected areas: 46682993

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029623.D
Acq On : 09 Feb 2024 22:57
Operator : MA/JU
Sample : P1398-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

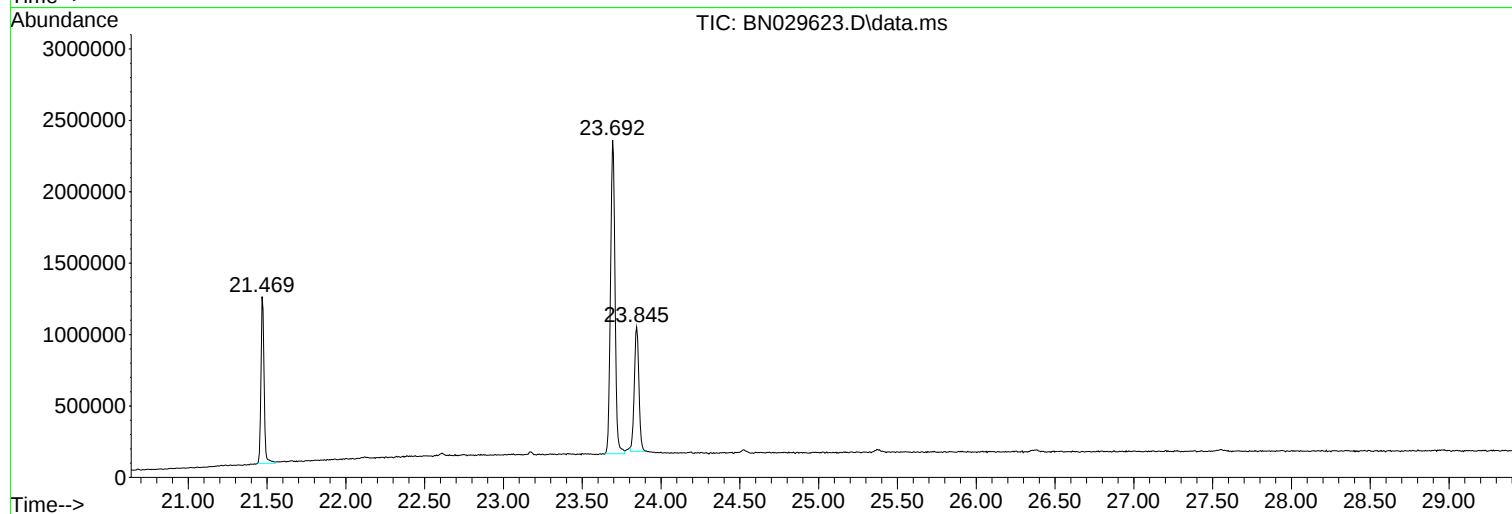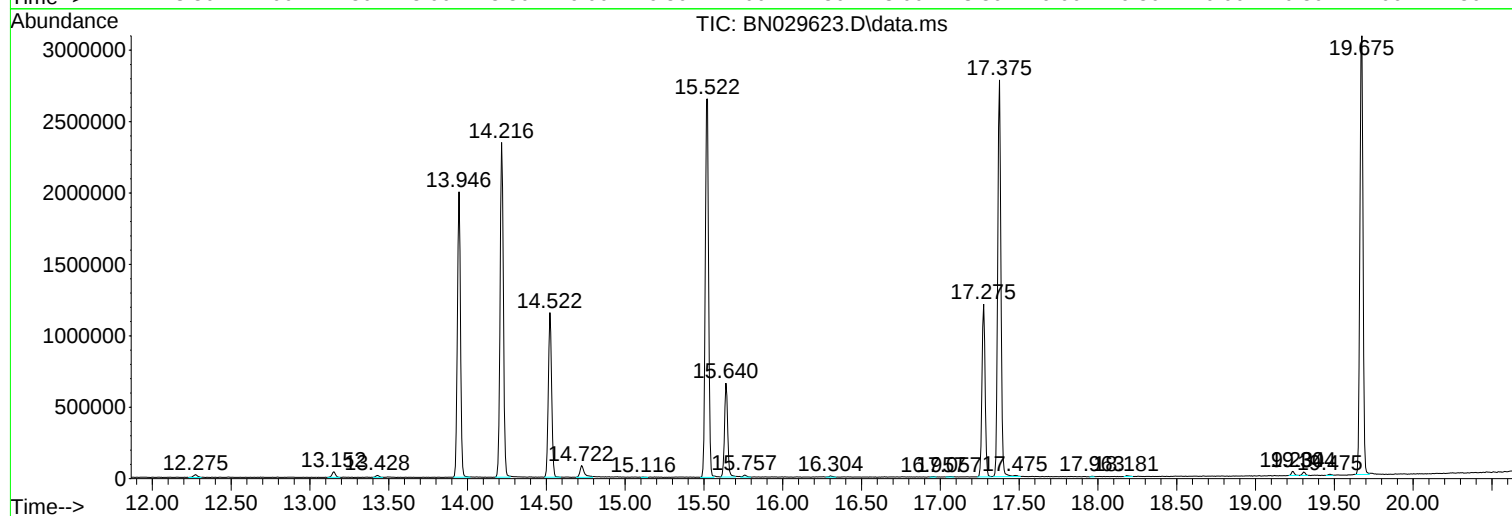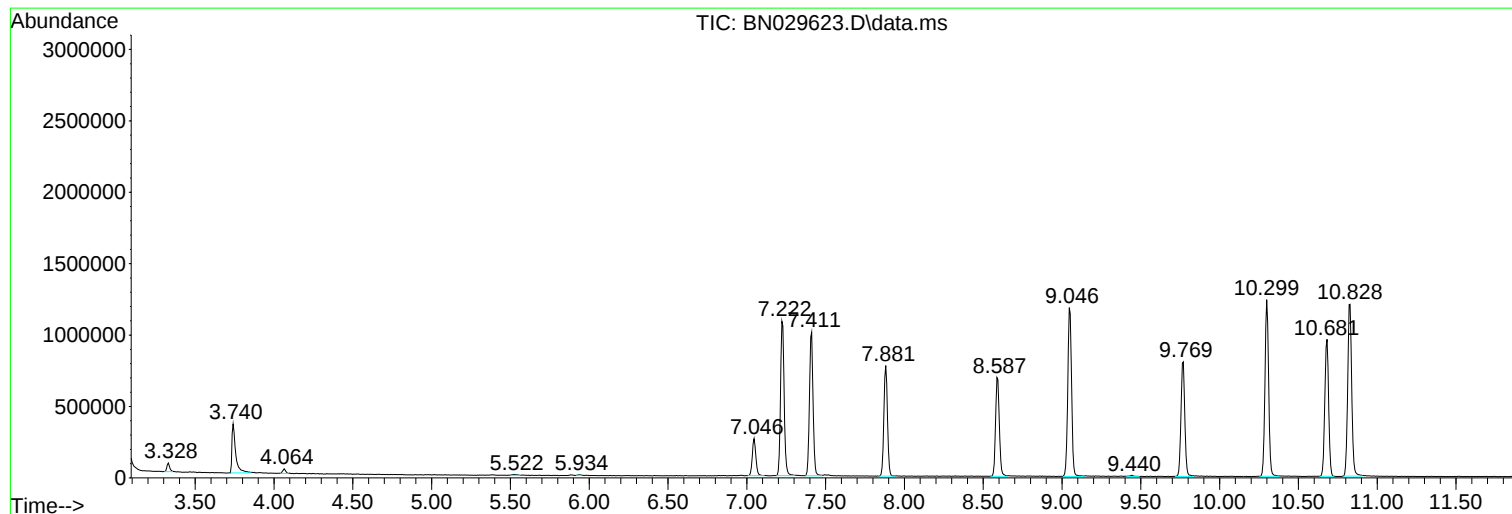

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029623.D
Acq On : 09 Feb 2024 22:57
Operator : MA/JU
Sample : P1398-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029623.D
Acq On : 09 Feb 2024 22:57
Operator : MA/JU
Sample : P1398-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
