

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029625.D
 Acq On : 10 Feb 2024 00:09
 Operator : MA/JU
 Sample : P1398-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	48	rVB	58196	75099	1.83%	0.163%
2	3.740	108	111	127	rBV	267079	443715	10.81%	0.965%
3	4.064	162	166	172	rVB	31975	43862	1.07%	0.095%
4	4.575	249	253	264	rVB	120308	165803	4.04%	0.361%
5	5.011	324	327	331	rVB4	5037	6920	0.17%	0.015%
6	5.305	373	377	385	rBV2	34752	55655	1.36%	0.121%
7	5.387	387	391	397	rVB	15093	21547	0.53%	0.047%
8	5.516	409	413	421	rBV	39734	84195	2.05%	0.183%
9	5.887	471	476	485	rVB	22838	38006	0.93%	0.083%
10	6.534	581	586	593	rVB4	10217	17500	0.43%	0.038%
11	6.852	635	640	644	rBV4	8381	13498	0.33%	0.029%
12	6.963	654	659	664	rVB2	18065	26997	0.66%	0.059%
13	7.046	664	673	679	rVV	264315	424928	10.36%	0.924%
14	7.099	679	682	690	rVB5	9385	16679	0.41%	0.036%
15	7.222	697	703	719	rVB	1015901	1636729	39.89%	3.559%
16	7.410	727	735	746	rBV	968918	1530692	37.31%	3.328%
17	7.522	748	754	758	rVB	25845	44986	1.10%	0.098%
18	7.881	808	815	824	rBV	774403	1221840	29.78%	2.657%
19	7.987	829	833	835	rBV5	4212	4160	0.10%	0.009%
20	8.593	929	936	946	rBV	664668	1090714	26.58%	2.372%
21	9.052	1006	1014	1026	rBV	1091009	1842838	44.91%	4.007%
22	9.446	1078	1081	1086	rVB5	3584	5065	0.12%	0.011%
23	9.769	1128	1136	1148	rBV	770643	1268248	30.91%	2.758%
24	10.298	1219	1226	1239	rBV	1146347	1889380	46.05%	4.108%
25	10.681	1282	1291	1301	rVB	964849	1598040	38.95%	3.475%
26	10.828	1307	1316	1329	rBV	1011531	1753711	42.74%	3.813%
27	11.451	1415	1422	1426	rBV7	7006	15246	0.37%	0.033%
28	11.504	1428	1431	1435	rVB6	3746	5808	0.14%	0.013%
29	12.275	1555	1562	1566	rBV2	19080	31911	0.78%	0.069%
30	12.892	1661	1667	1671	rVB7	2413	4134	0.10%	0.009%
31	13.428	1752	1758	1764	rBV3	17535	27527	0.67%	0.060%
32	13.945	1839	1846	1855	rBV	1832434	2547952	62.10%	5.540%
33	14.216	1884	1892	1903	rBV	2223732	3230175	78.73%	7.024%
34	14.522	1937	1944	1954	rBV	1165375	1694424	41.30%	3.684%
35	14.734	1973	1980	1981	rBV2	344696	466736	11.38%	1.015%
36	14.751	1981	1983	1998	rVB2	375366	497532	12.13%	1.082%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029625.D
 Acq On : 10 Feb 2024 00:09
 Operator : MA/JU
 Sample : P1398-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	15.516	2107	2113	2121	rBV	2505755	3696674	90.10%	8.038%
38	15.639	2127	2134	2144	rBV	621156	879672	21.44%	1.913%
39	15.757	2150	2154	2160	rVB6	10637	17238	0.42%	0.037%
40	16.086	2206	2210	2214	rVB6	3773	4506	0.11%	0.010%
41	16.257	2234	2239	2242	rBV5	3243	5092	0.12%	0.011%
42	16.304	2242	2247	2252	rVV5	8449	12564	0.31%	0.027%
43	16.681	2309	2311	2317	rVB5	4222	6536	0.16%	0.014%
44	17.275	2405	2412	2421	rBV	1250908	1740638	42.42%	3.785%
45	17.375	2421	2429	2446	rBV	2660306	3760130	91.64%	8.176%
46	17.575	2459	2463	2472	rVB	27371	38372	0.94%	0.083%
47	17.963	2526	2529	2539	rVB4	11843	20961	0.51%	0.046%
48	18.186	2561	2567	2573	rBV3	52271	81982	2.00%	0.178%
49	18.263	2577	2580	2584	rVB4	6002	8549	0.21%	0.019%
50	18.663	2645	2648	2653	rBV5	3909	5285	0.13%	0.011%
51	19.145	2727	2730	2734	rVB5	14862	16484	0.40%	0.036%
52	19.233	2741	2745	2750	rBV3	27902	39773	0.97%	0.086%
53	19.310	2750	2758	2762	rBV2	27001	47866	1.17%	0.104%
54	19.469	2780	2785	2791	rBV4	41107	53554	1.31%	0.116%
55	19.627	2809	2812	2813	rBV2	5565	5812	0.14%	0.013%
56	19.674	2813	2820	2828	rVV	2988476	4059169	98.93%	8.826%
57	21.204	3076	3080	3086	rBV8	25310	51715	1.26%	0.112%
58	21.474	3120	3126	3138	rBV	1208113	1690038	41.19%	3.675%
59	23.692	3496	3503	3516	rBV2	2023751	4103031	100.00%	8.922%
60	23.845	3523	3529	3538	rVB	922877	1802477	43.93%	3.919%


Sum of corrected areas: 45990370

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029625.D
Acq On : 10 Feb 2024 00:09
Operator : MA/JU
Sample : P1398-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

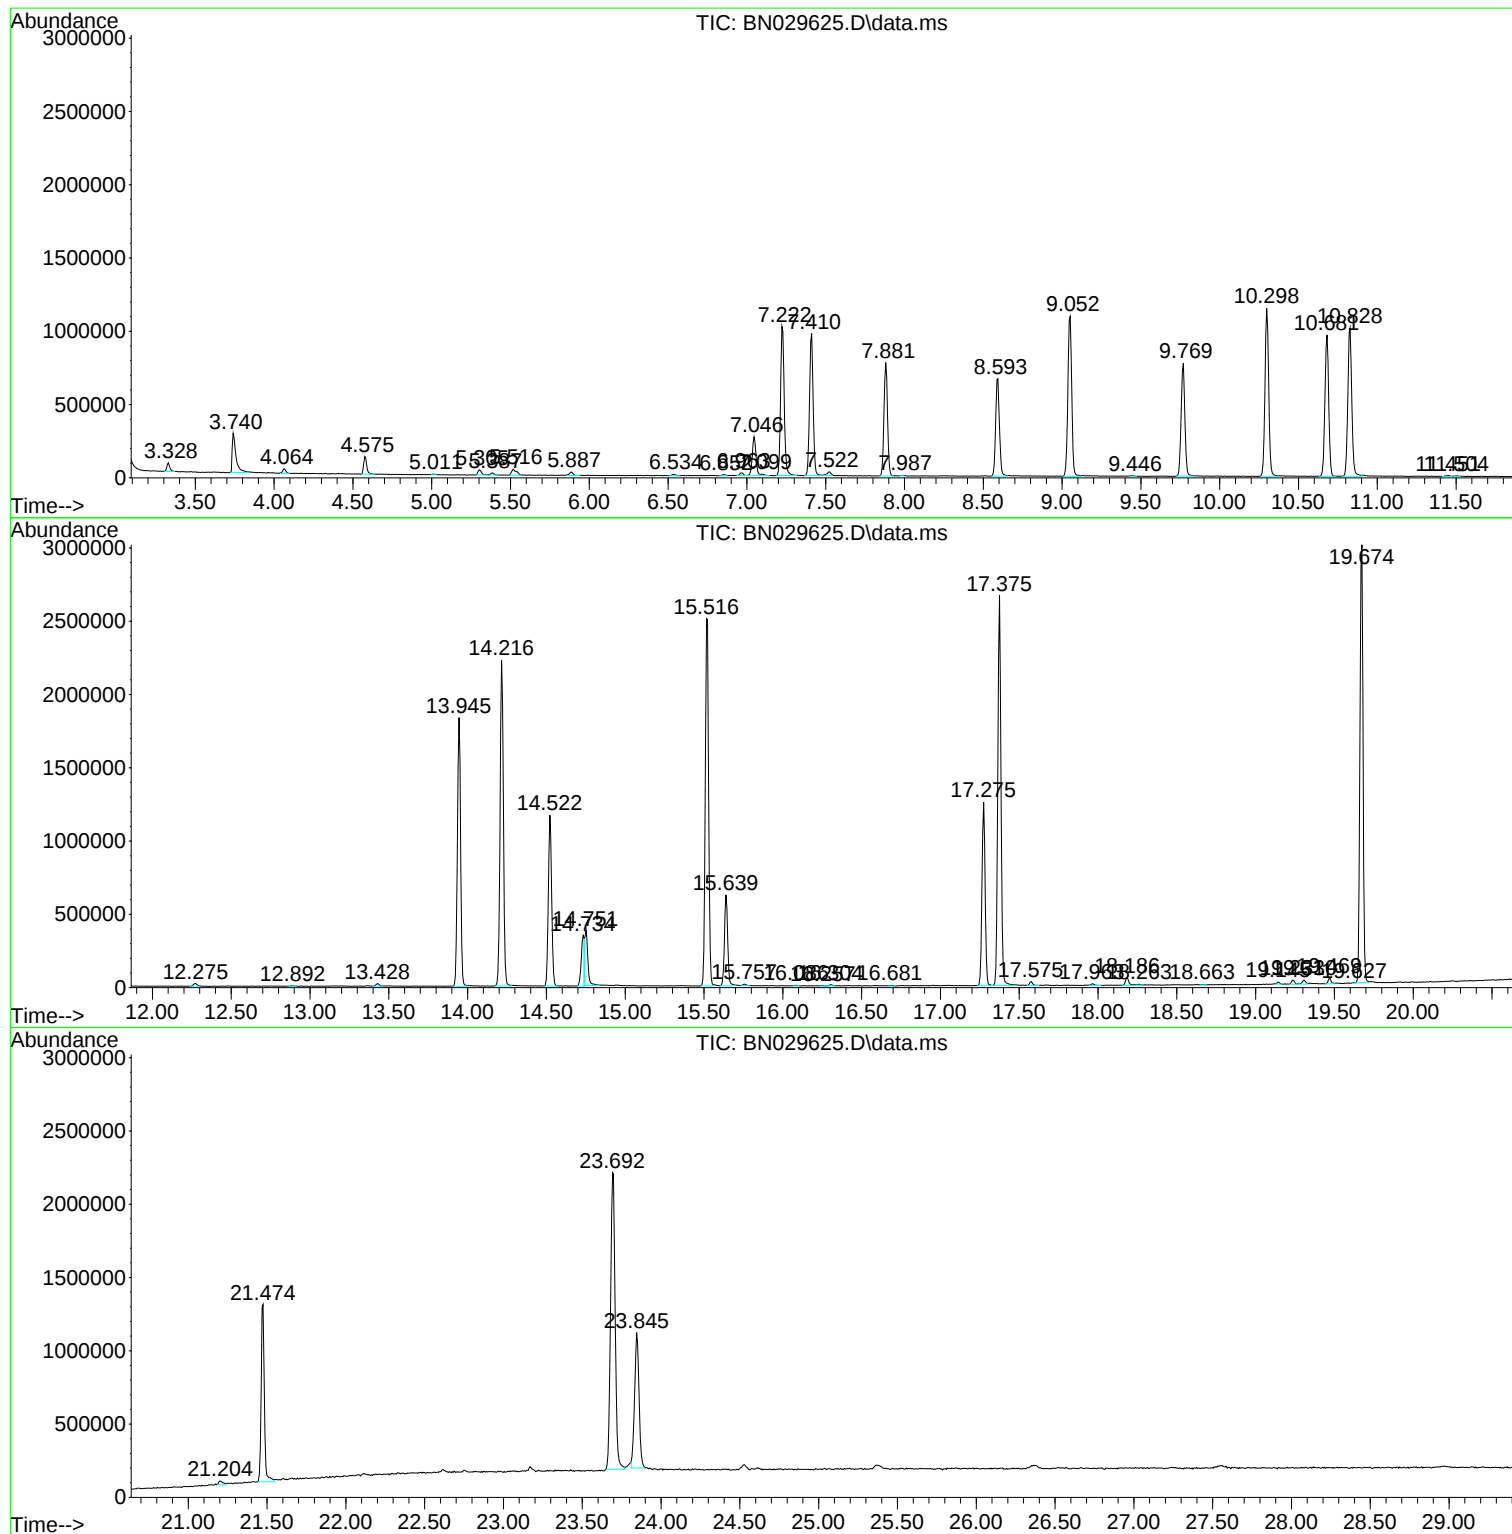

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029625.D
Acq On : 10 Feb 2024 00:09
Operator : MA/JU
Sample : P1398-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Acetic acid, butyl ester Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.575	2.71 ng/ul	165803	1,4-Dichlorobenzene-d4	7.881

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Acetic acid, butyl ester		116	C6H12O2		000123-86-4	78
2	Acetic acid, butyl ester		116	C6H12O2		000123-86-4	64
3	Acetic acid, butyl ester		116	C6H12O2		000123-86-4	64
4	Acetic acid, butyl ester		116	C6H12O2		000123-86-4	50
5	Isobutyl acetate		116	C6H12O2		000110-19-0	50

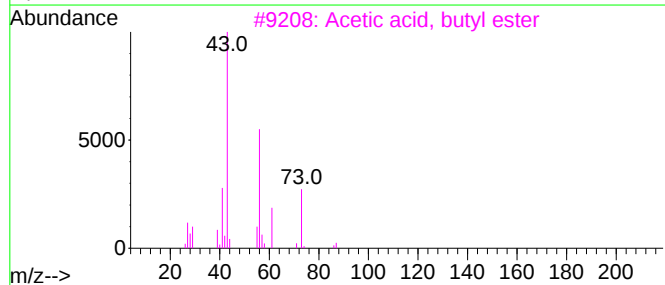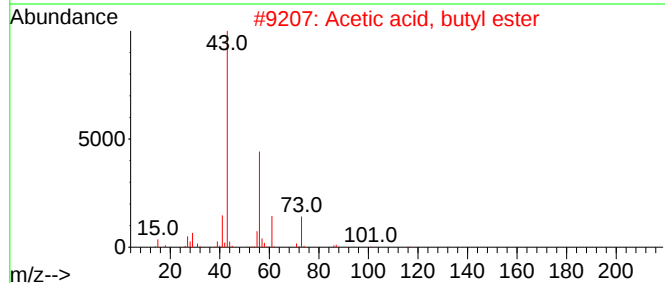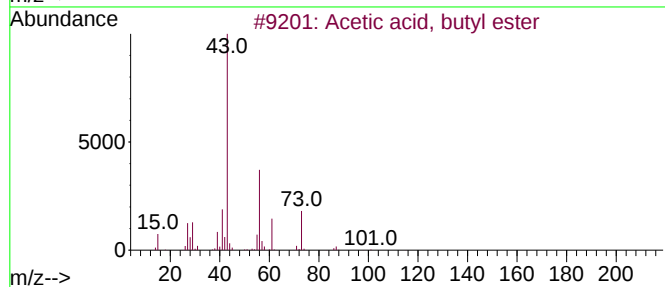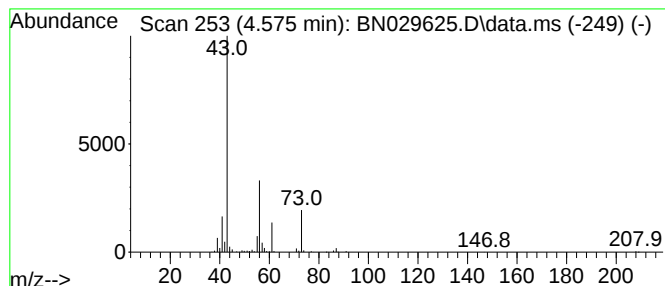

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029625.D
Acq On : 10 Feb 2024 00:09
Operator : MA/JU
Sample : P1398-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Acetic acid, bu...	4.575	2.7	ng/u1	165803	1	7.881	1221840	20.0