

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029626.D
 Acq On : 10 Feb 2024 00:45
 Operator : MA/JU
 Sample : P1398-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	47	rBV	57580	75067	1.76%	0.161%
2	3.740	108	111	127	rBV	301432	498288	11.70%	1.065%
3	4.063	162	166	172	rVB	32205	42272	0.99%	0.090%
4	4.581	250	254	257	rVB	9682	13133	0.31%	0.028%
5	5.393	387	392	395	rVB5	4968	7876	0.18%	0.017%
6	5.516	408	413	415	rBV3	12550	19095	0.45%	0.041%
7	5.887	471	476	481	rBV4	7899	12171	0.29%	0.026%
8	6.963	655	659	663	rBV7	5908	7476	0.18%	0.016%
9	7.046	666	673	687	rBV	234123	378259	8.88%	0.809%
10	7.222	696	703	717	rBV	1105963	1772153	41.61%	3.789%
11	7.410	727	735	746	rBV	980583	1549687	36.39%	3.314%
12	7.493	747	749	752	rVV4	8077	12099	0.28%	0.026%
13	7.522	752	754	761	rVB5	9670	12086	0.28%	0.026%
14	7.881	808	815	822	rBV	796278	1234582	28.99%	2.640%
15	8.593	928	936	945	rBV	639993	1062805	24.95%	2.272%
16	9.046	1006	1013	1022	rBV	1183548	1981955	46.53%	4.238%
17	9.157	1027	1032	1038	rVB2	19226	29733	0.70%	0.064%
18	9.440	1075	1080	1084	rVB6	3027	4807	0.11%	0.010%
19	9.769	1127	1136	1148	rBV	821456	1388965	32.61%	2.970%
20	10.298	1218	1226	1238	rBV	1229158	2031293	47.69%	4.343%
21	10.375	1238	1239	1244	rVB4	3638	4495	0.11%	0.010%
22	10.681	1282	1291	1303	rVB	970189	1669082	39.19%	3.569%
23	10.822	1308	1315	1327	rBV	1138913	2020311	47.44%	4.320%
24	11.422	1413	1417	1422	rVB7	2826	5229	0.12%	0.011%
25	12.110	1531	1534	1539	rBV4	4242	5351	0.13%	0.011%
26	12.269	1554	1561	1568	rVB2	20568	35413	0.83%	0.076%
27	13.357	1741	1746	1750	rBV6	7258	9002	0.21%	0.019%
28	13.428	1750	1758	1762	rVV5	15099	25867	0.61%	0.055%
29	13.498	1766	1770	1776	rVB6	4143	8972	0.21%	0.019%
30	13.945	1838	1846	1858	rBV	1987386	2774666	65.15%	5.933%
31	14.216	1885	1892	1905	rBV2	2395457	3503986	82.27%	7.492%
32	14.434	1923	1929	1933	rBV4	8792	12837	0.30%	0.027%
33	14.522	1937	1944	1954	rBV	1186824	1733627	40.70%	3.707%
34	14.634	1959	1963	1966	rBV5	3181	4607	0.11%	0.010%
35	14.728	1973	1979	1990	rBV	67875	144211	3.39%	0.308%
36	14.945	2011	2016	2017	rBV5	5096	7191	0.17%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029626.D
 Acq On : 10 Feb 2024 00:45
 Operator : MA/JU
 Sample : P1398-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	15.386	2087	2091	2095	rVB5	9016	12775	0.30%	0.027%
38	15.516	2106	2113	2126	rBV	2755054	4043834	94.95%	8.646%
39	15.639	2127	2134	2147	rVV	658335	919649	21.59%	1.966%
40	15.757	2150	2154	2158	rVV4	10088	16300	0.38%	0.035%
41	16.251	2233	2238	2242	rBV5	9118	13418	0.32%	0.029%
42	16.304	2244	2247	2252	rVB4	8916	10326	0.24%	0.022%
43	17.045	2370	2373	2378	rBV5	8914	14305	0.34%	0.031%
44	17.275	2406	2412	2419	rBV	1231062	1722034	40.43%	3.682%
45	17.375	2422	2429	2442	rBV2	2756751	3965068	93.10%	8.478%
46	17.575	2458	2463	2468	rVB	27876	36433	0.86%	0.078%
47	17.786	2495	2499	2503	rBV5	8613	13795	0.32%	0.029%
48	17.963	2526	2529	2534	rVB6	3914	6403	0.15%	0.014%
49	18.186	2563	2567	2573	rBV6	9656	17239	0.40%	0.037%
50	18.257	2577	2579	2584	rVB3	7226	9377	0.22%	0.020%
51	18.486	2614	2618	2623	rVB8	5505	7610	0.18%	0.016%
52	19.239	2741	2746	2750	rVB3	29635	43658	1.03%	0.093%
53	19.304	2750	2757	2766	rBV	28642	52212	1.23%	0.112%
54	19.474	2782	2786	2789	rBV6	8517	13488	0.32%	0.029%
55	19.622	2809	2811	2813	rBV2	5443	5053	0.12%	0.011%
56	19.674	2813	2820	2828	rVV	3007440	4159703	97.67%	8.894%
57	21.468	3120	3125	3140	rBV	1093064	1560018	36.63%	3.336%
58	23.692	3495	3503	3513	rBV2	2125256	4259100	100.00%	9.107%
59	23.845	3522	3529	3539	rVB	891212	1768163	41.51%	3.781%




Sum of corrected areas: 46768610

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029626.D
Acq On : 10 Feb 2024 00:45
Operator : MA/JU
Sample : P1398-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

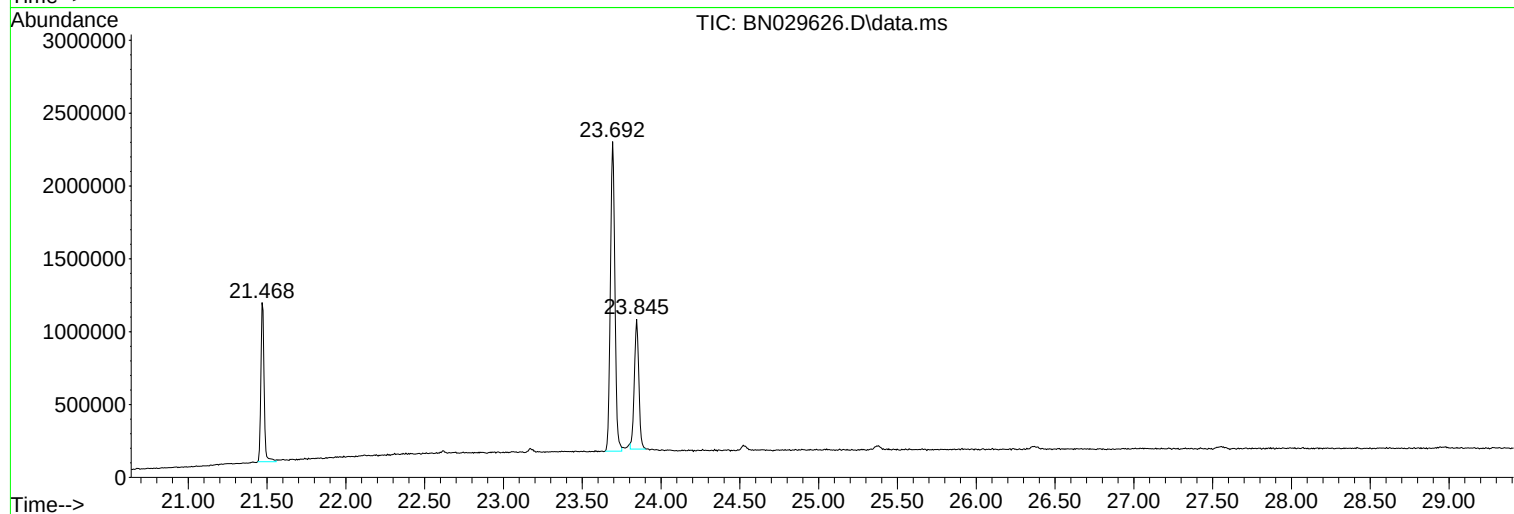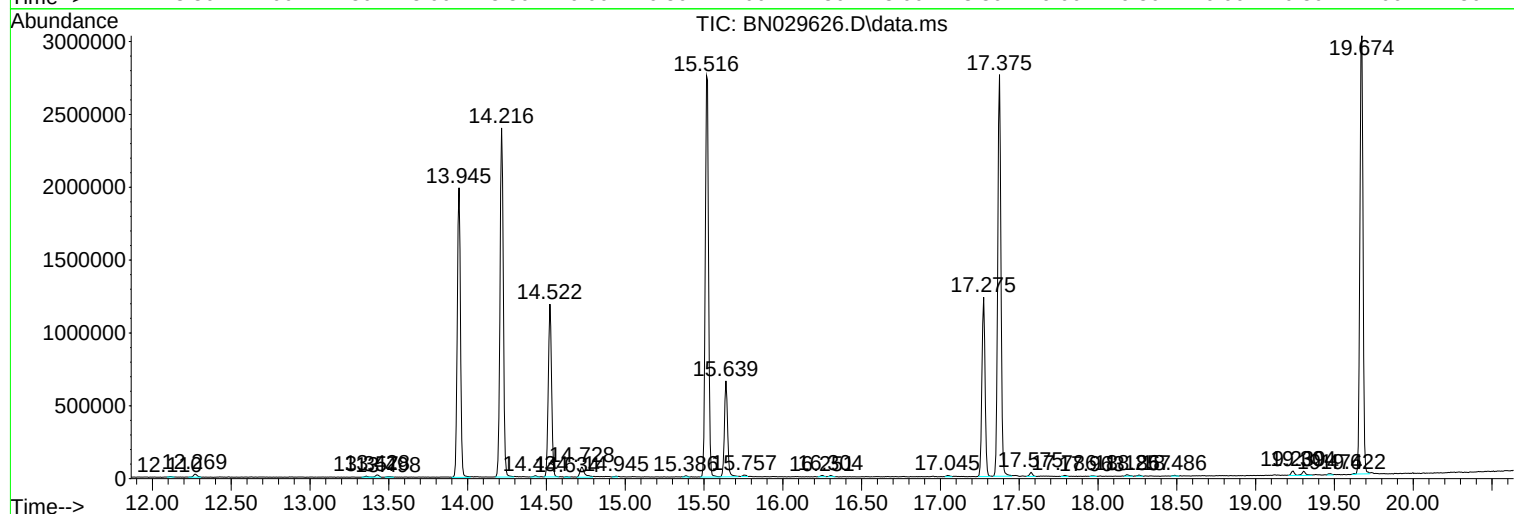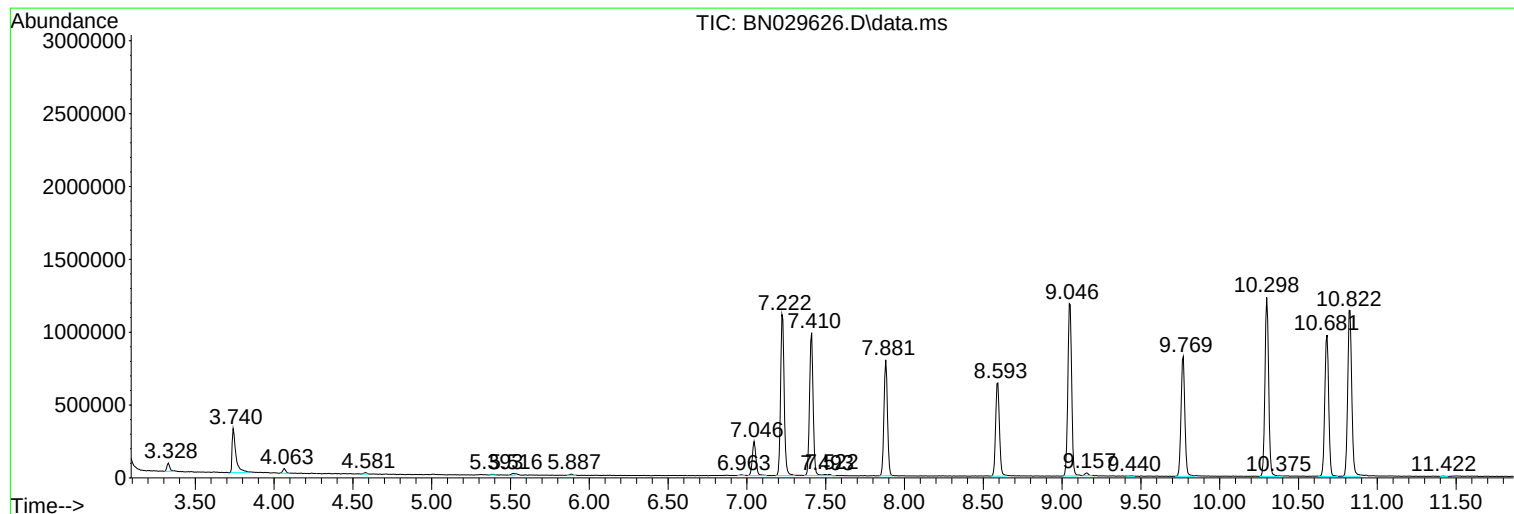

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029626.D
Acq On : 10 Feb 2024 00:45
Operator : MA/JU
Sample : P1398-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029626.D
Acq On : 10 Feb 2024 00:45
Operator : MA/JU
Sample : P1398-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc