

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029627.D
 Acq On : 10 Feb 2024 01:21
 Operator : MA/JU
 Sample : P1398-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	48	rVB	54286	68885	1.74%	0.159%
2	3.740	108	111	130	rBV	219402	373165	9.41%	0.859%
3	4.063	162	166	176	rVB	30413	44218	1.12%	0.102%
4	5.393	387	392	395	rVB5	5110	8832	0.22%	0.020%
5	5.516	409	413	416	rBV4	5821	9676	0.24%	0.022%
6	5.640	430	434	440	rVB6	2762	5165	0.13%	0.012%
7	5.887	474	476	481	rVB5	4983	5728	0.14%	0.013%
8	7.046	667	673	681	rBV	212112	331291	8.35%	0.763%
9	7.222	697	703	720	rBV	888379	1411941	35.61%	3.251%
10	7.410	728	735	745	rBV	798305	1274086	32.13%	2.933%
11	7.499	745	750	758	rVB10	6024	16292	0.41%	0.038%
12	7.881	808	815	823	rVB	849503	1306931	32.96%	3.009%
13	8.587	929	935	950	rBV	552235	911216	22.98%	2.098%
14	8.716	954	957	961	rVB5	3201	4444	0.11%	0.010%
15	9.046	1006	1013	1027	rBV	925315	1573193	39.67%	3.622%
16	9.157	1027	1032	1039	rBV	40340	70339	1.77%	0.162%
17	9.440	1077	1080	1084	rVB5	3147	4084	0.10%	0.009%
18	9.769	1126	1136	1148	rBV	636654	1088412	27.45%	2.506%
19	10.240	1211	1216	1219	rBV6	1811	3989	0.10%	0.009%
20	10.298	1219	1226	1242	rVV	969047	1618822	40.82%	3.727%
21	10.681	1282	1291	1299	rBV	1024838	1736132	43.78%	3.997%
22	10.828	1308	1316	1331	rBV	875895	1547372	39.02%	3.563%
23	11.451	1418	1422	1425	rBV5	3151	5055	0.13%	0.012%
24	11.504	1425	1431	1437	rVB10	5551	13279	0.33%	0.031%
25	12.275	1552	1562	1567	rBV	18211	29380	0.74%	0.068%
26	13.363	1744	1747	1751	rBV4	2548	4088	0.10%	0.009%
27	13.428	1751	1758	1764	rVV3	17429	27256	0.69%	0.063%
28	13.945	1838	1846	1859	rBV	1686742	2270689	57.26%	5.228%
29	14.216	1882	1892	1902	rBV2	1888063	2802830	70.68%	6.453%
30	14.522	1937	1944	1953	rBV	1242349	1823011	45.97%	4.197%
31	14.751	1973	1983	1995	rBV2	749912	1725819	43.52%	3.974%
32	15.522	2107	2114	2127	rBV	2263368	3388280	85.44%	7.801%
33	15.639	2127	2134	2145	rBV	602500	838980	21.16%	1.932%
34	15.757	2150	2154	2160	rVB3	11809	17441	0.44%	0.040%
35	16.086	2205	2210	2214	rBV7	3222	4591	0.12%	0.011%
36	16.304	2243	2247	2251	rBV7	7086	10451	0.26%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029627.D
 Acq On : 10 Feb 2024 01:21
 Operator : MA/JU
 Sample : P1398-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	16.951	2355	2357	2363	rVB7	4837	7363	0.19%	0.017%
38	17.275	2405	2412	2422	rBV	1336322	1846522	46.57%	4.251%
39	17.375	2422	2429	2447	rVV	2544108	3578546	90.24%	8.239%
40	17.675	2476	2480	2482	rBV5	3944	5171	0.13%	0.012%
41	17.969	2525	2530	2533	rVB4	7673	11437	0.29%	0.026%
42	18.186	2562	2567	2573	rBV3	30952	47051	1.19%	0.108%
43	18.657	2646	2647	2654	rVB7	3407	5924	0.15%	0.014%
44	19.051	2710	2714	2717	rBV4	4447	6061	0.15%	0.014%
45	19.145	2726	2730	2733	rVB6	13987	16922	0.43%	0.039%
46	19.239	2741	2746	2750	rBV3	25777	38534	0.97%	0.089%
47	19.274	2750	2752	2753	rBV2	5745	4425	0.11%	0.010%
48	19.304	2754	2757	2762	rVB	24010	31232	0.79%	0.072%
49	19.469	2781	2785	2791	rBV7	20902	31200	0.79%	0.072%
50	19.674	2814	2820	2829	rBV	2831722	3839309	96.82%	8.840%
51	21.198	3077	3079	3084	rBV5	16170	23288	0.59%	0.054%
52	21.468	3120	3125	3132	rBV	1272869	1687524	42.56%	3.885%
53	23.692	3495	3503	3515	rBV2	1933699	3965454	100.00%	9.130%
54	23.845	3522	3529	3541	rVB2	929454	1911809	48.21%	4.402%




Sum of corrected areas: 43433135

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029627.D
Acq On : 10 Feb 2024 01:21
Operator : MA/JU
Sample : P1398-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

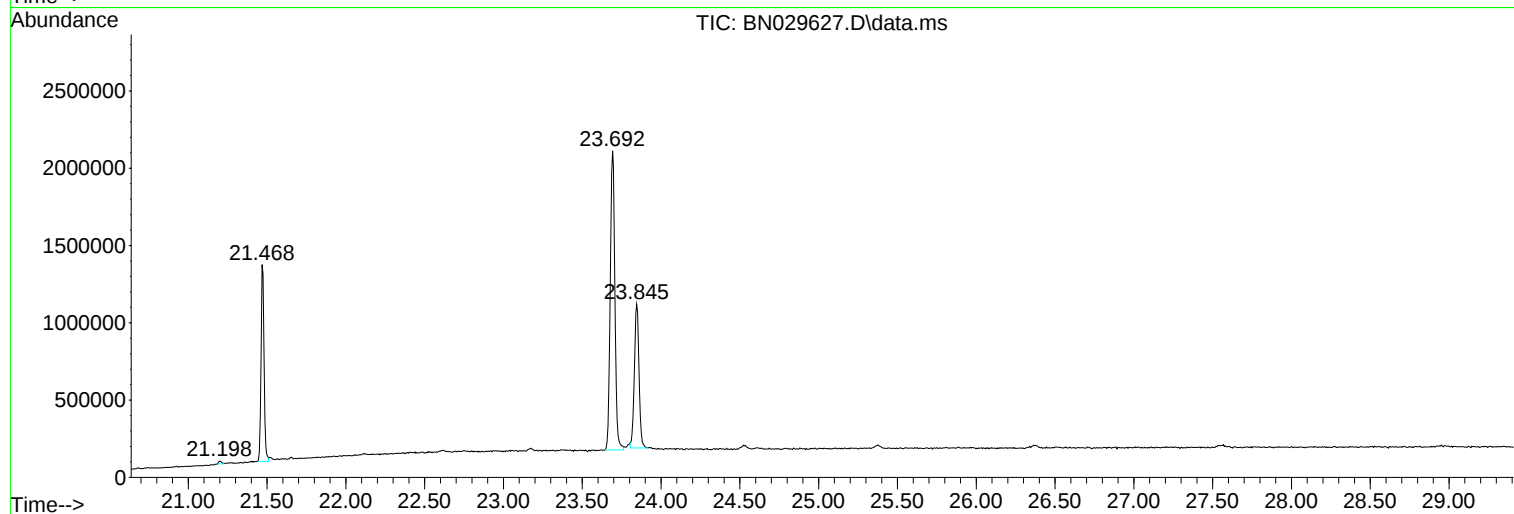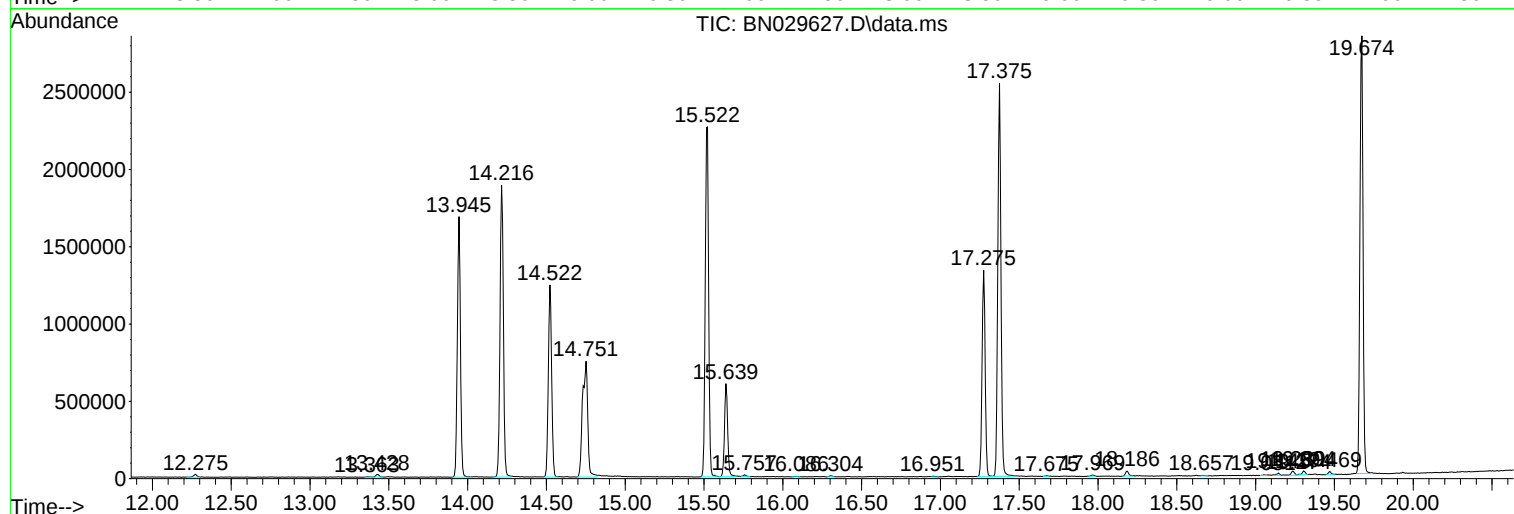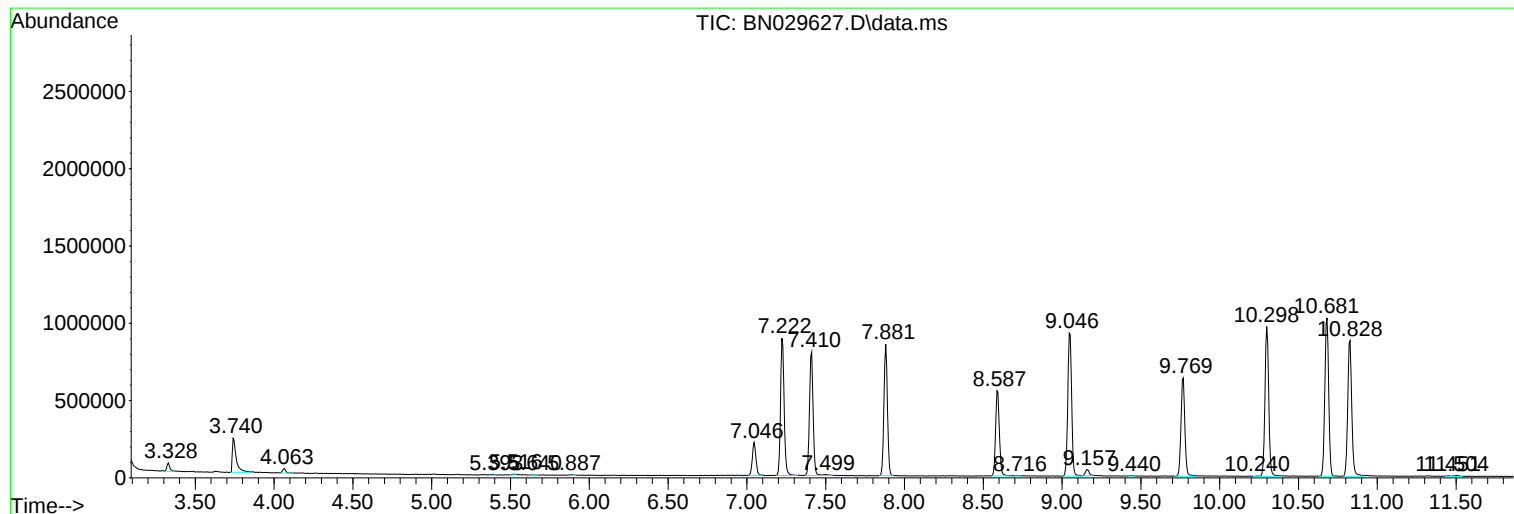

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029627.D
Acq On : 10 Feb 2024 01:21
Operator : MA/JU
Sample : P1398-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029627.D
Acq On : 10 Feb 2024 01:21
Operator : MA/JU
Sample : P1398-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc