

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029628.D
 Acq On : 10 Feb 2024 01:57
 Operator : MA/JU
 Sample : P1398-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	52	rVB	62294	92015	2.10%	0.203%
2	3.740	108	111	132	rBV	227078	402568	9.20%	0.887%
3	4.064	162	166	172	rVB	33535	46353	1.06%	0.102%
4	4.587	250	255	260	rVB2	66835	99764	2.28%	0.220%
5	5.310	375	378	383	rVB4	8021	11978	0.27%	0.026%
6	5.387	388	391	397	rVB3	8628	12245	0.28%	0.027%
7	5.516	408	413	422	rBV3	19544	45368	1.04%	0.100%
8	5.887	470	476	481	rBV	11908	18565	0.42%	0.041%
9	6.852	637	640	644	rBV5	3372	6382	0.15%	0.014%
10	6.963	655	659	664	rVB2	10719	17777	0.41%	0.039%
11	7.046	664	673	680	rBV	244647	390122	8.92%	0.860%
12	7.222	696	703	718	rBV	972838	1579013	36.10%	3.480%
13	7.410	727	735	743	rBV	917715	1452117	33.20%	3.200%
14	7.499	747	750	751	rVV3	8398	10374	0.24%	0.023%
15	7.528	751	755	759	rVB2	12985	21419	0.49%	0.047%
16	7.881	807	815	827	rBV	858750	1343293	30.71%	2.960%
17	8.587	928	935	948	rBV	634825	1050015	24.01%	2.314%
18	9.051	1006	1014	1028	rBV	1050232	1770957	40.49%	3.903%
19	9.769	1128	1136	1146	rBV	719547	1211005	27.69%	2.669%
20	10.298	1219	1226	1237	rBV	1118219	1834530	41.95%	4.043%
21	10.681	1283	1291	1301	rVB	1046784	1758174	40.20%	3.874%
22	10.828	1307	1316	1330	rBV	955989	1681772	38.45%	3.706%
23	12.269	1557	1561	1567	rBV3	16771	29491	0.67%	0.065%
24	13.428	1752	1758	1763	rBV2	15410	23978	0.55%	0.053%
25	13.945	1839	1846	1859	rBV	1922112	2618274	59.87%	5.770%
26	14.216	1883	1892	1908	rBV	2113300	3091485	70.69%	6.813%
27	14.522	1937	1944	1952	rBV	1227941	1825891	41.75%	4.024%
28	14.722	1971	1978	1997	rBV	83969	184020	4.21%	0.406%
29	15.475	2102	2106	2107	rBV4	4359	5281	0.12%	0.012%
30	15.516	2107	2113	2126	rVB	2551288	3725363	85.18%	8.209%
31	15.639	2128	2134	2143	rBV	673283	924042	21.13%	2.036%
32	15.757	2150	2154	2159	rVB4	11000	17574	0.40%	0.039%
33	16.304	2240	2247	2251	rVB8	7680	12181	0.28%	0.027%
34	17.275	2405	2412	2418	rBV	1294395	1823100	41.68%	4.017%
35	17.375	2421	2429	2441	rBV2	2737455	3923106	89.70%	8.645%
36	17.575	2459	2463	2466	rVB6	3524	5408	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029628.D
Acq On : 10 Feb 2024 01:57
Operator : MA/JU
Sample : P1398-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	18.180	2562	2566	2572	rBV5	21395	33454	0.76%	0.074%
38	18.857	2677	2681	2684	rBV4	2626	4495	0.10%	0.010%
39	19.239	2741	2746	2752	rVB3	28282	41887	0.96%	0.092%
40	19.304	2752	2757	2763	rBV2	26514	42720	0.98%	0.094%
41	19.469	2782	2785	2788	rBV3	19686	22047	0.50%	0.049%
42	19.622	2808	2811	2813	rBV4	6636	8315	0.19%	0.018%
43	19.674	2813	2820	2828	rVV	2999832	4180456	95.58%	9.212%
44	21.468	3120	3125	3138	rBV2	1240934	1697997	38.82%	3.742%
45	23.692	3495	3503	3517	rBV2	2181045	4373576	100.00%	9.638%
46	23.845	3522	3529	3542	rVB	944637	1909644	43.66%	4.208%




Sum of corrected areas: 45379591

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029628.D
Acq On : 10 Feb 2024 01:57
Operator : MA/JU
Sample : P1398-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

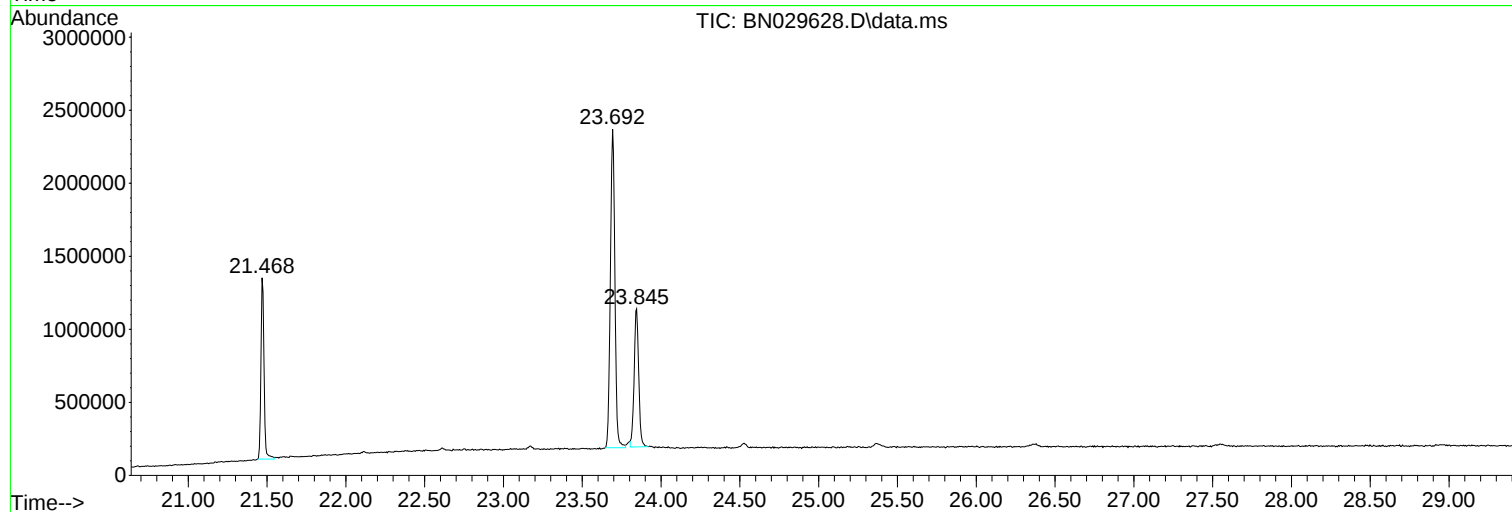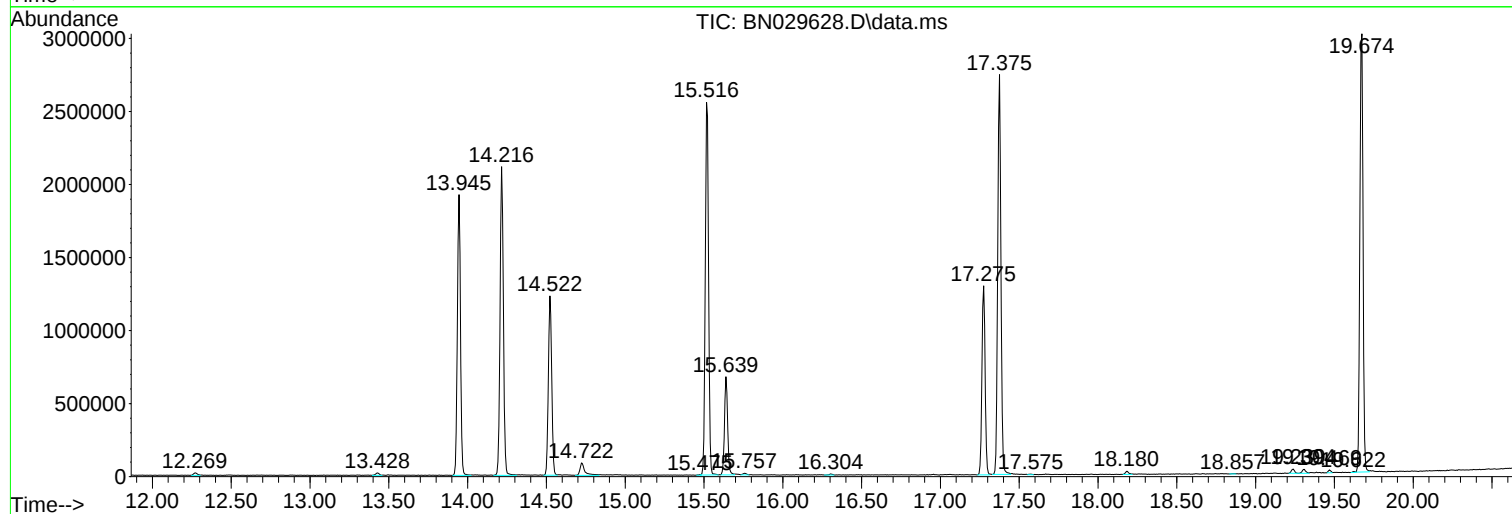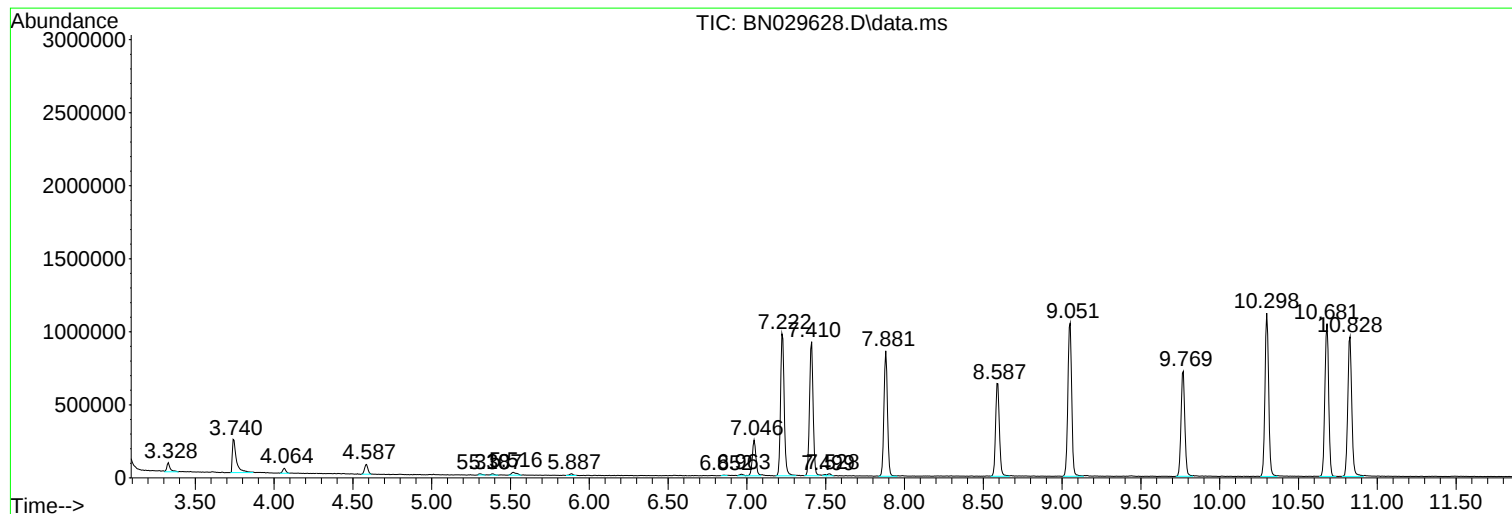

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029628.D
Acq On : 10 Feb 2024 01:57
Operator : MA/JU
Sample : P1398-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029628.D
Acq On : 10 Feb 2024 01:57
Operator : MA/JU
Sample : P1398-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------