

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029631.D
 Acq On : 10 Feb 2024 04:21
 Operator : MA/JU
 Sample : PB158923BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK923

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	47	rBV	83421	108129	3.44%	0.249%
2	3.734	107	110	133	rBV	913974	1419691	45.13%	3.265%
3	4.063	163	166	172	rVB	21751	27437	0.87%	0.063%
4	7.045	666	673	688	rBV	1083998	1677844	53.33%	3.858%
5	7.222	697	703	715	rVB	861396	1363929	43.35%	3.137%
6	7.410	727	735	746	rBV	1071894	1701614	54.09%	3.913%
7	7.881	808	815	824	rBV	794200	1257884	39.98%	2.893%
8	8.087	846	850	854	rVV6	2034	4284	0.14%	0.010%
9	8.592	928	936	945	rBV	1177206	1923062	61.13%	4.422%
10	9.045	1005	1013	1022	rBV	927935	1543529	49.06%	3.550%
11	9.769	1127	1136	1149	rBV	666225	1116331	35.48%	2.567%
12	10.298	1215	1226	1237	rBV	1073054	1787701	56.82%	4.111%
13	10.681	1283	1291	1303	rVB	996554	1692606	53.80%	3.892%
14	10.828	1306	1316	1330	rBV	1067076	1892205	60.15%	4.351%
15	12.269	1555	1561	1568	rBV3	14699	27385	0.87%	0.063%
16	12.892	1661	1667	1669	rVB6	1709	3149	0.10%	0.007%
17	13.427	1752	1758	1763	rBV3	17176	27983	0.89%	0.064%
18	13.945	1839	1846	1858	rBV	1563998	2162009	68.72%	4.972%
19	14.216	1884	1892	1906	rVV	1888538	2724799	86.61%	6.266%
20	14.521	1935	1944	1952	rBV	1216781	1778116	56.52%	4.089%
21	14.721	1972	1978	1995	rBV	542601	891558	28.34%	2.050%
22	15.516	2107	2113	2124	rBV	2120124	3116382	99.06%	7.167%
23	15.639	2128	2134	2146	rVV	502332	703422	22.36%	1.618%
24	15.757	2148	2154	2159	rVB5	10587	14649	0.47%	0.034%
25	16.063	2202	2206	2209	rBV5	2225	3559	0.11%	0.008%
26	16.304	2241	2247	2252	rBV6	6669	11534	0.37%	0.027%
27	17.274	2405	2412	2422	rBV	1266876	1755545	55.80%	4.037%
28	17.374	2422	2429	2442	rBV2	2139275	3025181	96.16%	6.957%
29	18.186	2564	2567	2572	rVB7	3679	5499	0.17%	0.013%
30	18.780	2665	2668	2671	rBV4	2176	3291	0.10%	0.008%
31	19.233	2741	2745	2752	rVB3	22315	35904	1.14%	0.083%
32	19.309	2752	2758	2764	rBV	19275	35363	1.12%	0.081%
33	19.674	2813	2820	2828	rBV	2284929	3146051	100.00%	7.235%
34	21.468	3120	3125	3137	rBV2	1179684	1611010	51.21%	3.705%
35	23.692	3496	3503	3514	rBV	1587676	3137793	99.74%	7.216%
36	23.845	3523	3529	3538	rVB	880061	1748630	55.58%	4.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029631.D
Acq On : 10 Feb 2024 04:21
Operator : MA/JU
Sample : PB158923BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK923

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 43485058

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029631.D
Acq On : 10 Feb 2024 04:21
Operator : MA/JU
Sample : PB158923BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK923

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

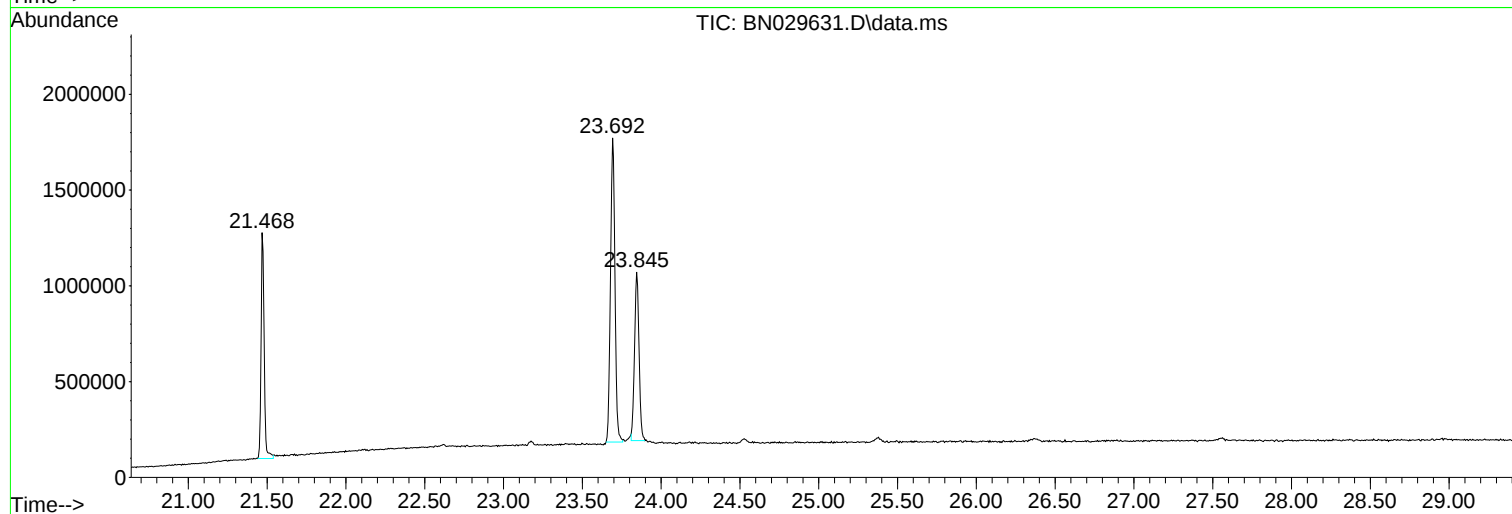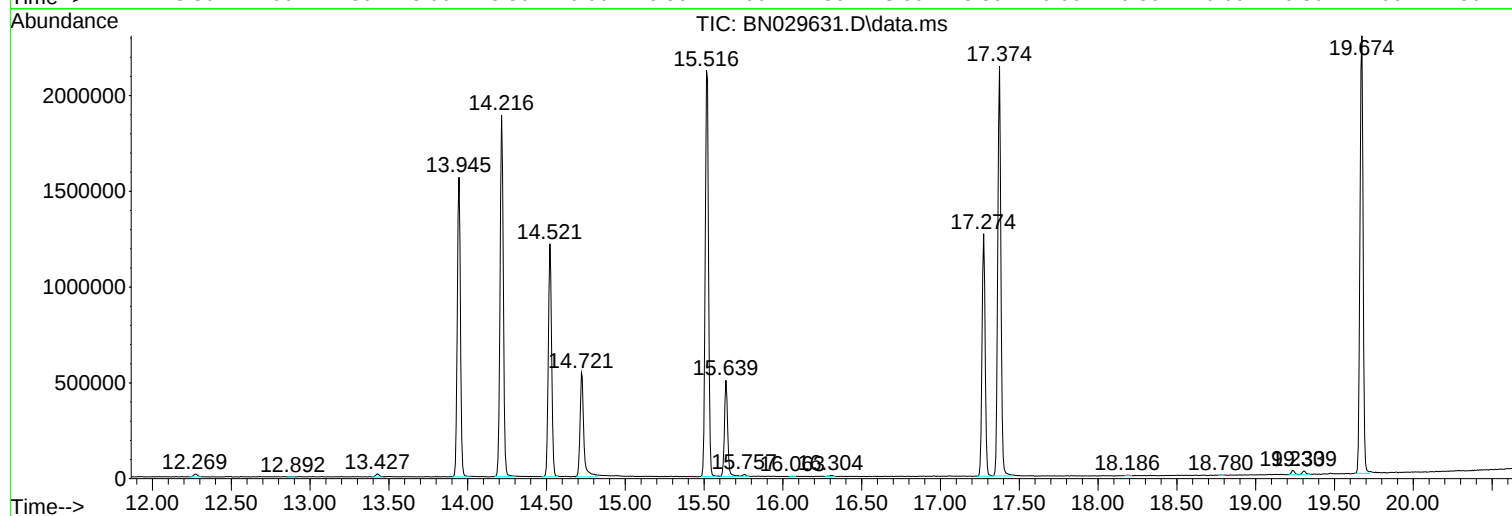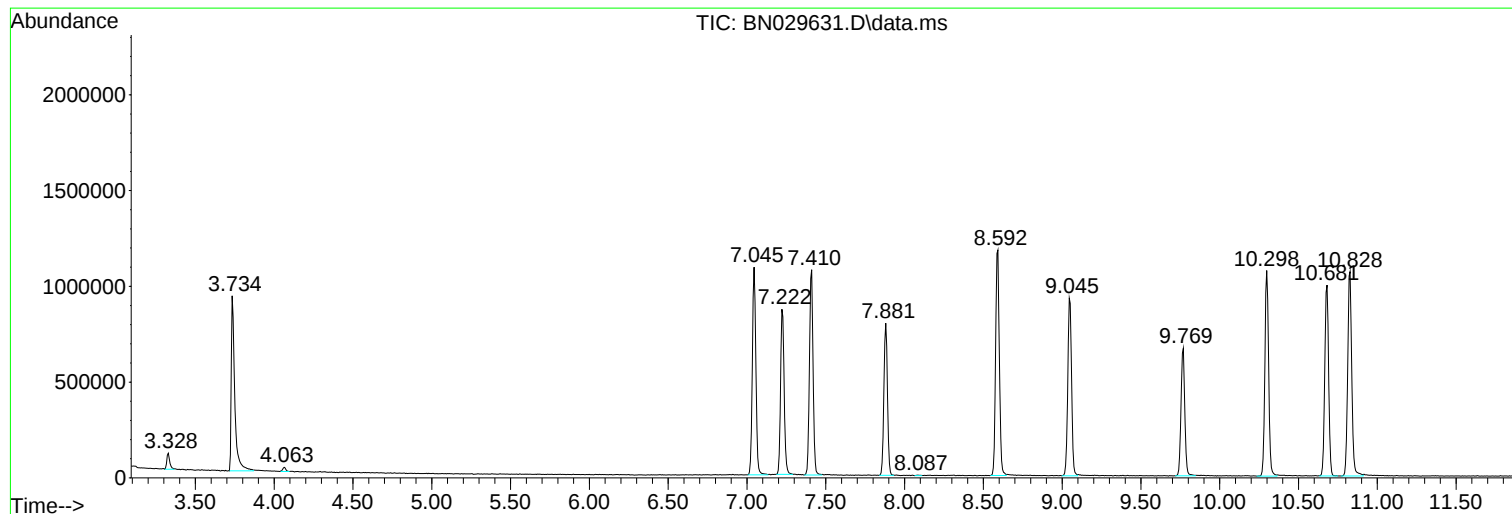

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029631.D
Acq On : 10 Feb 2024 04:21
Operator : MA/JU
Sample : PB158923BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK923

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029631.D
Acq On : 10 Feb 2024 04:21
Operator : MA/JU
Sample : PB158923BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK923

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------